

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
 Data File : BM004830.D
 Acq On : 29 Mar 2016 21:03
 Operator : UM/SJ
 Sample : H1939-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9SG7

Quant Time: Mar 30 03:45:17 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 30 03:41:15 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	48097	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	239613	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.46	164	154125	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.20	188	369075	20.00	ng/ul	0.00
78) Chrysene-d12	21.39	240	460050	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	437067	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	4921	3.53	ng/uL	0.00
5) Phenol-d5	6.99	99	111691	28.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	68245	30.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	87306	27.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	96292	30.23	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	44512	26.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	48681	27.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	90927	25.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	123967	29.34	ng/ul	0.00
44) Dimethylphthalate-d6	13.87	166	330035	27.39	ng/ul	0.00
47) Acenaphthylene-d8	14.15	160	397125	26.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.65	143	51378	22.06	ng/ul	0.00
58) Fluorene-d10	15.46	176	290664	27.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.57	200	42984	22.16	ng/ul	0.00
71) Anthracene-d10	17.30	188	460568	27.10	ng/ul	0.00
79) Pyrene-d10	19.60	212	553196	26.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	593728	30.41	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.92	163	116486	9.52	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
Data File : BM004830.D
Acq On : 29 Mar 2016 21:03
Operator : UM/SJ
Sample : H1939-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9SG7

Quant Time: Mar 30 03:45:17 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 30 03:41:15 2016
Response via : Initial Calibration

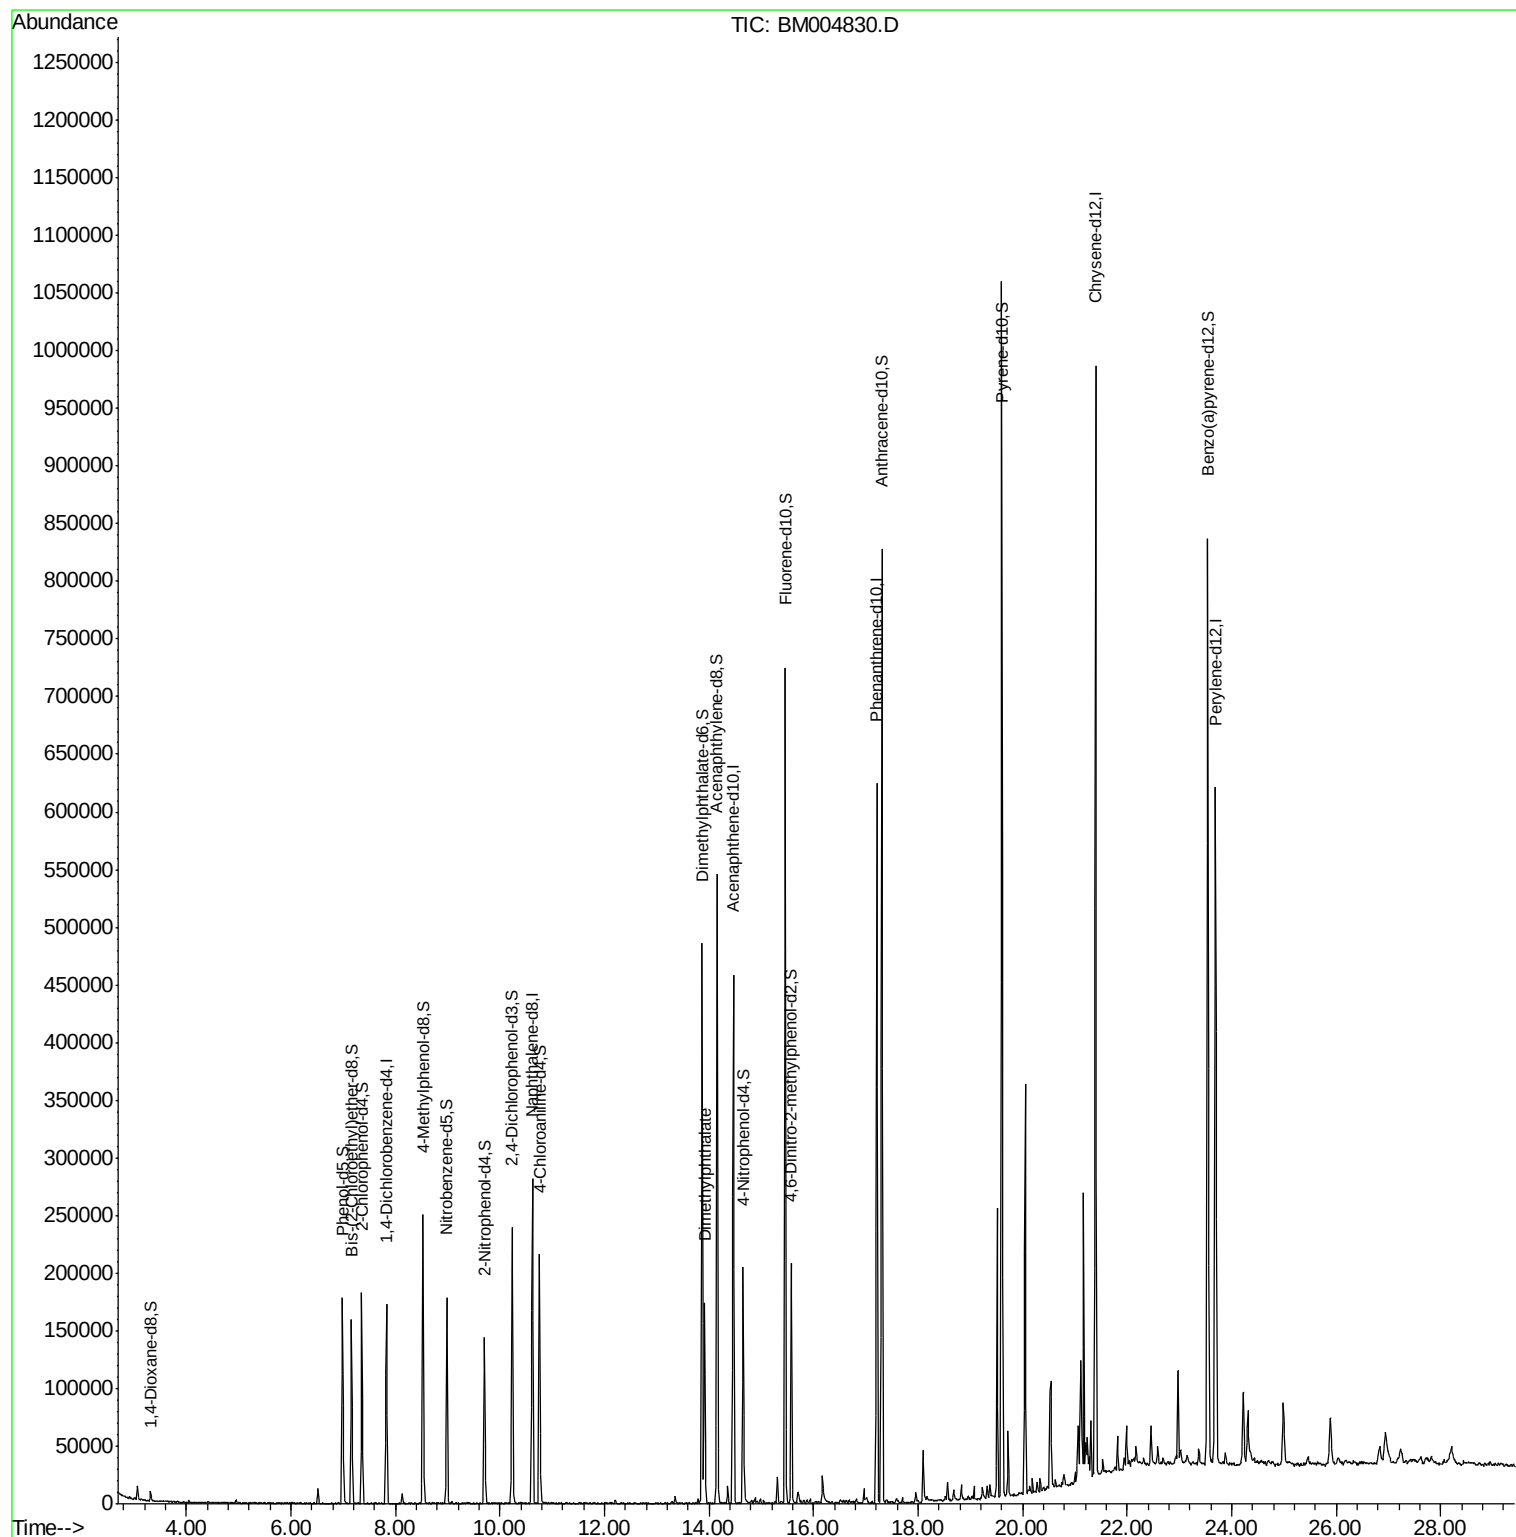

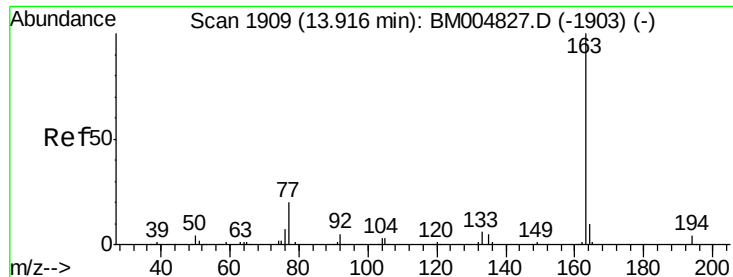

#45

Dimethylphthalate

Concen: 9.52 ng/ul

RT: 13.92 min Scan# 1909

Delta R.T. -0.00 min

Lab File: BM004830.D


Acq: 29 Mar 2016 21:03

Instrument :

BNA_M

ClientSampleId :

D9SG7

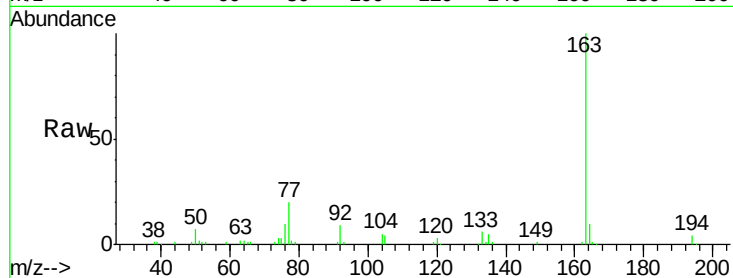

Tgt Ion:	163	Resp:	116486
Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.2	4.8
164	10.1	7.8	11.8

