

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
 Data File : BM004839.D
 Acq On : 30 Mar 2016 02:27
 Operator : UM/SJ
 Sample : H1939-24
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9SH6

Quant Time: Mar 30 03:46:05 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 30 03:41:15 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	64288	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	311196	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.46	164	194929	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.21	188	444240	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	441946	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	396042	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	3343	1.79	ng/uL	0.00
5) Phenol-d5	6.99	99	89167	16.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	50478	16.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	71200	16.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	70645	16.59	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	35548	16.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	40590	17.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	77771	16.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	54677	9.96	ng/ul	0.00
44) Dimethylphthalate-d6	13.87	166	251459	16.50	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	318129	17.03	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	39464	13.40	ng/ul	0.00
58) Fluorene-d10	15.46	176	231767	17.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.57	200	32338	13.85	ng/ul	0.00
71) Anthracene-d10	17.30	188	348779	17.05	ng/ul	0.00
79) Pyrene-d10	19.60	212	383859	19.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.55	264	344033	19.45	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.92	163	94781	6.13	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
Data File : BM004839.D
Acq On : 30 Mar 2016 02:27
Operator : UM/SJ
Sample : H1939-24
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9SH6

Quant Time: Mar 30 03:46:05 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 30 03:41:15 2016
Response via : Initial Calibration

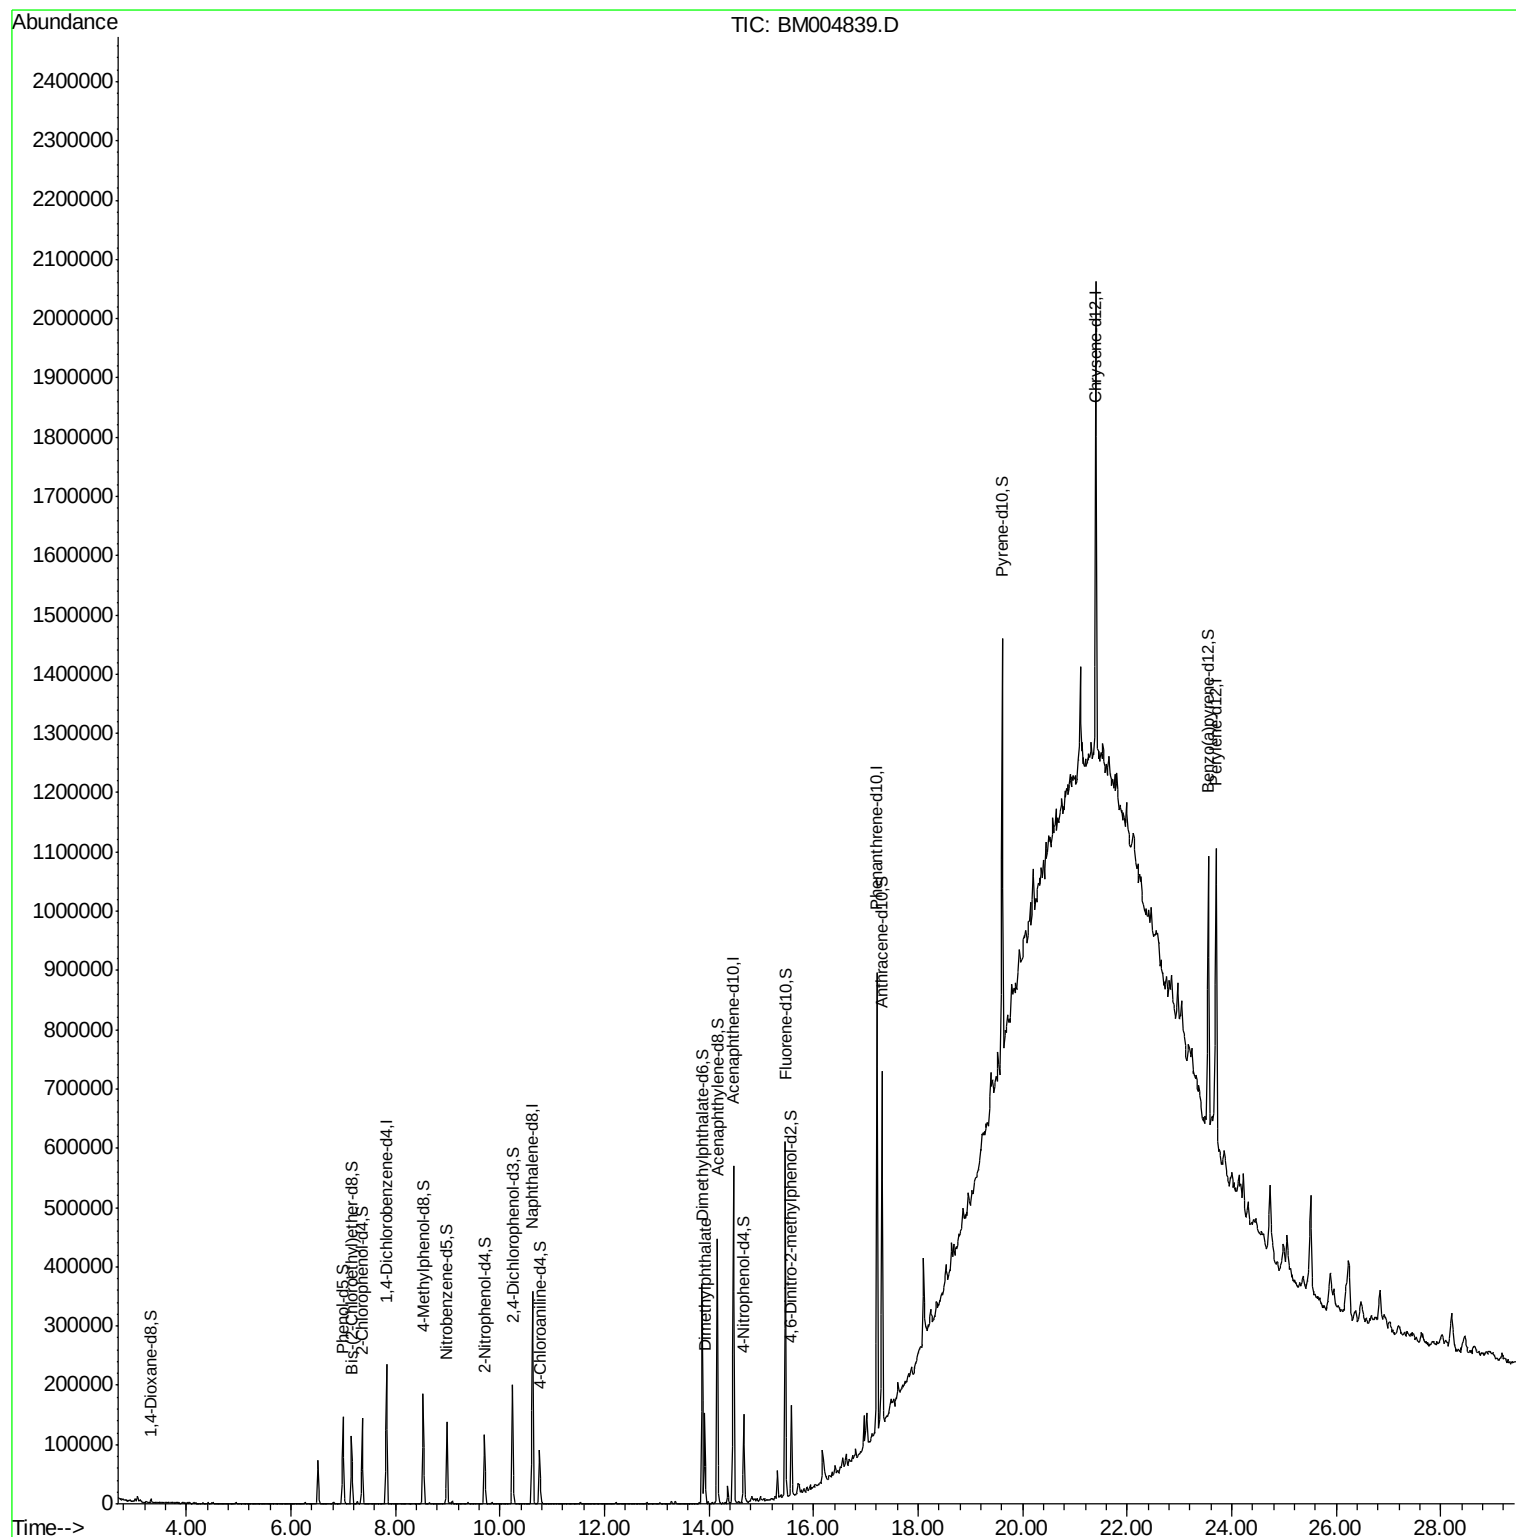

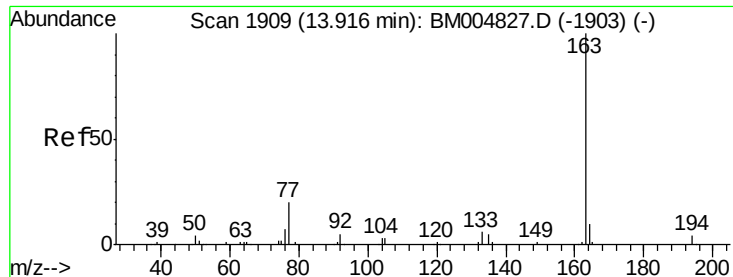

#45

Dimethylphthalate

Concen: 6.13 ng/ul

RT: 13.92 min Scan# 1909

Delta R.T. -0.00 min

Lab File: BM004839.D

Acq: 30 Mar 2016 02:27

Instrument :

BNA_M

ClientSampleId :

D9SH6


Tgt Ion:163 Resp: 94781

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.2 7.8 11.8

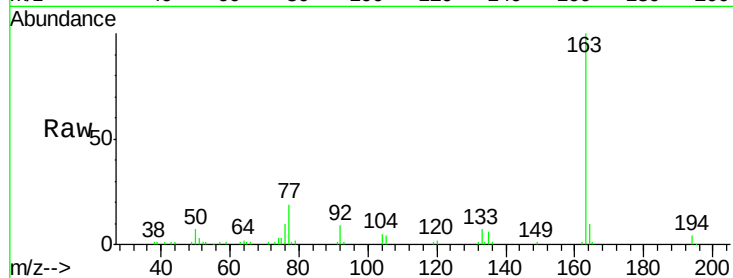

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

