

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
 Data File : BM004829.D
 Acq On : 29 Mar 2016 20:27
 Operator : UM/SJ
 Sample : H1939-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9SG6

Quant Time: Mar 30 03:45:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 30 03:41:15 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	52092	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	260957	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.46	164	164899	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.20	188	393476	20.00	ng/ul	0.00
78) Chrysene-d12	21.39	240	484510	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	450509	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	6113	4.05	ng/uL	0.00
5) Phenol-d5	6.99	99	138900	32.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	85592	35.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	110965	32.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	120416	34.90	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	56098	30.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	61641	31.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	116075	30.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	159729	34.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.87	166	406248	31.51	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	490304	31.02	ng/ul	0.00
52) 4-Nitrophenol-d4	14.65	143	67088	26.92	ng/ul	0.00
58) Fluorene-d10	15.46	176	358530	31.91	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.57	200	55492	26.83	ng/ul	0.00
71) Anthracene-d10	17.30	188	565773	31.23	ng/ul	0.00
79) Pyrene-d10	19.60	212	680287	30.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	728738	36.22	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.92	163	148452	11.34	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
Data File : BM004829.D
Acq On : 29 Mar 2016 20:27
Operator : UM/SJ
Sample : H1939-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9SG6

Quant Time: Mar 30 03:45:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 30 03:41:15 2016
Response via : Initial Calibration

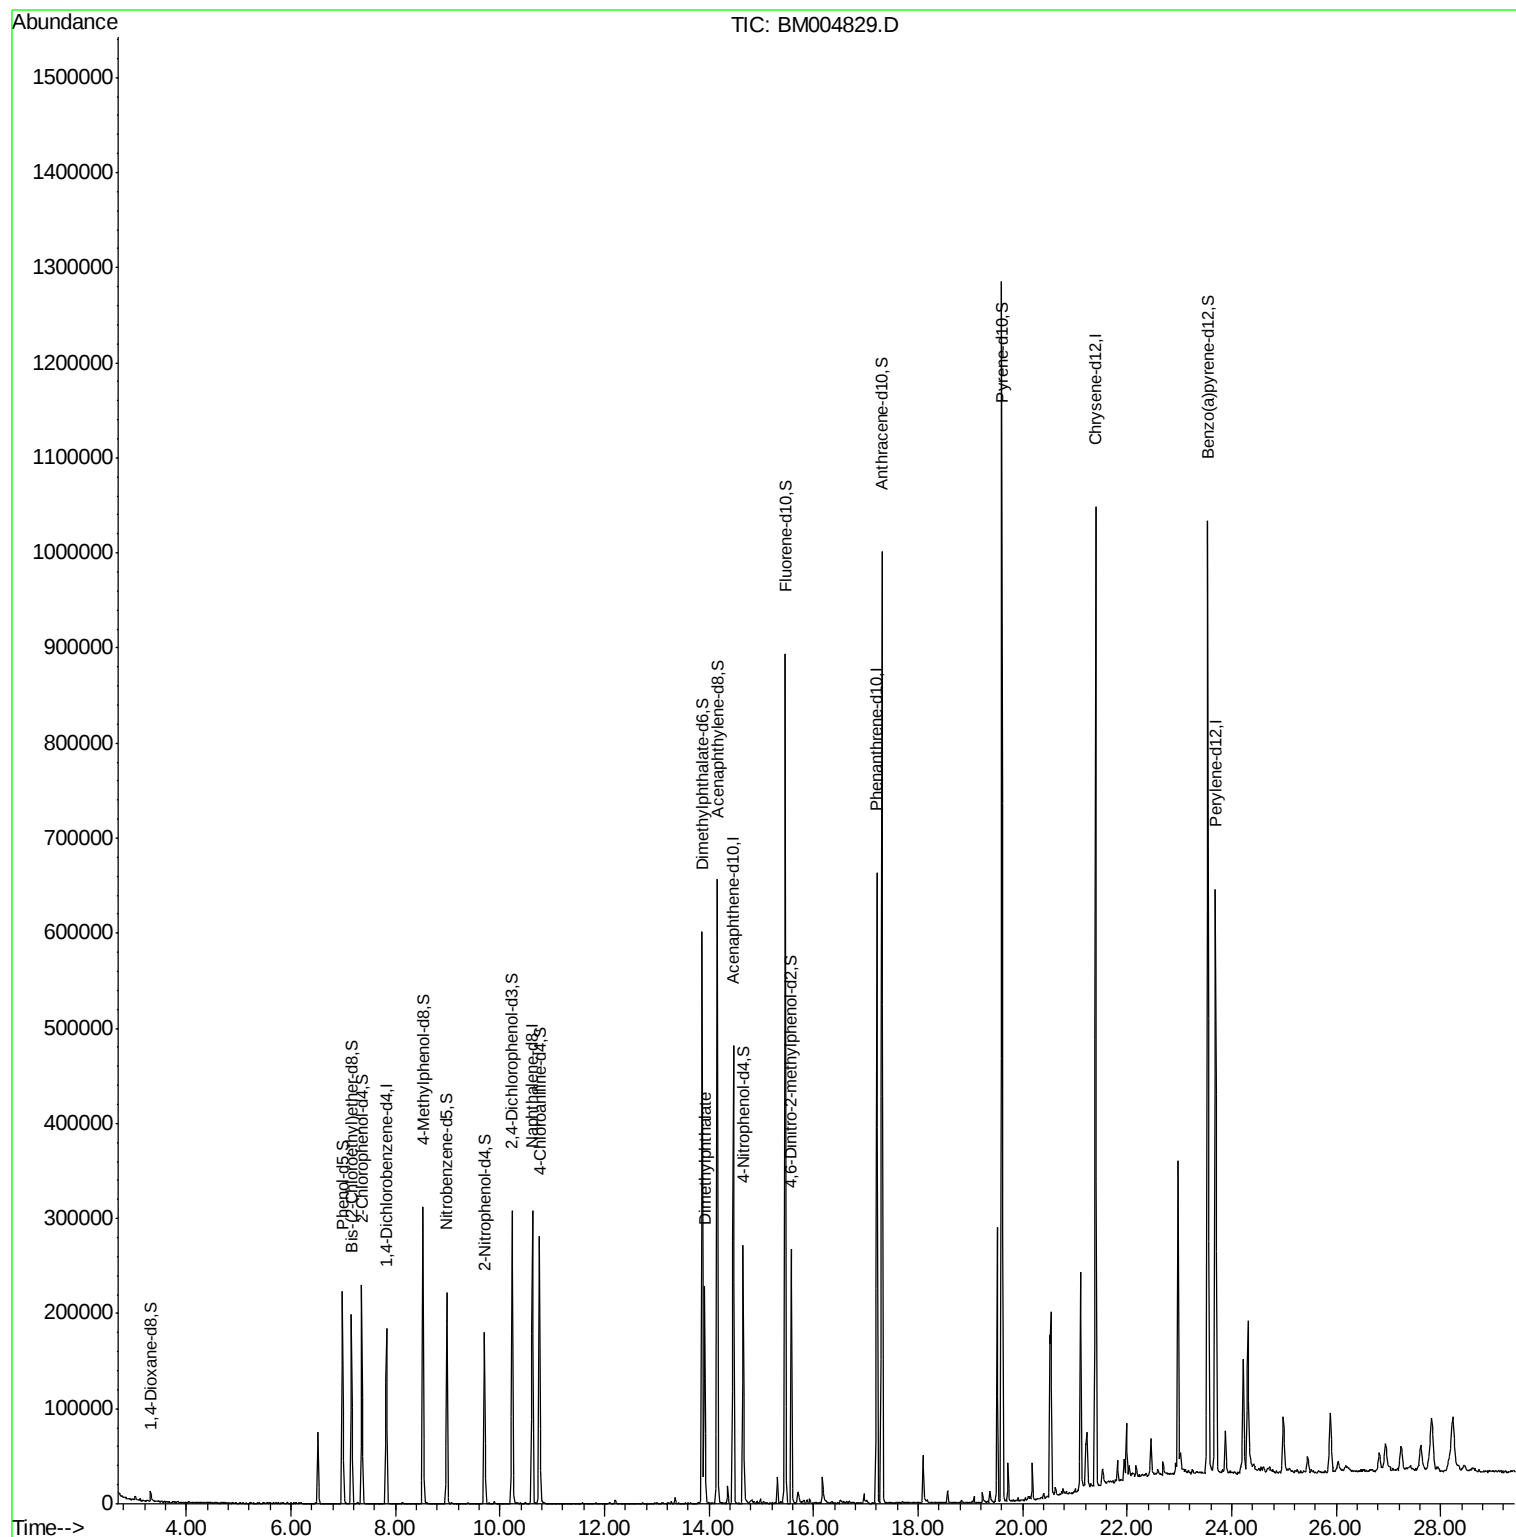

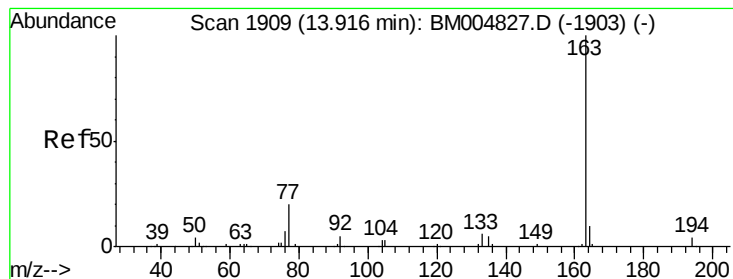

#45

Dimethylphthalate

Concen: 11.34 ng/ul

RT: 13.92 min Scan# 1909

Delta R.T. -0.00 min

Lab File: BM004829.D

Acq: 29 Mar 2016 20:27

Instrument :

BNA_M

ClientSampleId :

D9SG6


Tgt Ion:163 Resp: 148452

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 9.8 7.8 11.8

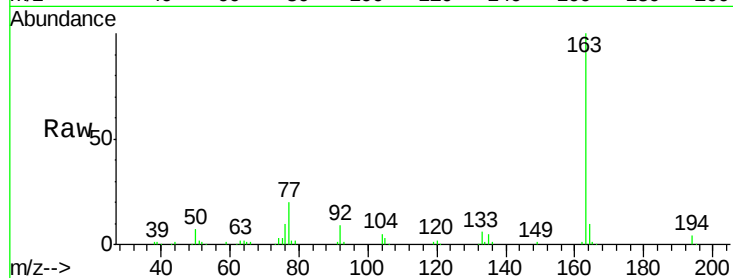

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

