

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
 Data File : BM004816.D
 Acq On : 29 Mar 2016 12:09
 Operator : UM/SJ
 Sample : H1939-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9SF3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.987	726	731	743	rVB	51442	78892	4.46%	0.532%
2	7.157	753	760	771	rBV	178069	273124	15.45%	1.843%
3	7.357	786	794	802	rBV	175000	275146	15.57%	1.857%
4	7.828	868	874	881	rBV	180050	286205	16.19%	1.931%
5	8.522	986	992	1000	rBV	157235	244825	13.85%	1.652%
6	8.981	1064	1070	1079	rBV	201313	322578	18.25%	2.177%
7	9.698	1186	1192	1201	rBV	155906	258426	14.62%	1.744%
8	10.234	1276	1283	1297	rVB	252325	415383	23.50%	2.803%
9	10.616	1340	1348	1358	rVB	280992	477101	26.99%	3.219%
10	13.869	1895	1901	1913	rVB	571419	776238	43.91%	5.238%
11	14.157	1943	1950	1956	rBV	615131	930092	52.62%	6.276%
12	14.463	1995	2002	2018	rBV2	459300	721040	40.79%	4.865%
13	14.651	2029	2034	2047	rVB	47724	73480	4.16%	0.496%
14	15.457	2164	2171	2179	rVB	849350	1227759	69.46%	8.285%
15	15.569	2184	2190	2197	rBV	244422	326335	18.46%	2.202%
16	17.204	2462	2468	2475	rBV2	595245	878721	49.71%	5.929%
17	17.304	2479	2485	2496	rVV	965019	1364299	77.18%	9.206%
18	19.598	2869	2875	2885	rBV	1226008	1705002	96.46%	11.505%
19	21.392	3175	3180	3190	rVB	960518	1196849	67.71%	8.076%
20	22.456	3357	3361	3365	rBV3	13588	19501	1.10%	0.132%
21	22.974	3446	3449	3456	rVB	17563	24111	1.36%	0.163%
22	23.544	3538	3546	3559	rBV	907459	1767618	100.00%	11.927%
23	23.686	3563	3570	3583	rVB2	553162	1111101	62.86%	7.497%
24	24.221	3657	3661	3667	rVB3	17797	31551	1.78%	0.213%
25	24.991	3787	3792	3800	rVB3	16849	34373	1.94%	0.232%


Sum of corrected areas: 14819750

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
Data File : BM004816.D
Acq On : 29 Mar 2016 12:09
Operator : UM/SJ
Sample : H1939-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9SF3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

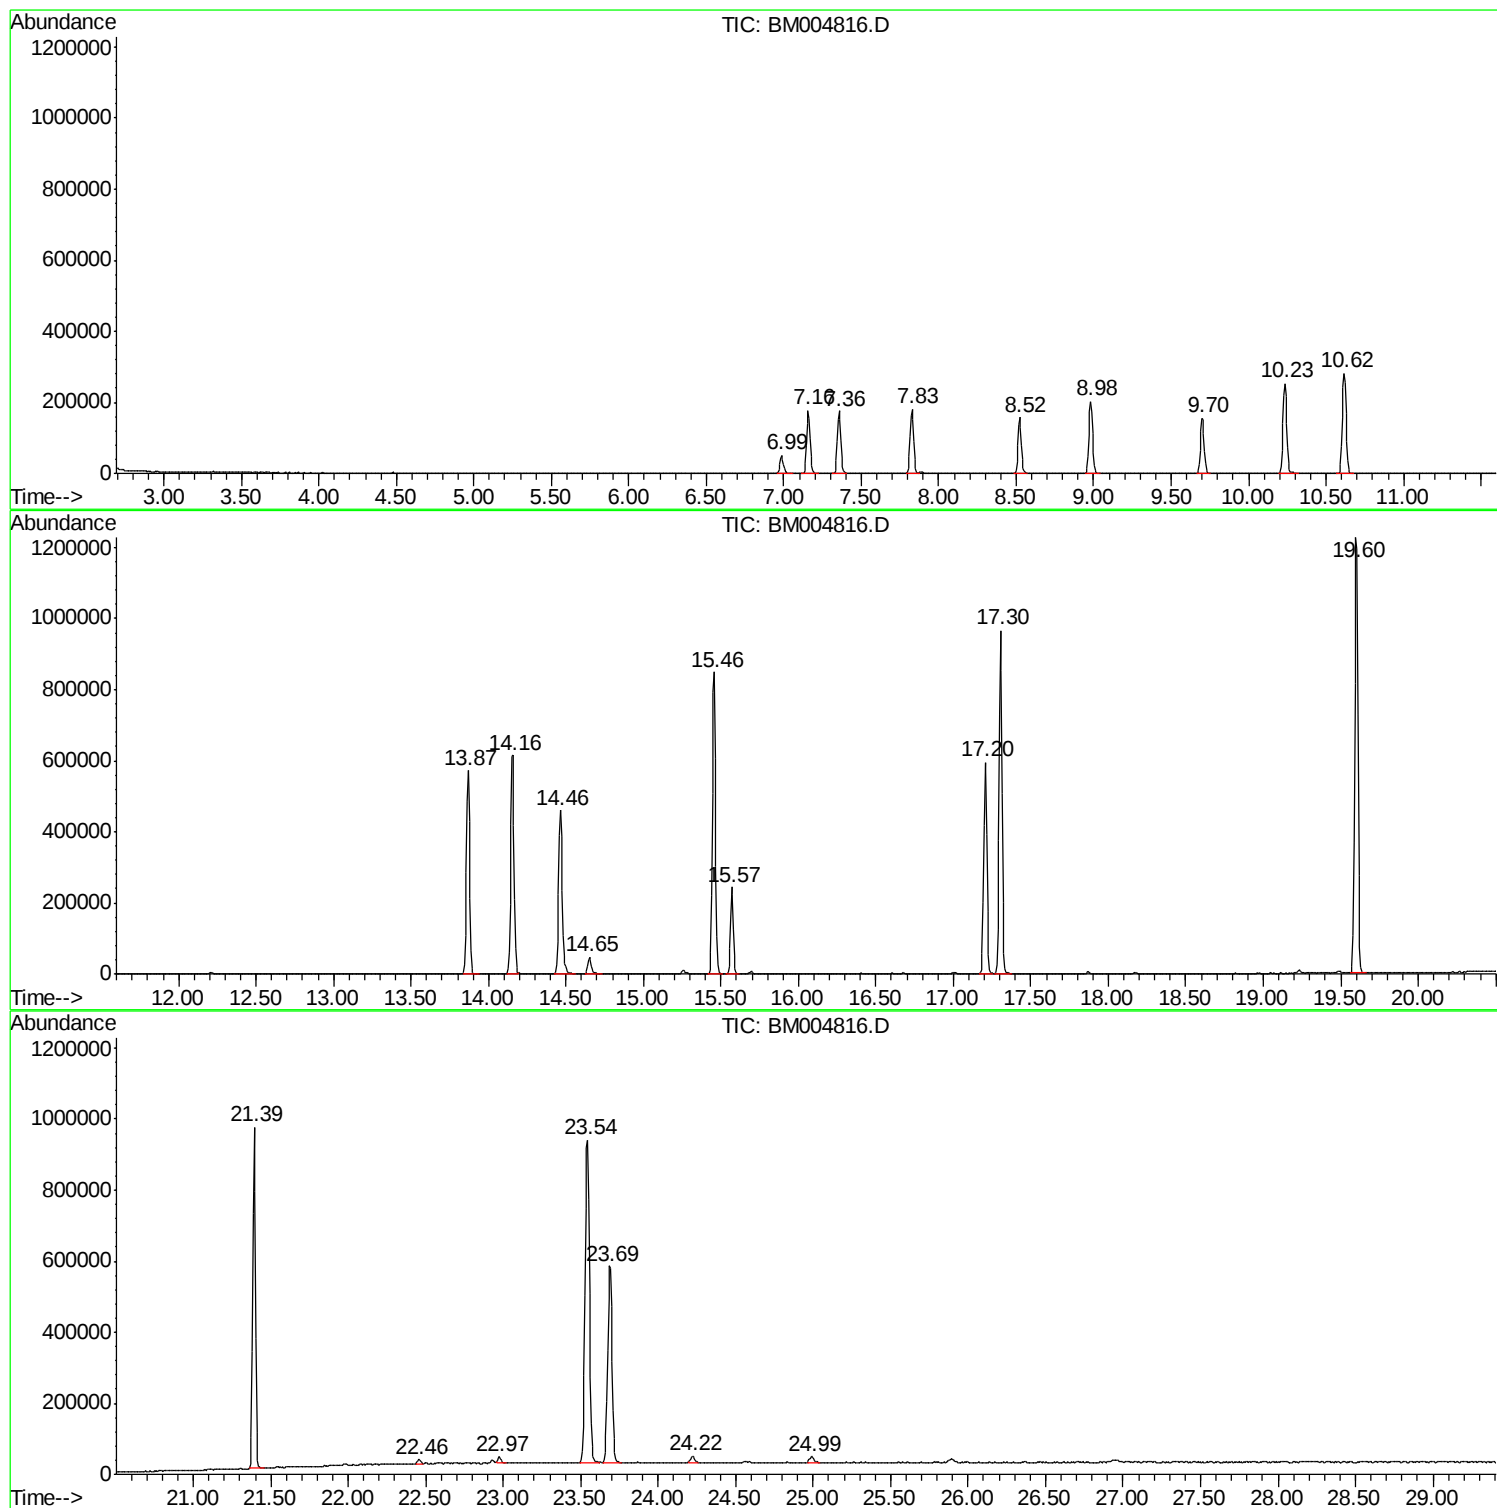

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
Data File : BM004816.D
Acq On : 29 Mar 2016 12:09
Operator : UM/SJ
Sample : H1939-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9SF3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032916\
Data File : BM004816.D
Acq On : 29 Mar 2016 12:09
Operator : UM/SJ
Sample : H1939-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9SF3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc