
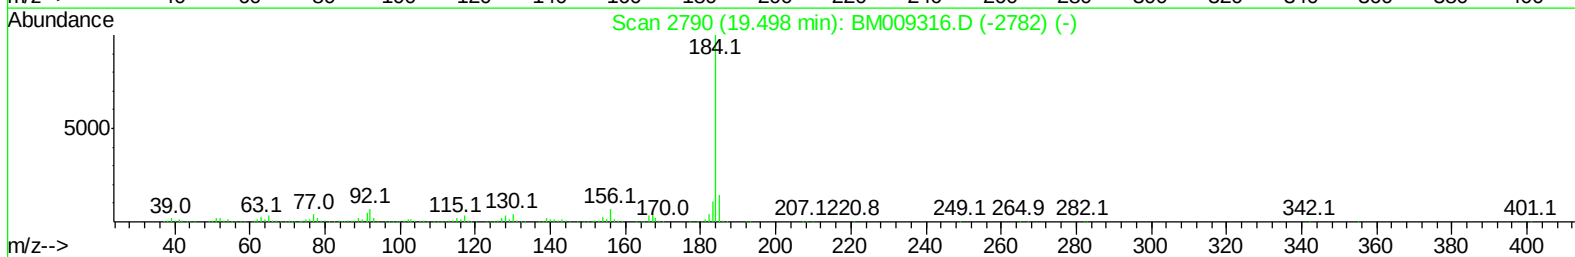
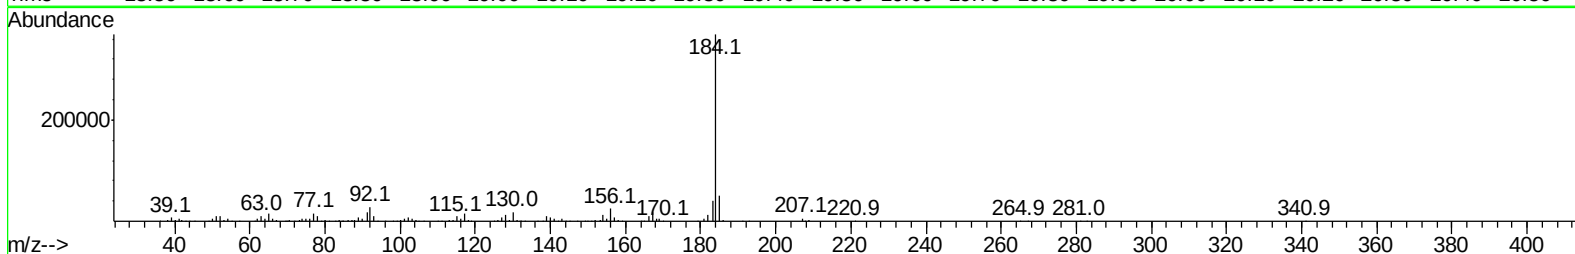


Data Path : Z:\HPCHEM1\BNA M\Data\BM032917\
 Data File : BM009431.D
 Acq On : 29 Mar 2017 14:13
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 07:21:11 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 22 16:43:02 2017
 Response via : Initial Calibration

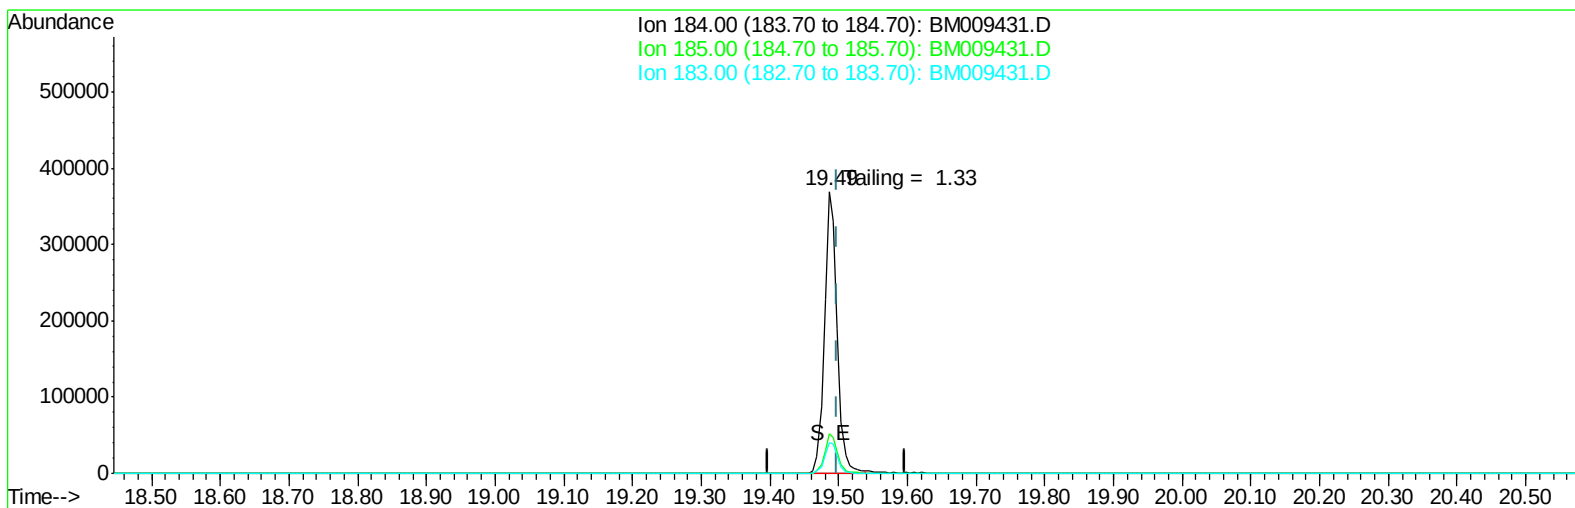

TIC: BM009431.D

(76) Benzidine




19.486min (-0.012) 0.00ng

response 480281

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.89
183.00	11.10	10.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM032917\
Data File : BM009431.D
Acq On : 29 Mar 2017 14:13
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 07:21:11 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 16:43:02 2017
Response via : Initial Calibration

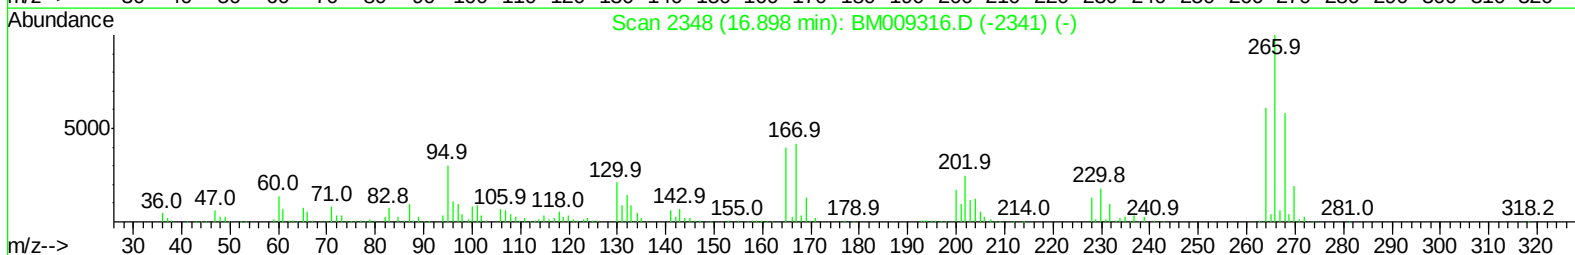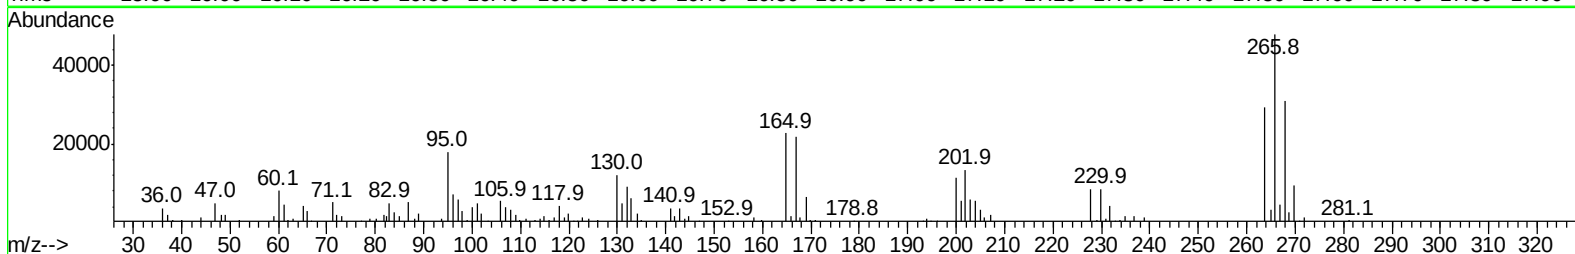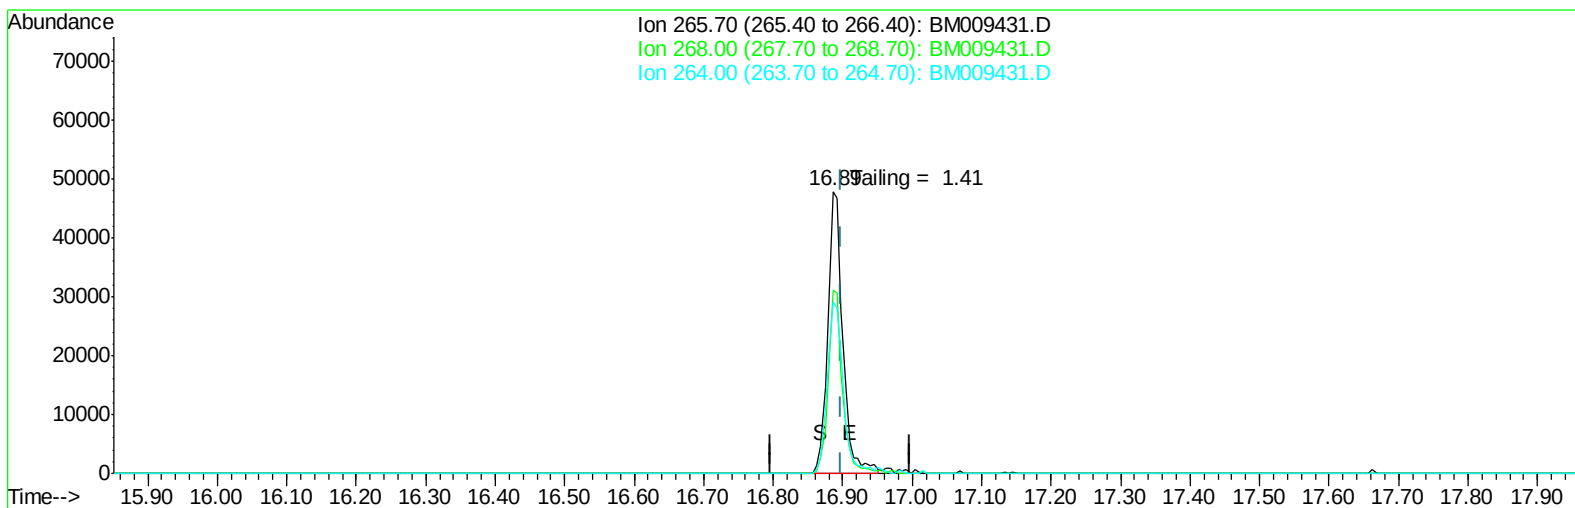

TIC: BM009431.D

(69) Pentachlorophenol (C)

16.886min (-0.012) 0.00ng

response 72747

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.87
264.00	61.20	61.10
0.00	0.00	0.00