


Data Path : Z:\HPCHEM1\BNA M\Data\BM032917\
 Data File : BM009443.D
 Acq On : 30 Mar 2017 09:12
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 27 16:10:49 2017

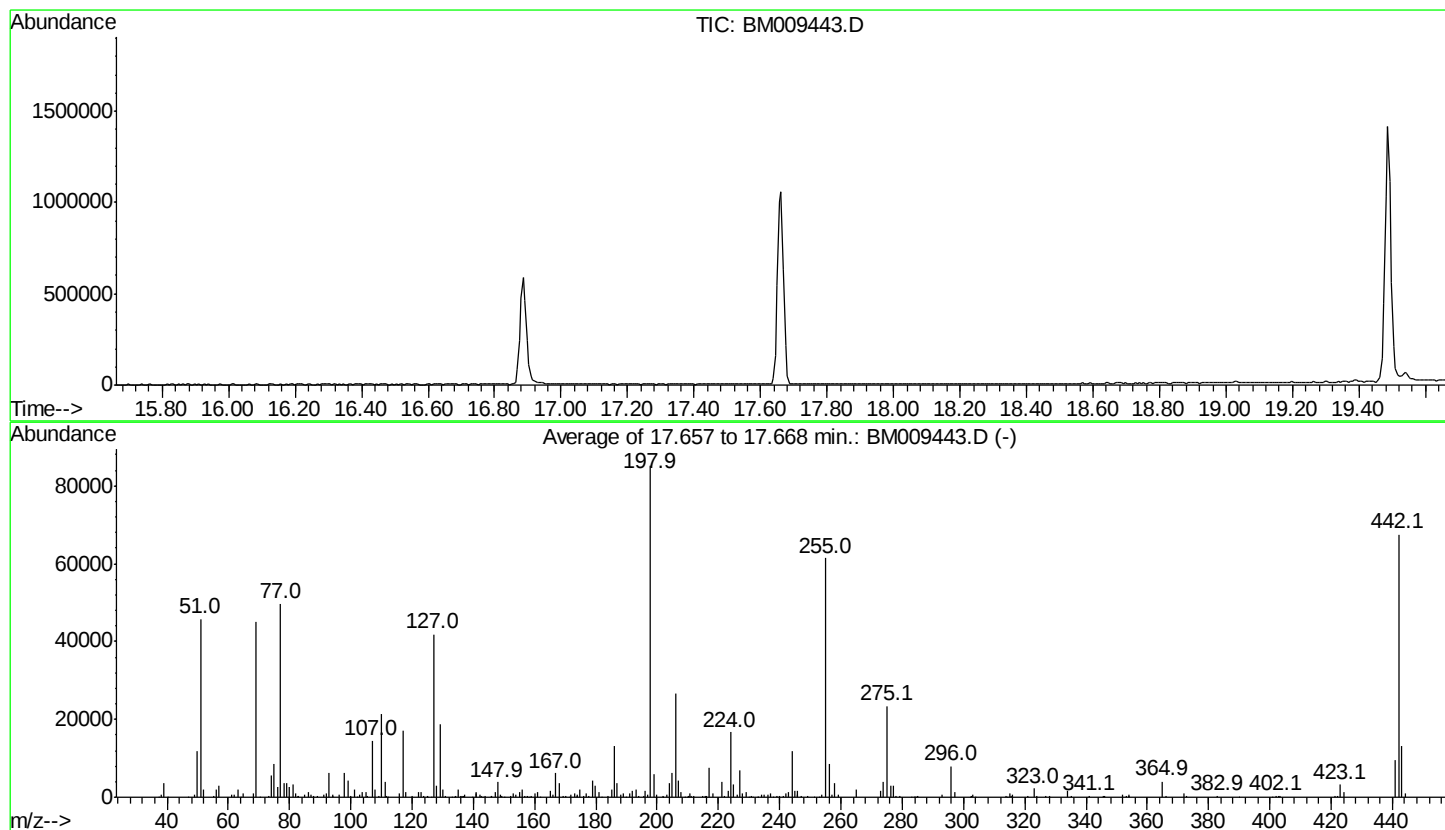

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.8	45829	PASS
68	69	0.00	2	1.9	848	PASS
69	198	0.00	100	52.9	45045	PASS
70	69	0.00	2	0.4	171	PASS
127	198	10	80	49.1	41810	PASS
197	198	0.00	2	0.8	715	PASS
198	198	100	100	100.0	85200	PASS
199	198	5	9	6.8	5798	PASS
275	198	10	60	27.5	23416	PASS
365	198	1	100	4.6	3957	PASS
441	442	0.01	24	14.3	9654	PASS
442	198	50	100	79.3	67549	PASS
443	442	15	24	19.3	13004	PASS