




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034402.D
 Acq On : 29 Mar 2022 12:04
 Operator : CG/JU
 Sample : N2079-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5W6

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:29:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/02/2022

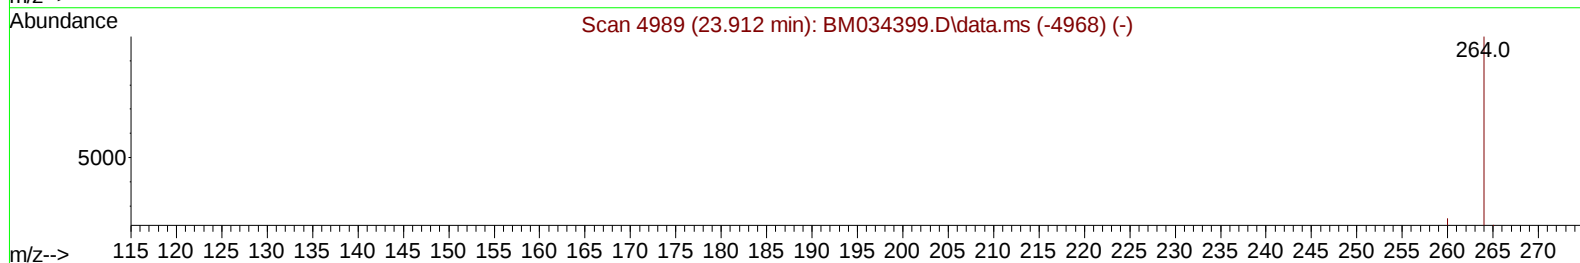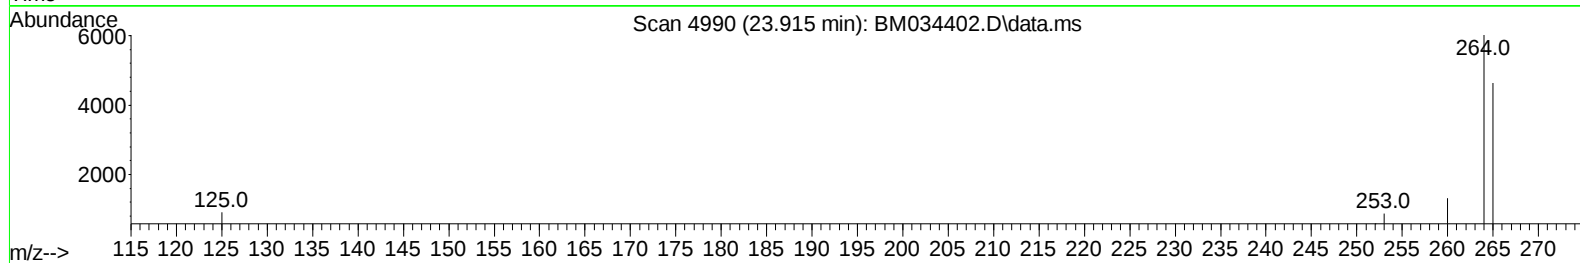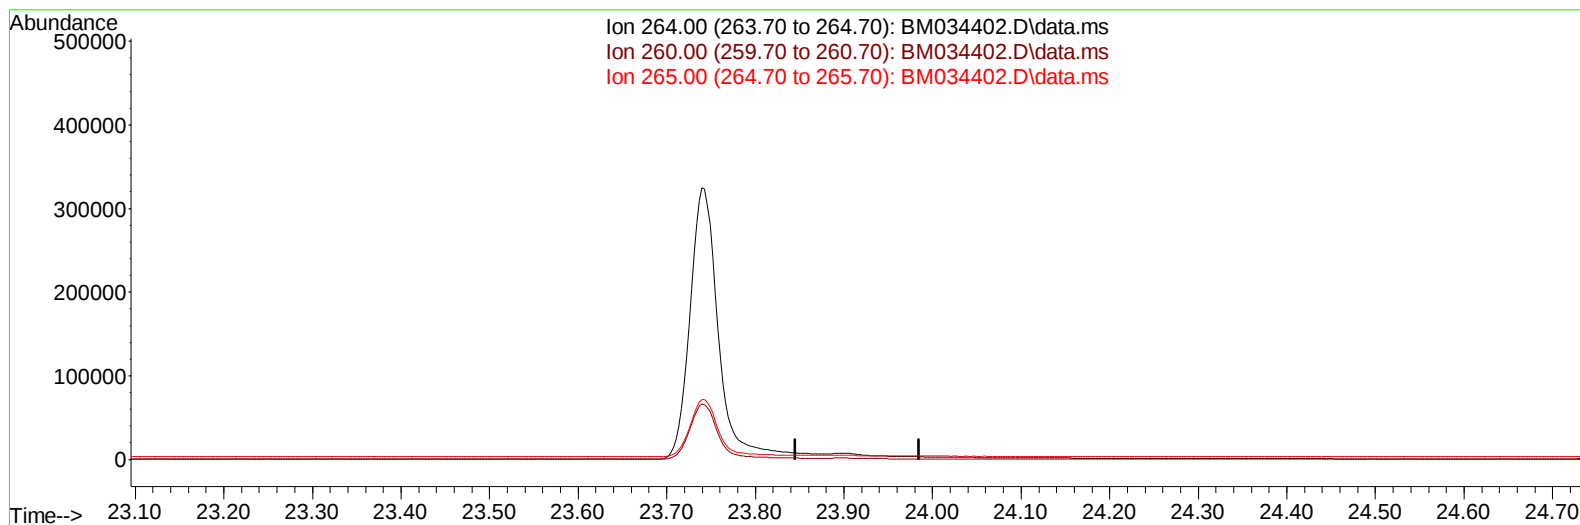

TIC: BM034402.D\data.ms

(23) Perylene-d12 (I)

23.915min (-23.915) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034402.D
Acq On : 29 Mar 2022 12:04
Operator : CG/JU
Sample : N2079-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW5W6

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:29:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/02/2022

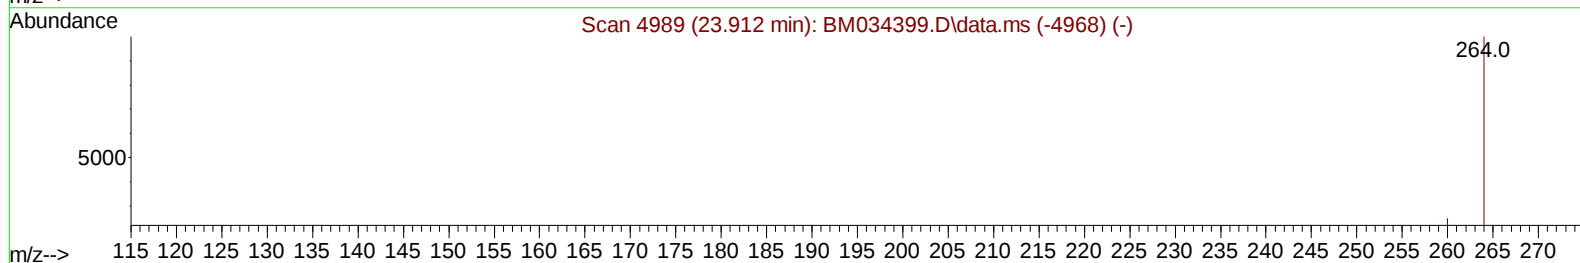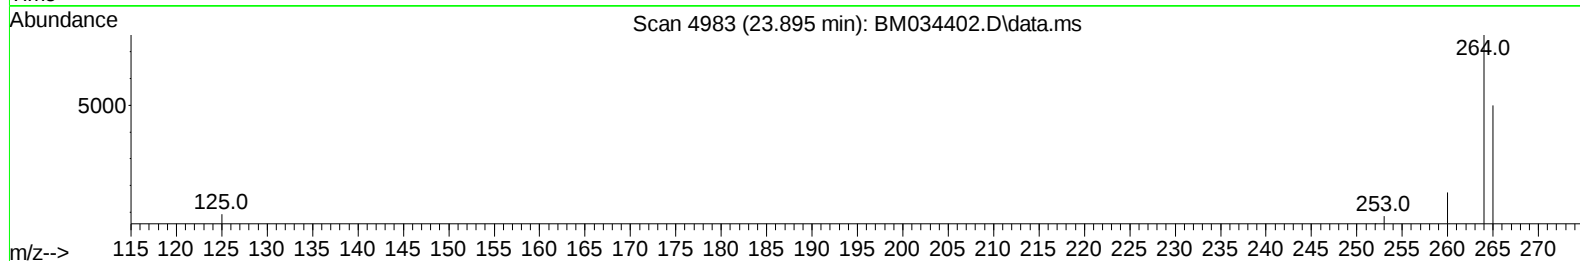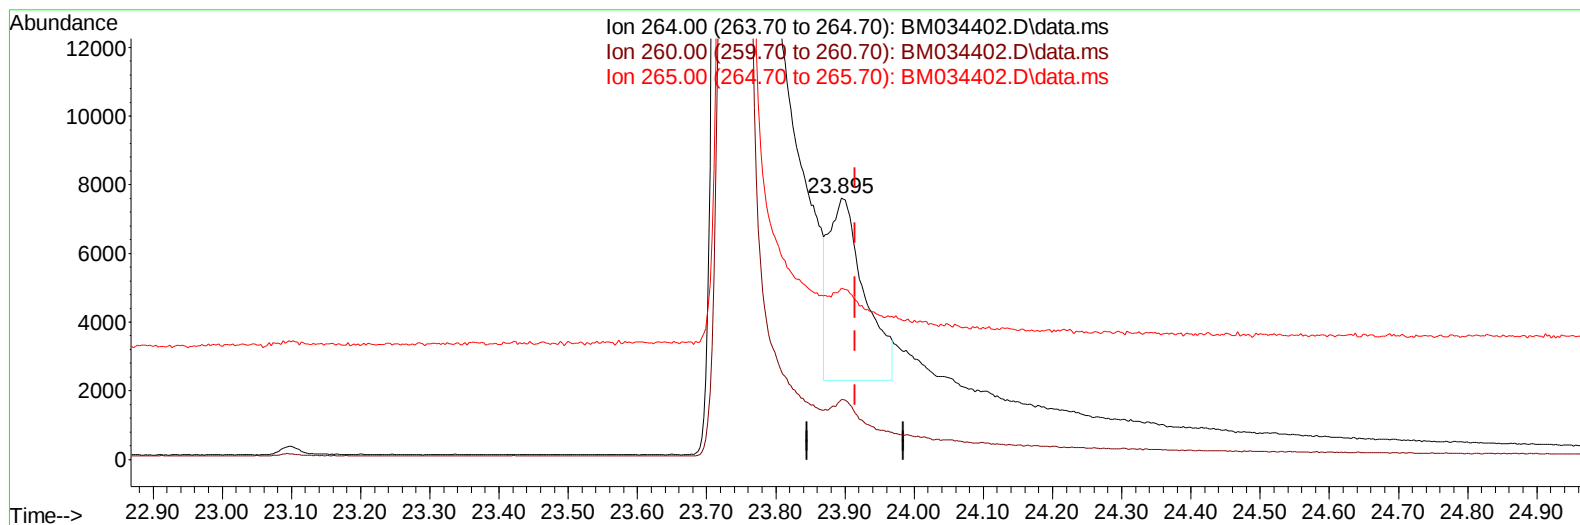

TIC: BM034402.D\data.ms

(23) Perylene-d12 (I)

23.895min (-0.020) 0.40 ng/ul m

response 19170

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	22.82
265.00	95.30	65.39#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034402.D
 Acq On : 29 Mar 2022 12:04
 Operator : CG/JU
 Sample : N2079-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5W6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 02:29:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.933	152		2512	0.400	ng/ul	0.00
4) Naphthalene-d8	10.741	136		6607	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.574	164		3997	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.312	188		7400	0.400	ng/ul	-0.01
17) Chrysene-d12	21.495	240		5591	0.400	ng/ul	# 0.00
23) Perylene-d12	23.895	264		19170m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.305	96		16019	4.287	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152		3365	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.338	212		8265	0.474	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.343	88		7012	1.699	ng/ul#	85
14) Pentachlorophenol	16.974	266		408	0.137	ng/ul	98
15) Phenanthrene	17.354	178		566	0.024	ng/ul#	59
19) Fluoranthene	19.371	202		635	0.025	ng/ul#	44
26) Benzo(a)pyrene	23.740	252		2463	0.036	ng/ul#	31

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034402.D
Acq On : 29 Mar 2022 12:04
Operator : CG/JU
Sample : N2079-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW5W6

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:29:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

04/01/2022
Supervised By :Yogesh
Patel

04/02/2022

