




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034403.D
 Acq On : 29 Mar 2022 12:40
 Operator : CG/JU
 Sample : N2079-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW618

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:29:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/02/2022

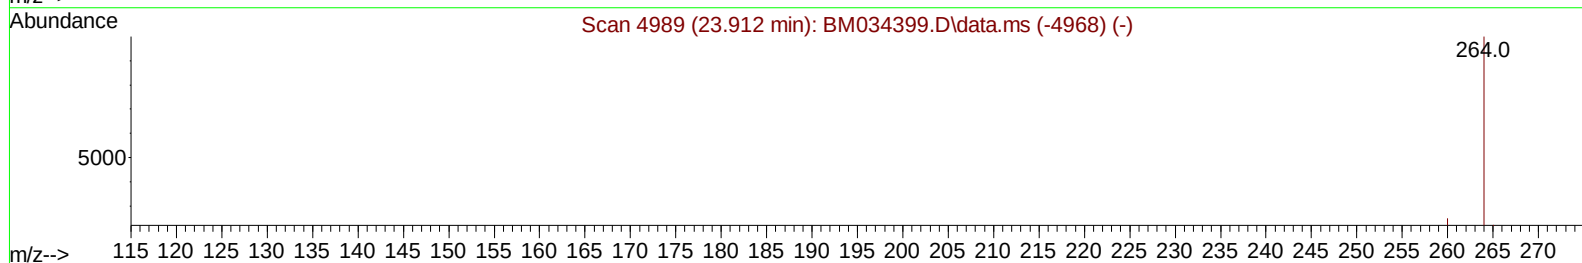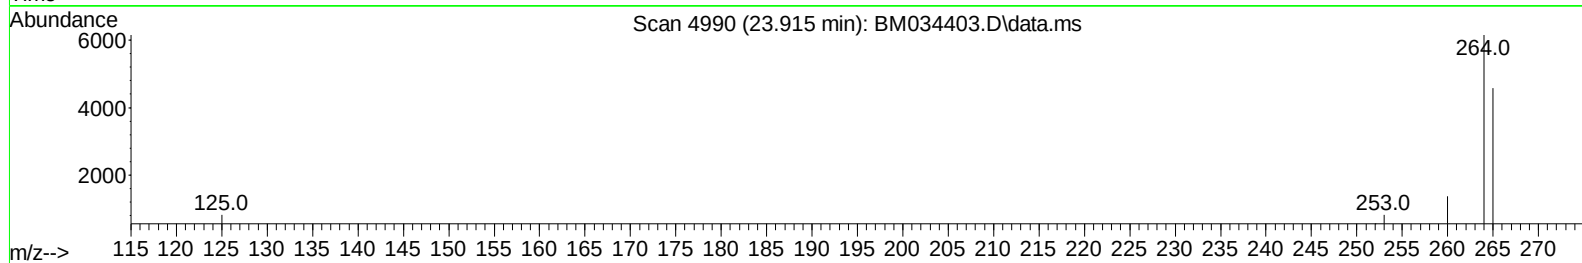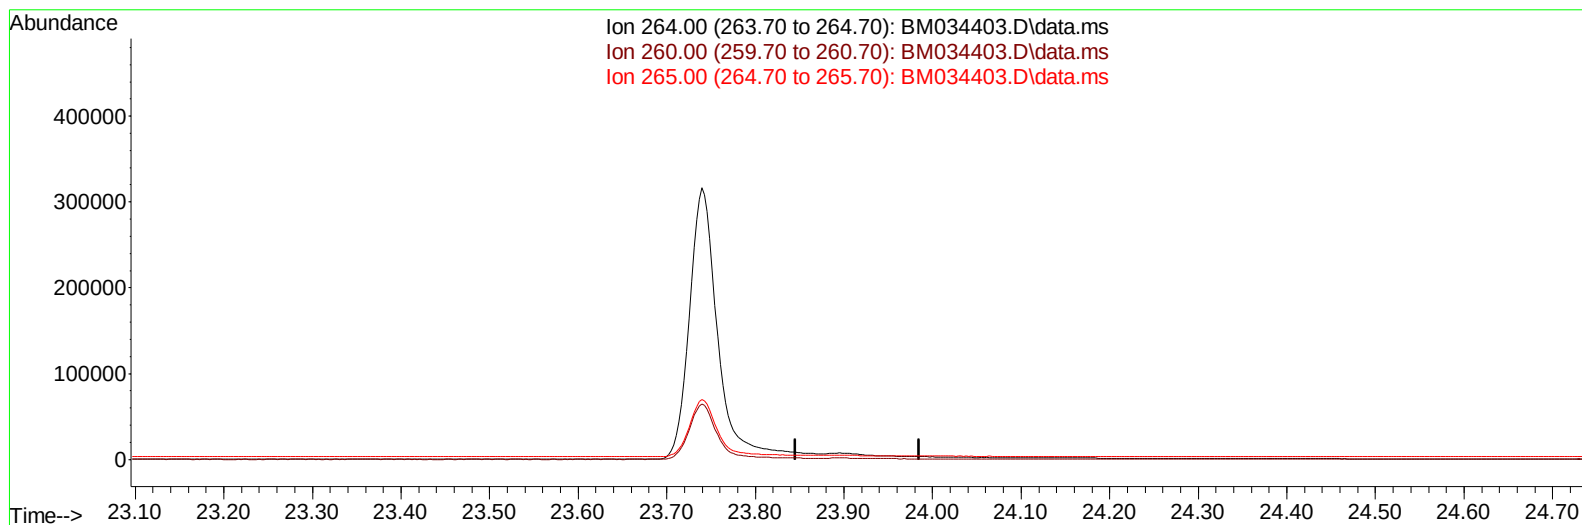

TIC: BM034403.D\data.ms

(23) Perylene-d12 (I)

23.915min (-23.915) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034403.D
 Acq On : 29 Mar 2022 12:40
 Operator : CG/JU
 Sample : N2079-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW618

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:29:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/02/2022

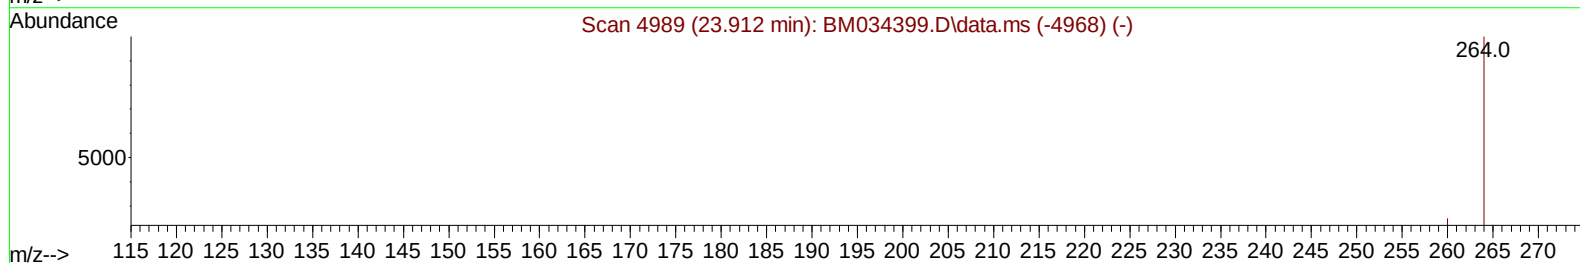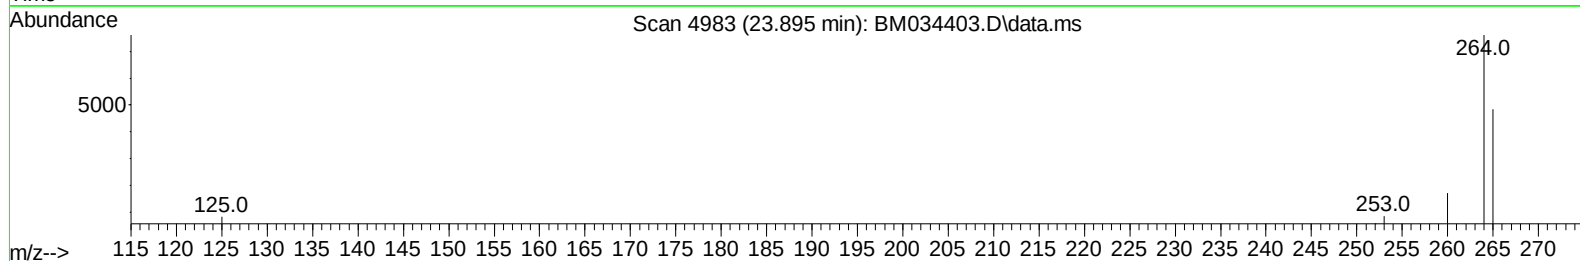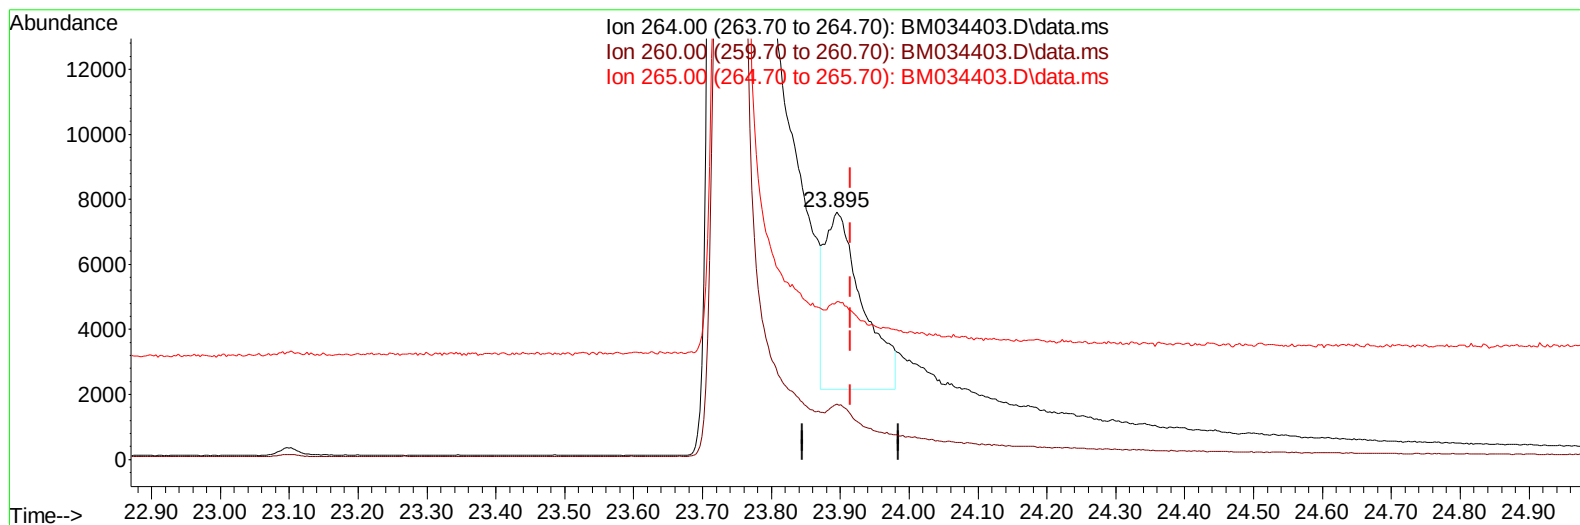

TIC: BM034403.D\data.ms

(23) Perylene-d12 (I)

23.895min (-0.020) 0.40 ng/ul m

response 20780

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	22.39
265.00	95.30	63.72#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034403.D
 Acq On : 29 Mar 2022 12:40
 Operator : CG/JU
 Sample : N2079-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW618

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 02:29:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	2385	0.400	ng/ul	0.00
4) Naphthalene-d8	10.741	136	6438	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.573	164	3571	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.316	188	6585	0.400	ng/ul	0.00
17) Chrysene-d12	21.504	240	5064	0.400	ng/ul	# 0.00
23) Perylene-d12	23.895	264	20780m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	15818	4.459	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	3533	0.407	ng/ul	0.00
18) Fluoranthene-d10	19.338	212	7648	0.484	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.343	88	2911	0.743	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034403.D
Acq On : 29 Mar 2022 12:40
Operator : CG/JU
Sample : N2079-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW618

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:29:38 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/02/2022

