




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034410.D
 Acq On : 29 Mar 2022 16:53
 Operator : CG/JU
 Sample : N2079-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Z5

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:31:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

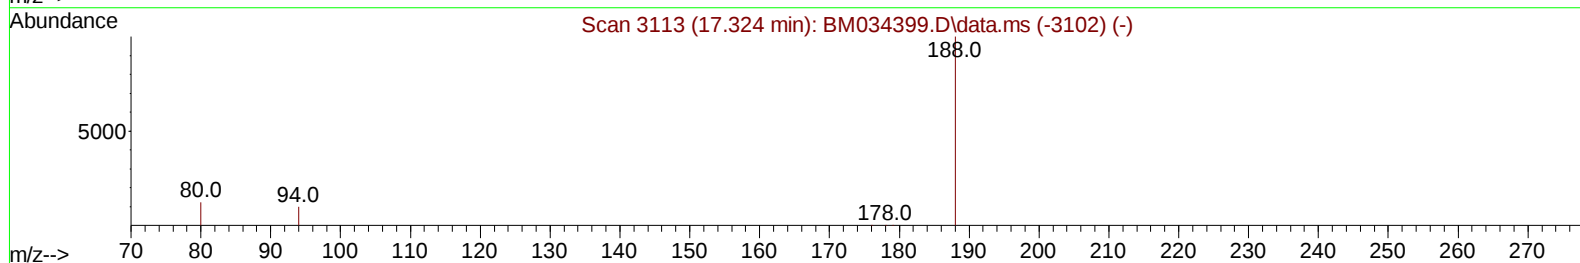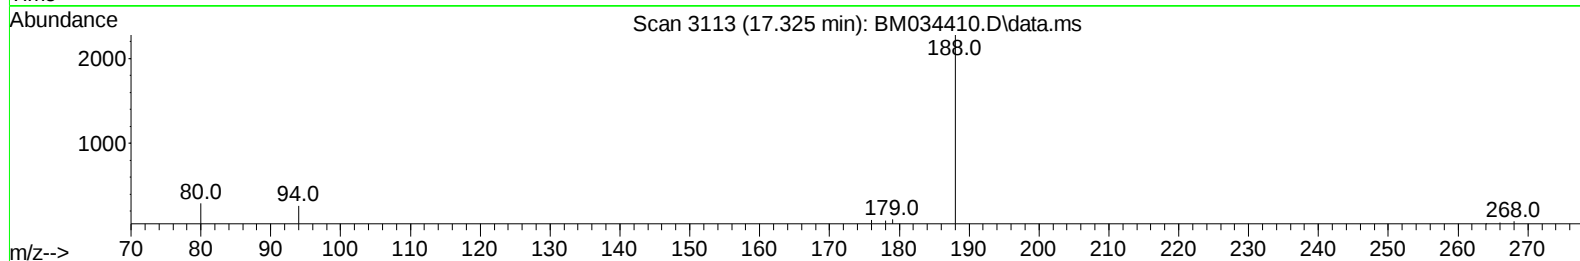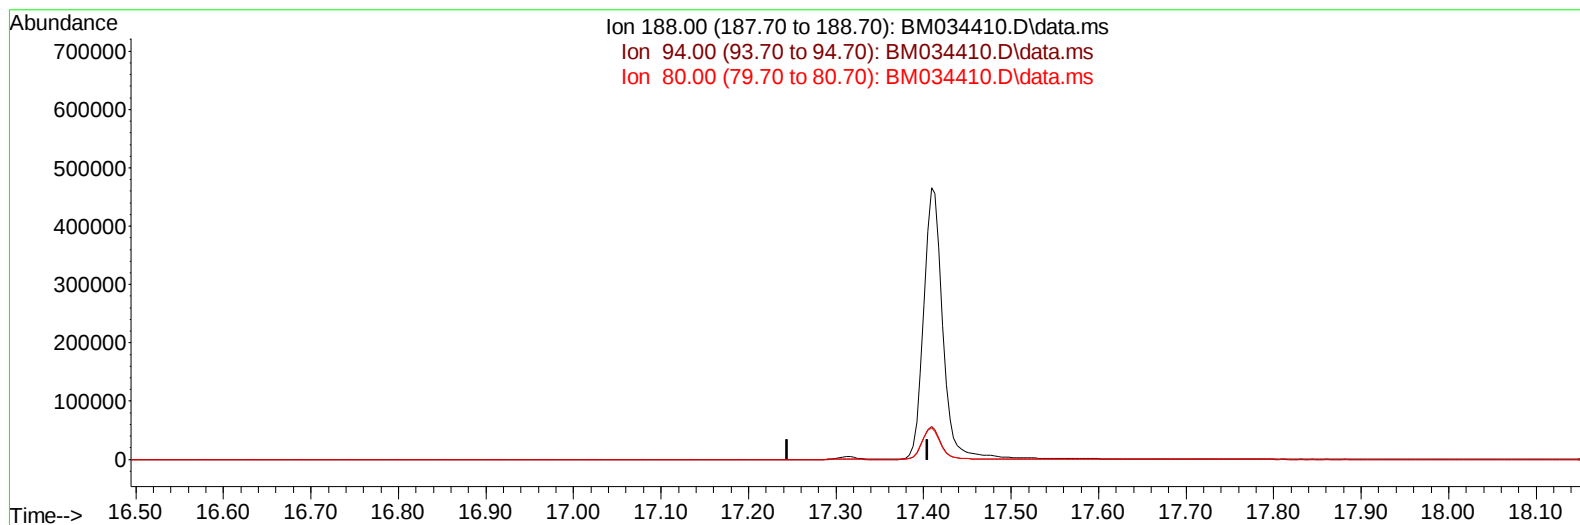

TIC: BM034410.D\data.ms

(13) Phenanthrene-d10 (I)

17.324min (-17.324) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	13.30	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034410.D
 Acq On : 29 Mar 2022 16:53
 Operator : CG/JU
 Sample : N2079-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Z5

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:31:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

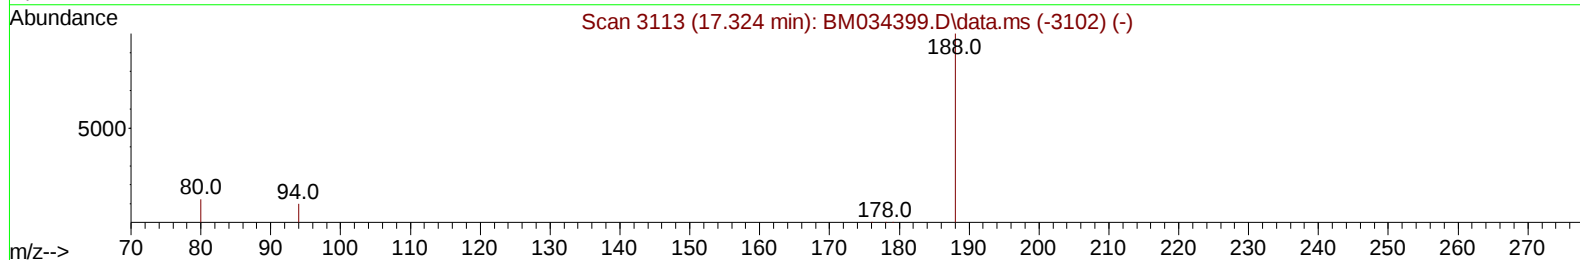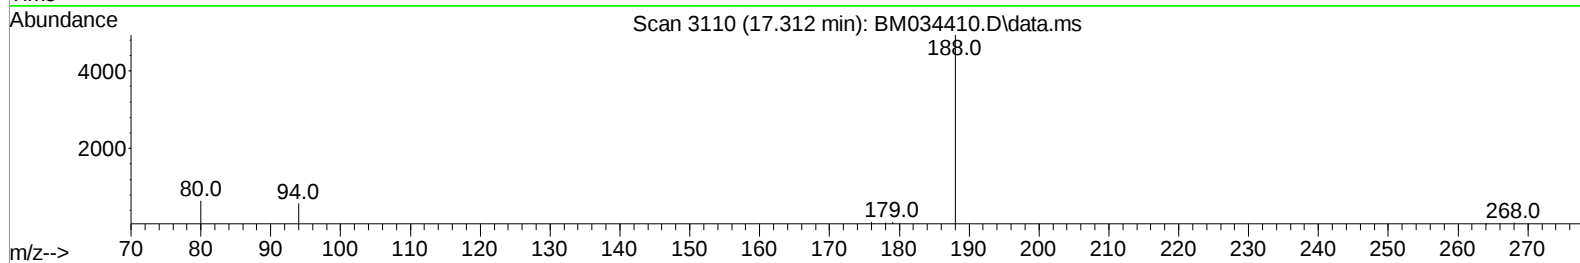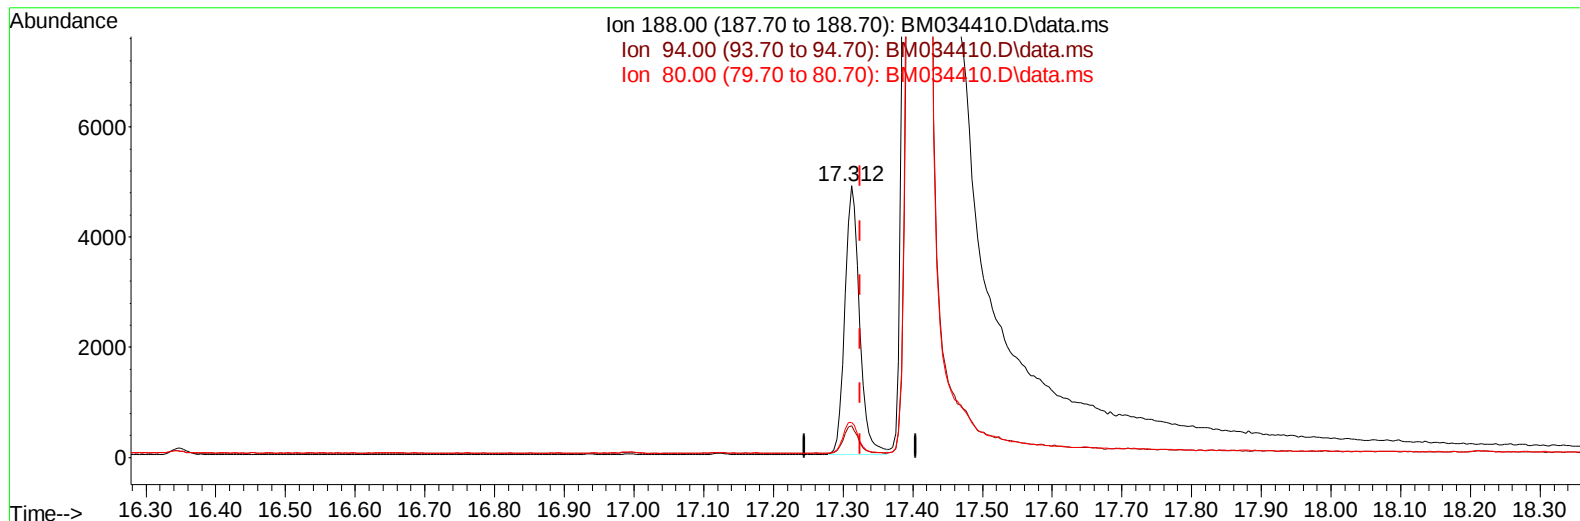

TIC: BM034410.D\data.ms

(13) Phenanthrene-d10 (I)

17.312min (-0.012) 0.40 ng/ul m

response 7144

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.30	11.69
80.00	15.50	12.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034410.D
 Acq On : 29 Mar 2022 16:53
 Operator : CG/JU
 Sample : N2079-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Z5

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:31:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

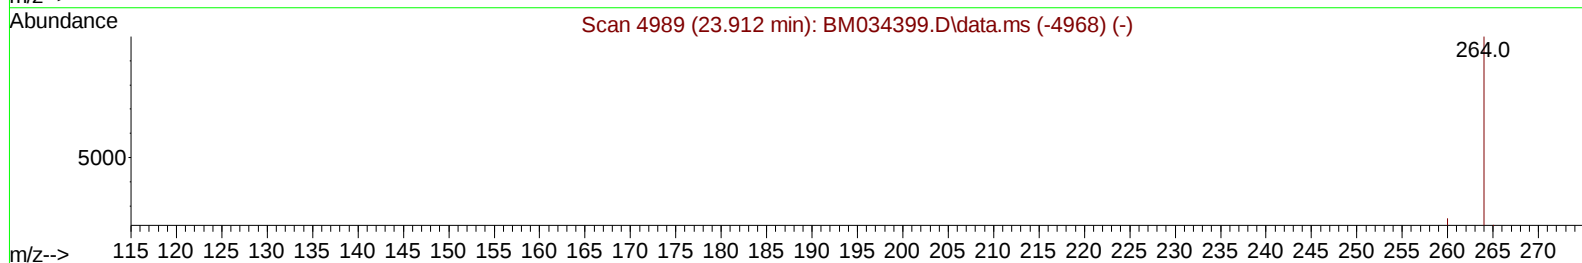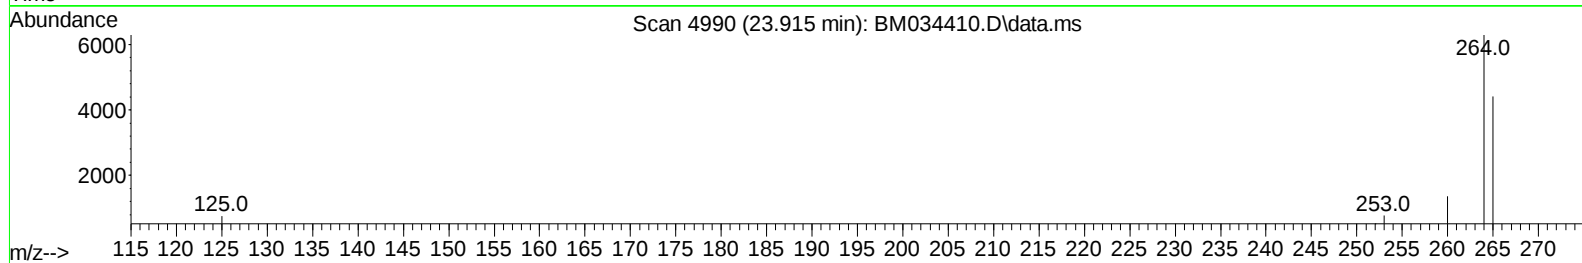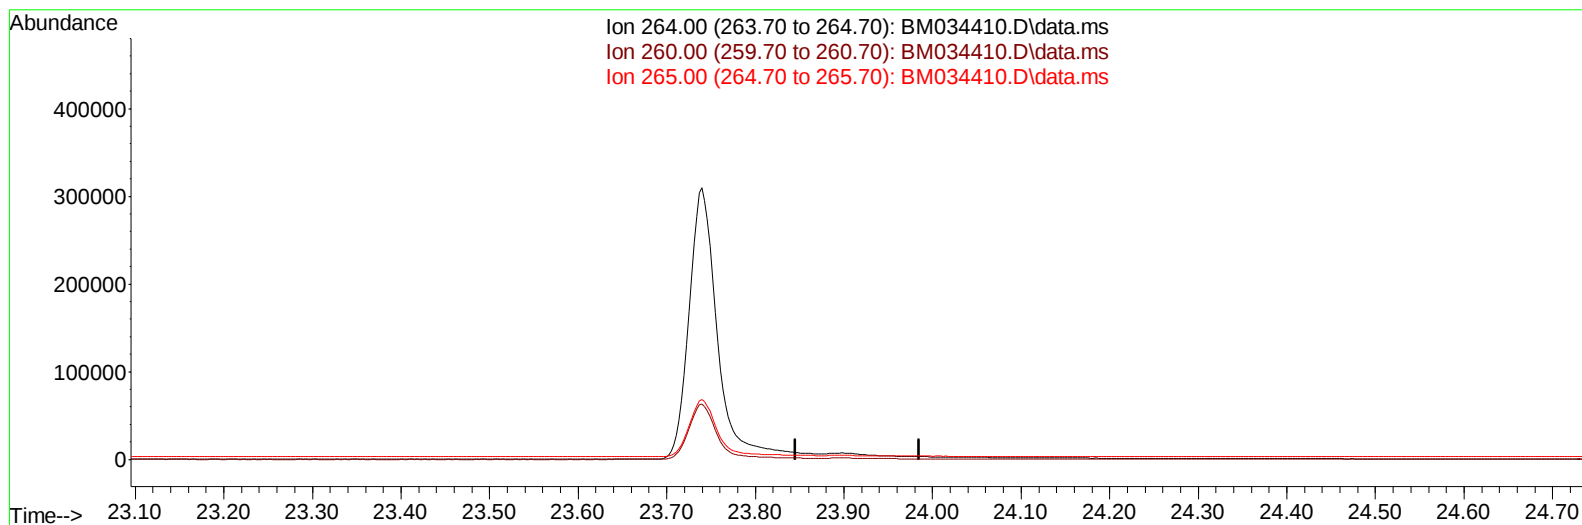

TIC: BM034410.D\data.ms

(23) Perylene-d12 (I)

23.915min (-23.915) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034410.D
 Acq On : 29 Mar 2022 16:53
 Operator : CG/JU
 Sample : N2079-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Z5

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:31:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

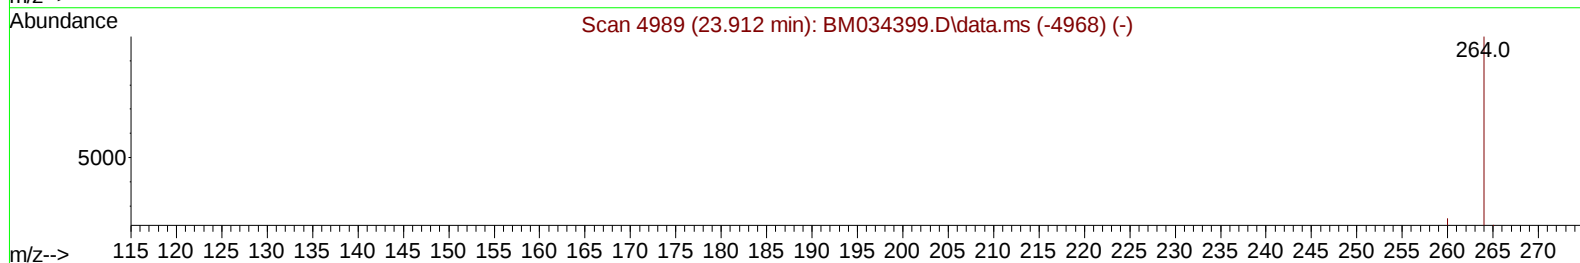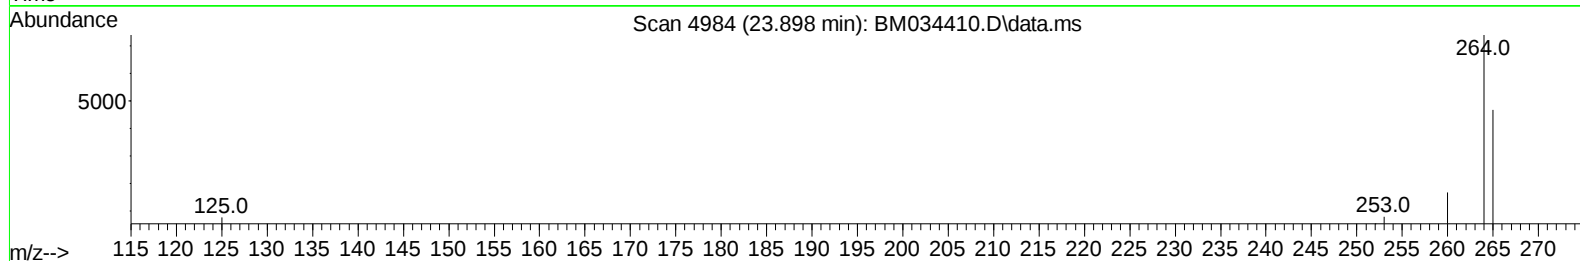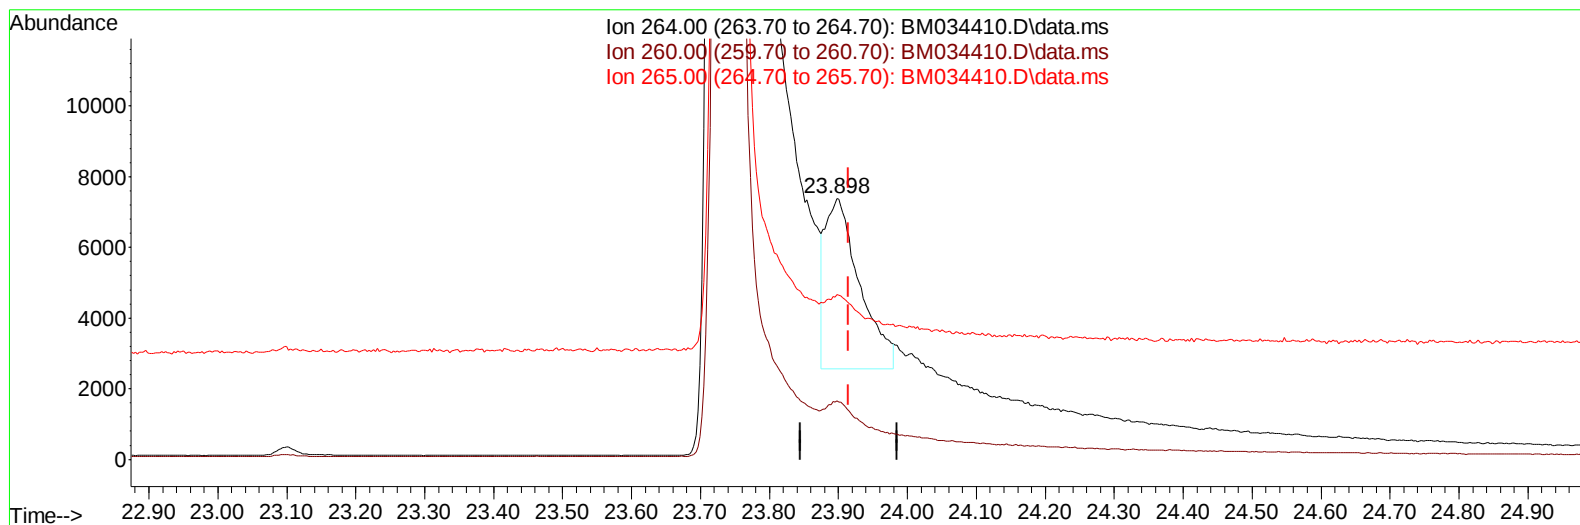

TIC: BM034410.D\data.ms

(23) Perylene-d12 (I)

23.898min (-0.017) 0.40 ng/ul m

response 16904

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	22.59
265.00	95.30	63.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034410.D
 Acq On : 29 Mar 2022 16:53
 Operator : CG/JU
 Sample : N2079-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Z5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 02:31:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.929	152		2449	0.400	ng/ul	0.00
4) Naphthalene-d8	10.741	136		6817	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.574	164		3826	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.312	188		7144m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.504	240		5351	0.400	ng/ul	# 0.00
23) Perylene-d12	23.898	264		16904m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.305	96		16757	4.600	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152		3217	0.350	ng/ul	0.00
18) Fluoranthene-d10	19.338	212		7589	0.455	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034410.D
Acq On : 29 Mar 2022 16:53
Operator : CG/JU
Sample : N2079-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW5Z5

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:31:03 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

