




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034413.D
 Acq On : 29 Mar 2022 18:41
 Operator : CG/JU
 Sample : N2079-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW609

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:31:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

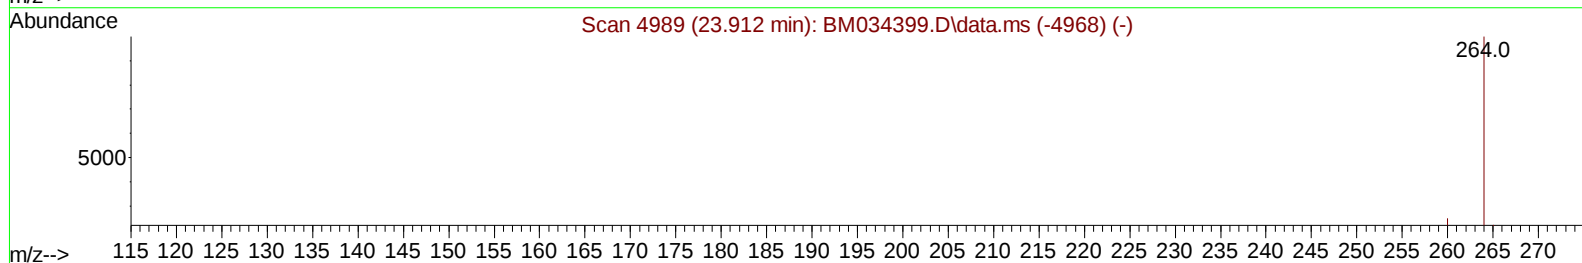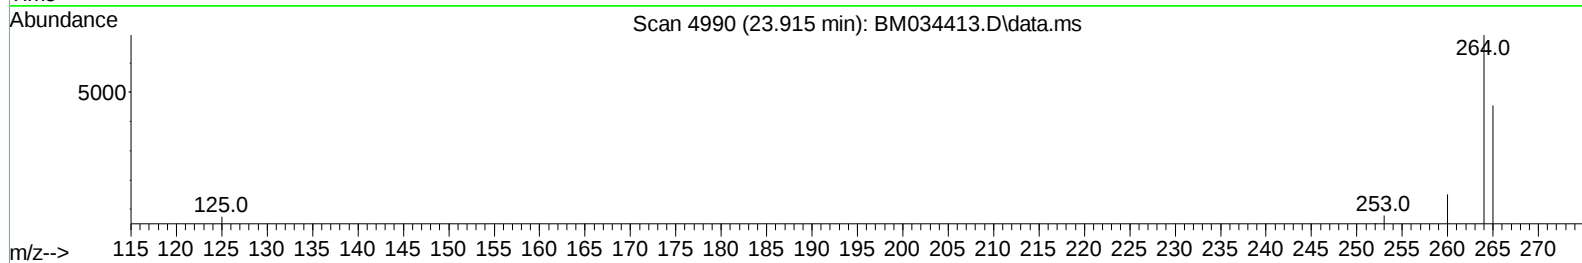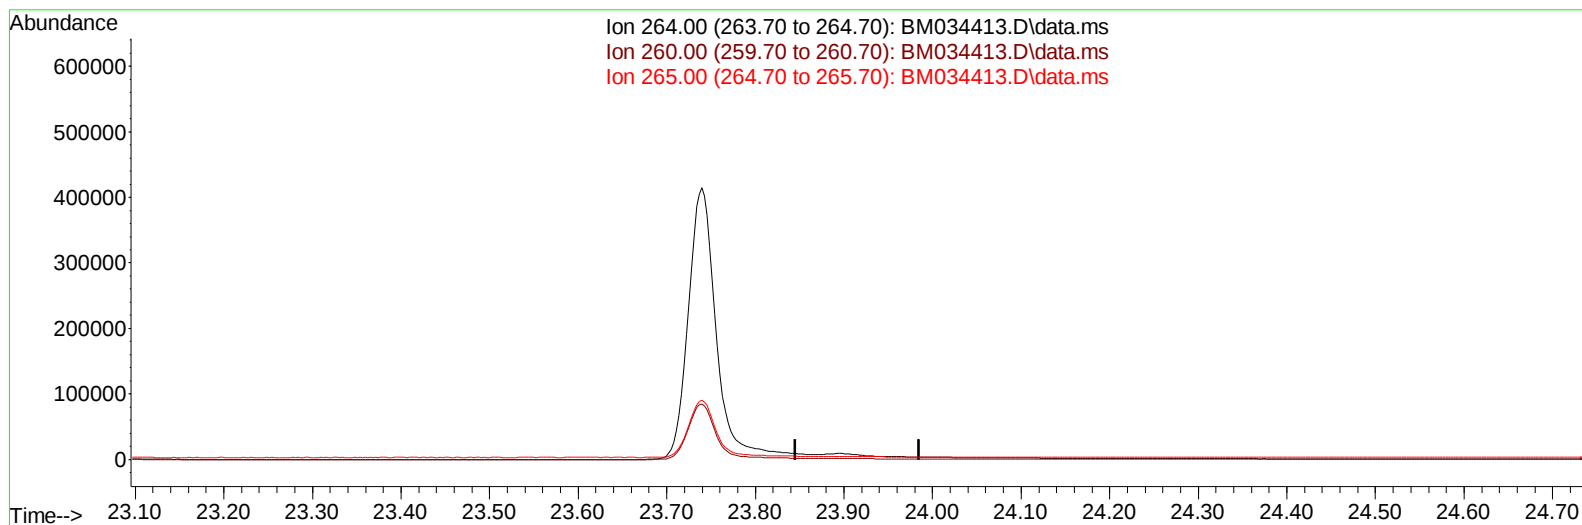

TIC: BM034413.D\data.ms

(23) Perylene-d12 (I)

23.915min (-23.915) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034413.D
 Acq On : 29 Mar 2022 18:41
 Operator : CG/JU
 Sample : N2079-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW609

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:31:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

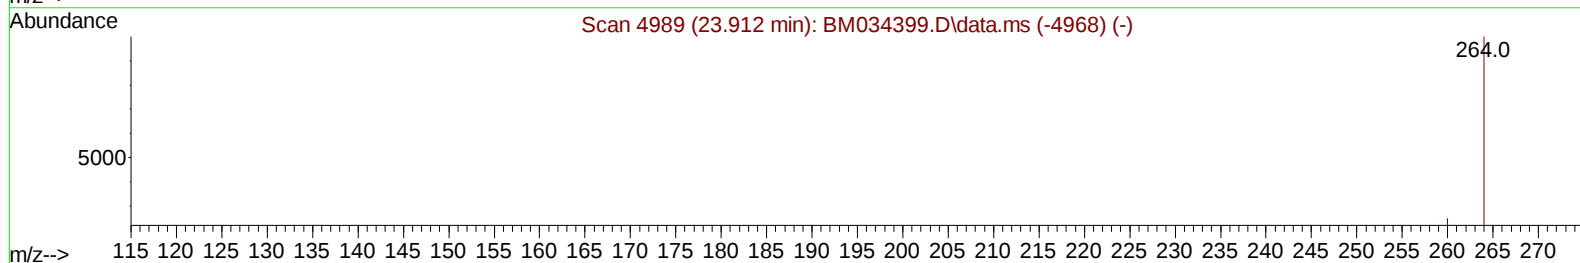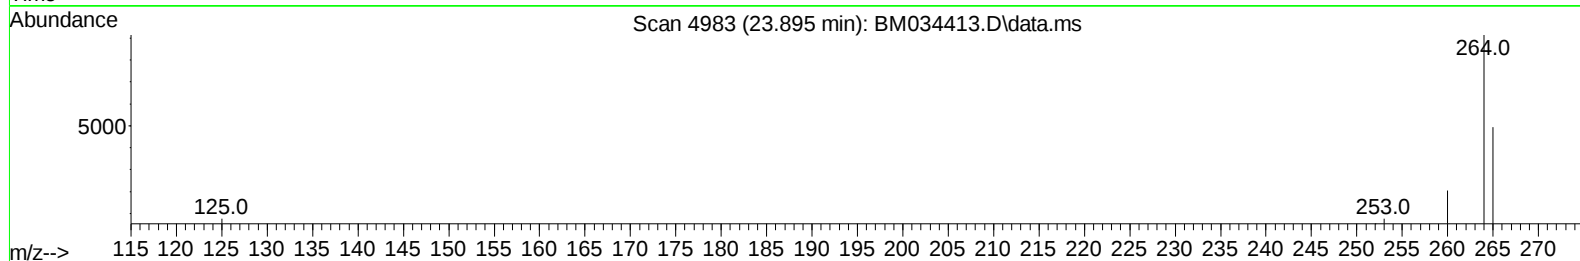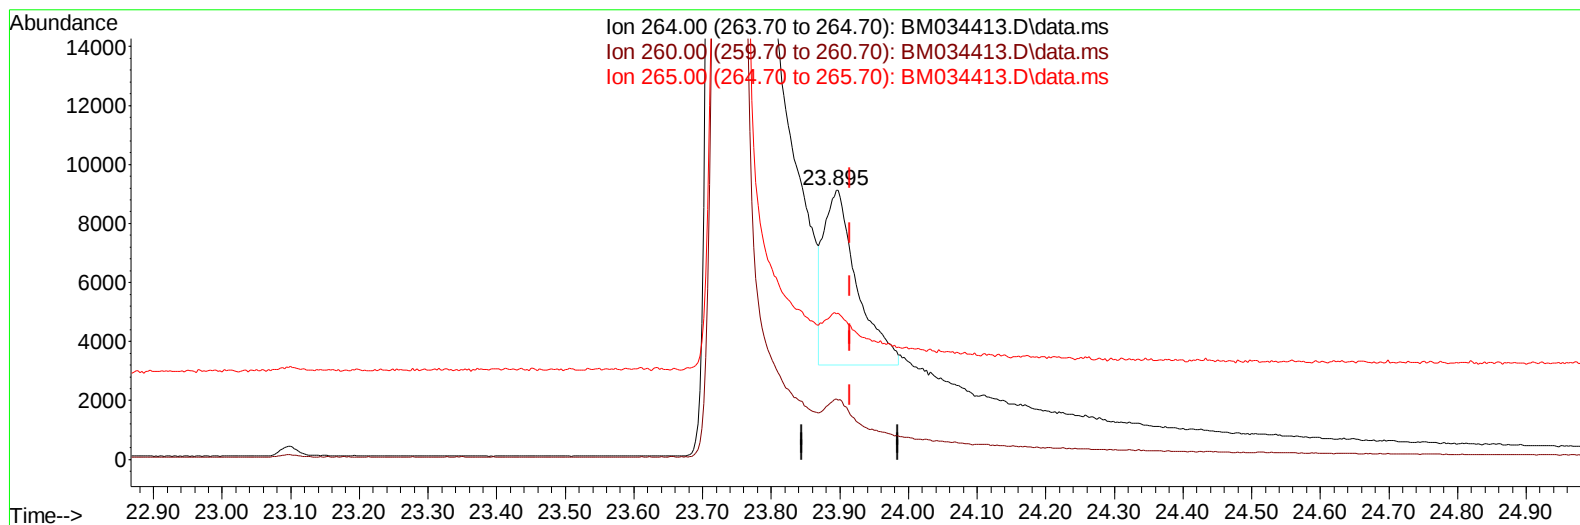

TIC: BM034413.D\data.ms

(23) Perylene-d12 (I)

23.895min (-0.021) 0.40 ng/ul m

response 20183

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	22.41
265.00	95.30	54.13#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034413.D
 Acq On : 29 Mar 2022 18:41
 Operator : CG/JU
 Sample : N2079-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW609

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 02:31:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.929	152		3003	0.400	ng/ul	0.00
4) Naphthalene-d8	10.735	136		8591	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.569	164		4993	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.312	188		9781	0.400	ng/ul	-0.01
17) Chrysene-d12	21.498	240		7278	0.400	ng/ul	# 0.00
23) Perylene-d12	23.895	264		20183m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.305	96		20146	4.510	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152		3965	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.338	212		10442	0.460	ng/ul	0.00
Target Compounds							
							Qvalue
15) Phenanthrene	17.350	178		766	0.025	ng/ul#	77
19) Fluoranthene	19.371	202		748	0.023	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034413.D
Acq On : 29 Mar 2022 18:41
Operator : CG/JU
Sample : N2079-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW609

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:31:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

