




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034424.D
 Acq On : 30 Mar 2022 01:53
 Operator : CG/JU
 Sample : N2079-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Z3

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:33:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

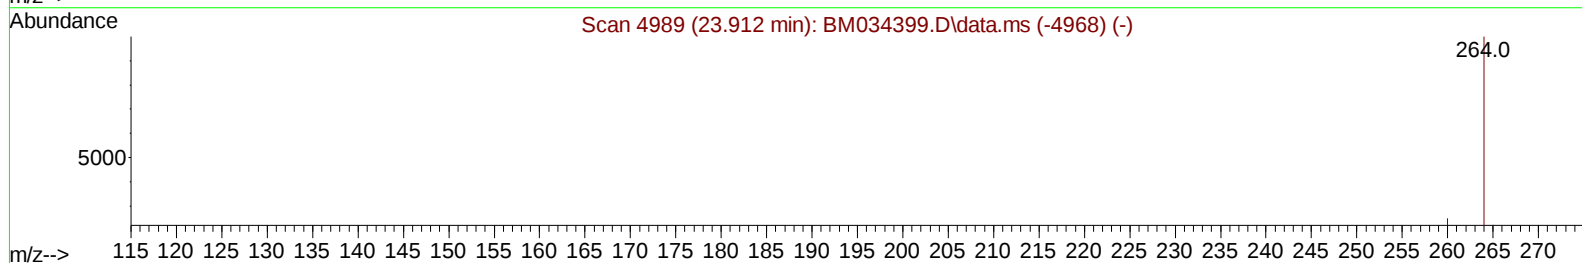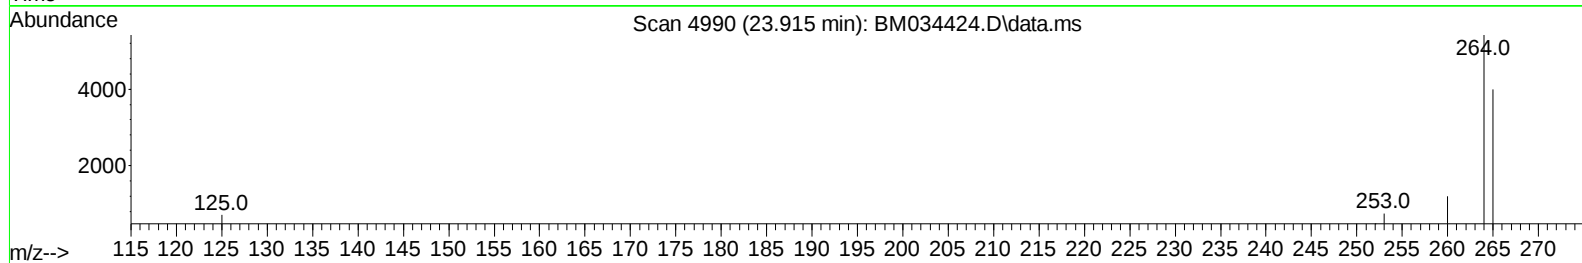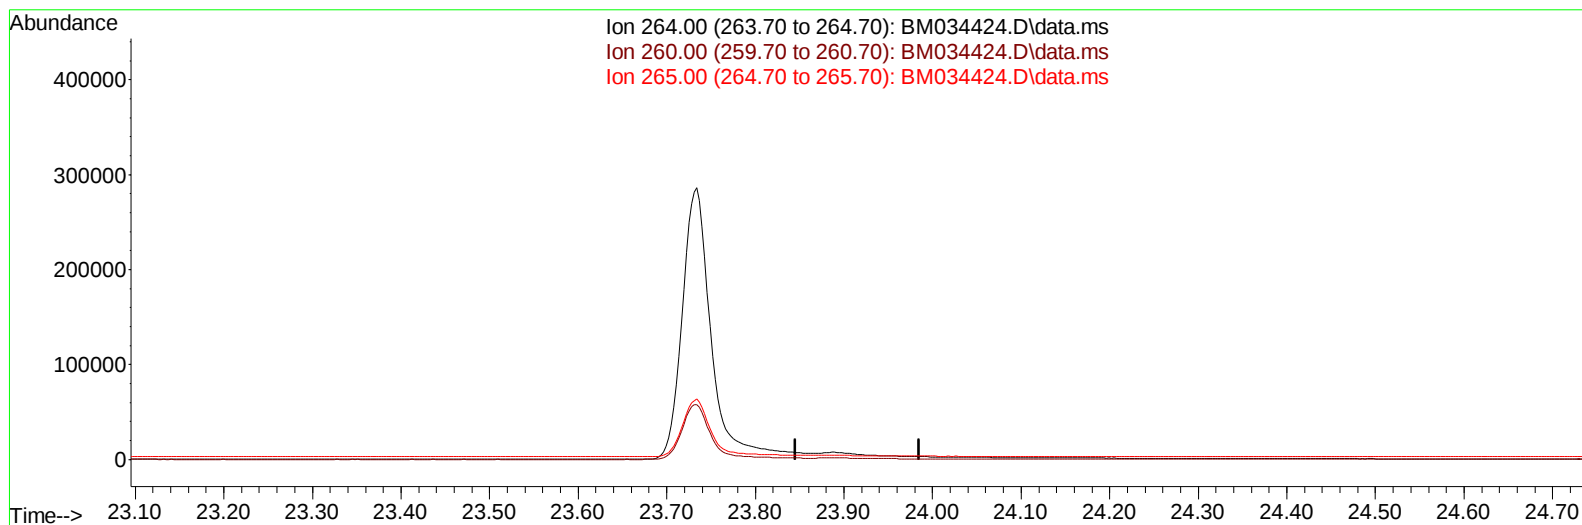

TIC: BM034424.D\data.ms

(23) Perylene-d12 (I)

23.915min (-23.915) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034424.D
 Acq On : 30 Mar 2022 01:53
 Operator : CG/JU
 Sample : N2079-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Z3

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:33:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

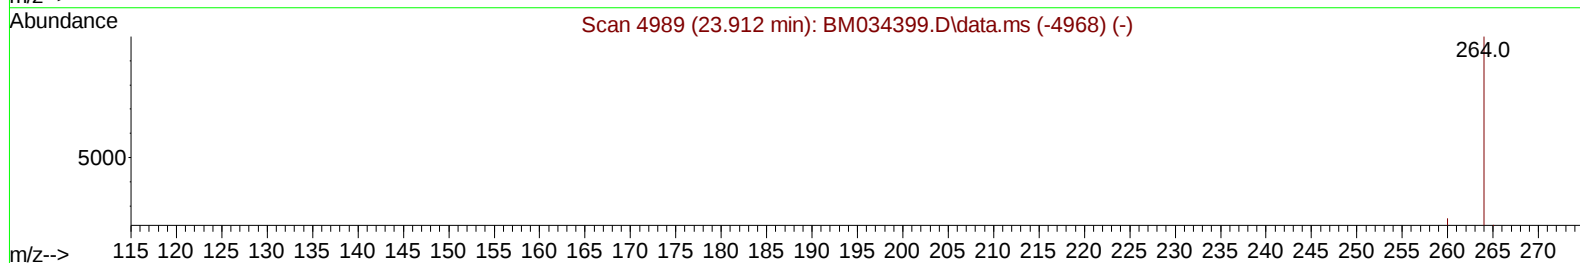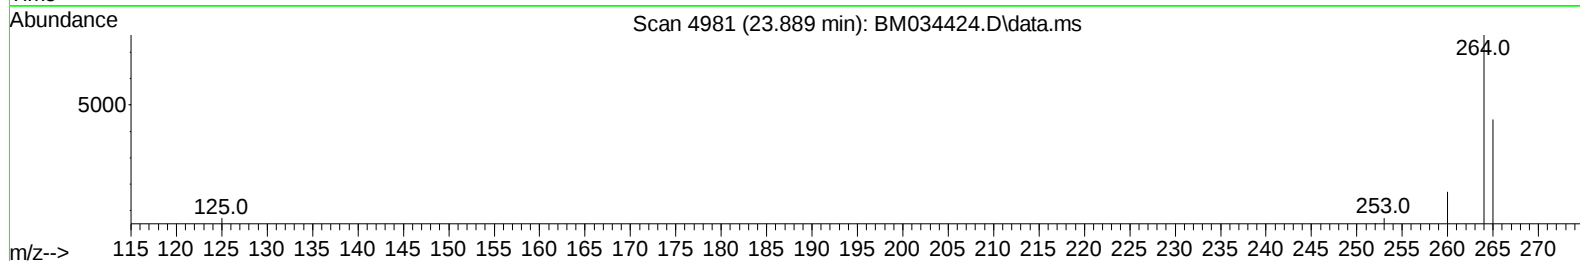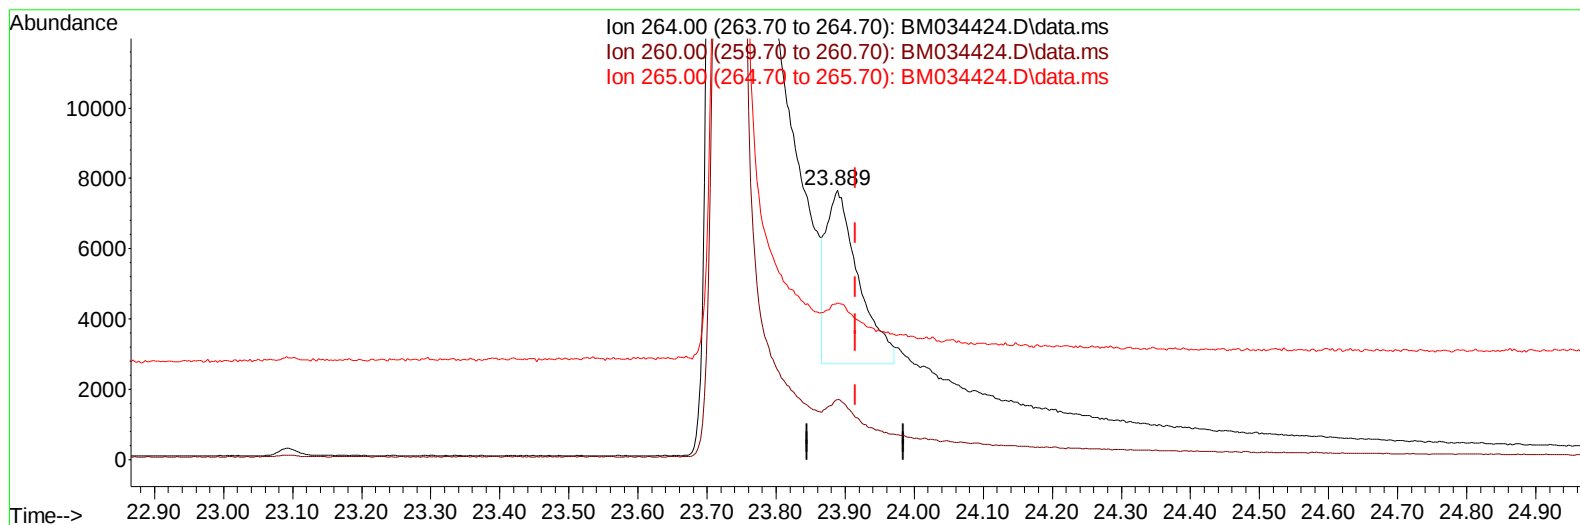

TIC: BM034424.D\data.ms

(23) Perylene-d12 (I)

23.889min (-0.026) 0.40 ng/ul m

response 16181

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	22.17#
265.00	95.30	58.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034424.D
 Acq On : 30 Mar 2022 01:53
 Operator : CG/JU
 Sample : N2079-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Z3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 02:33:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.929	152		3355	0.400	ng/ul	0.00
4) Naphthalene-d8	10.735	136		8489	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.569	164		4397	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.312	188		7795	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.504	240		5741	0.400	ng/ul	# 0.00
23) Perylene-d12	23.889	264		16181m	0.400	ng/ul	-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.309	96		18425	3.692	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152		3196	0.279	ng/ul	0.00
18) Fluoranthene-d10	19.338	212		7304	0.408	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.343	88		4013	0.728	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034424.D
Acq On : 30 Mar 2022 01:53
Operator : CG/JU
Sample : N2079-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW5Z3

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:33:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

