




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034426.D
Acq On : 30 Mar 2022 03:05
Operator : CG/JU
Sample : N2082-12
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW604

Manual IntegrationsAPPROVED

Quant Time: Mar 30 03:53:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

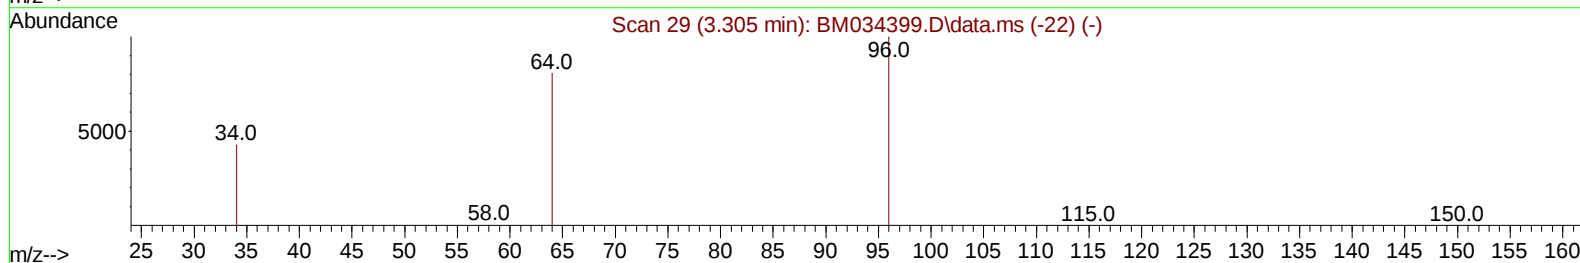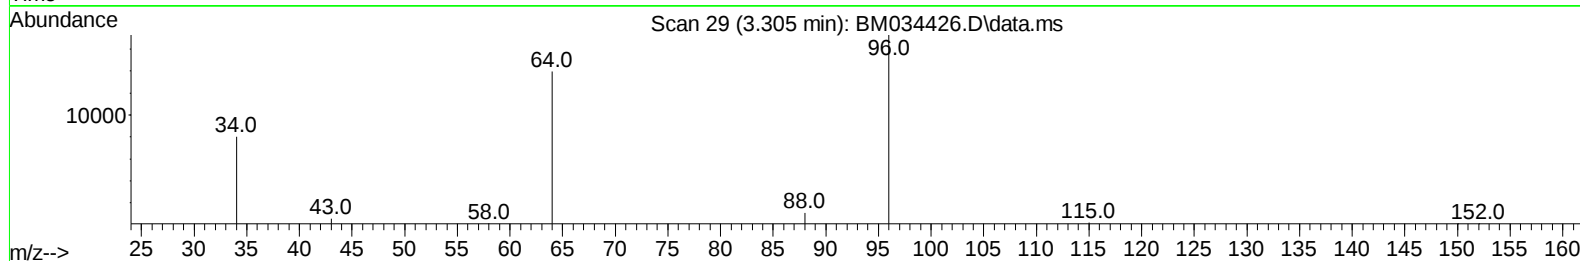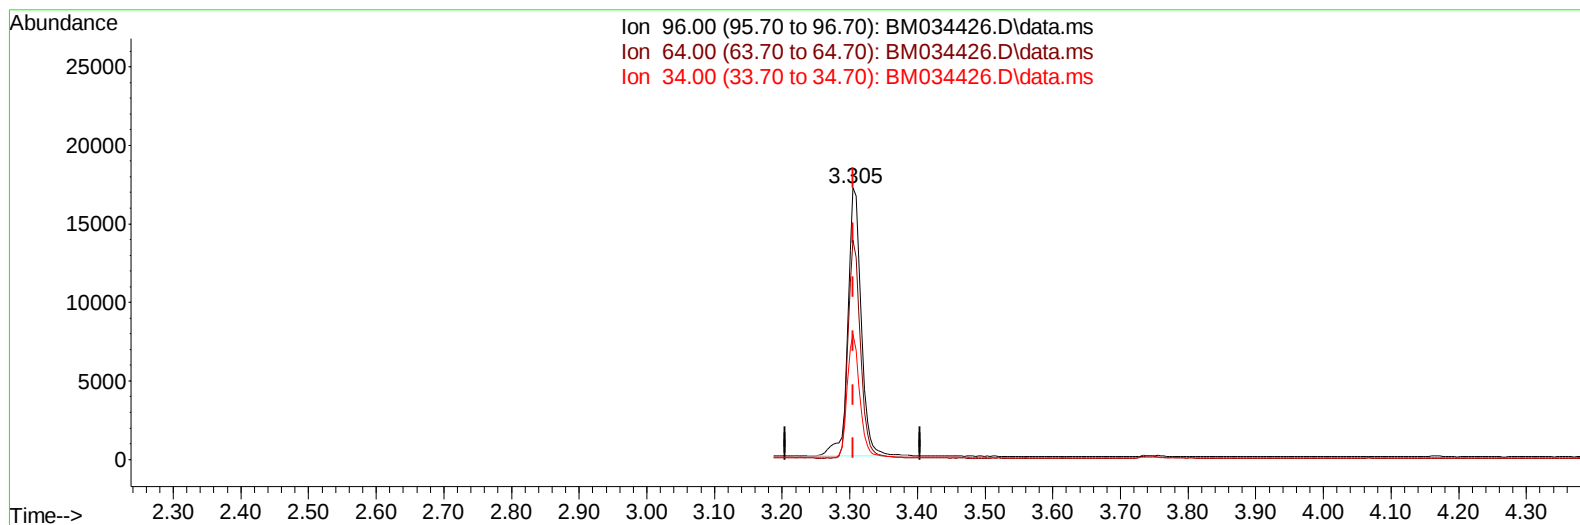

TIC: BM034426.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.305min (+ 0.000) 5.37 ng/u1

response 23252

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	80.66
34.00	243.00	46.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034426.D
 Acq On : 30 Mar 2022 03:05
 Operator : CG/JU
 Sample : N2082-12
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW604

Manual IntegrationsAPPROVED

Quant Time: Mar 30 03:53:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

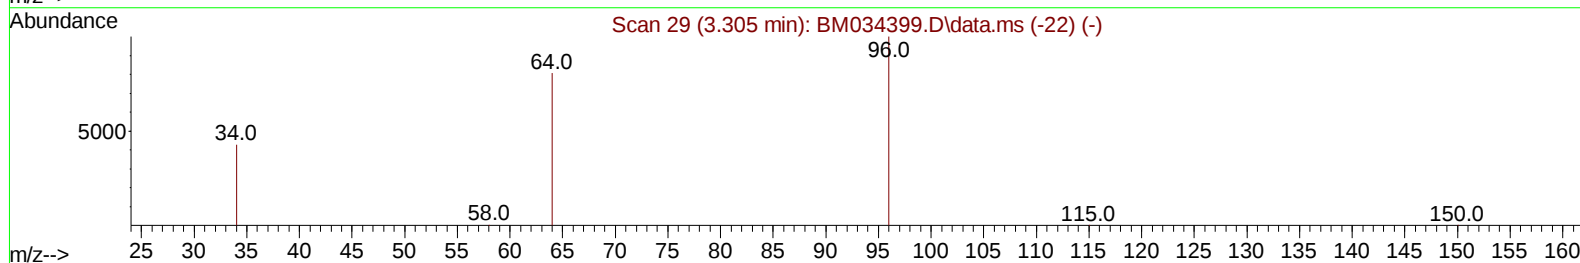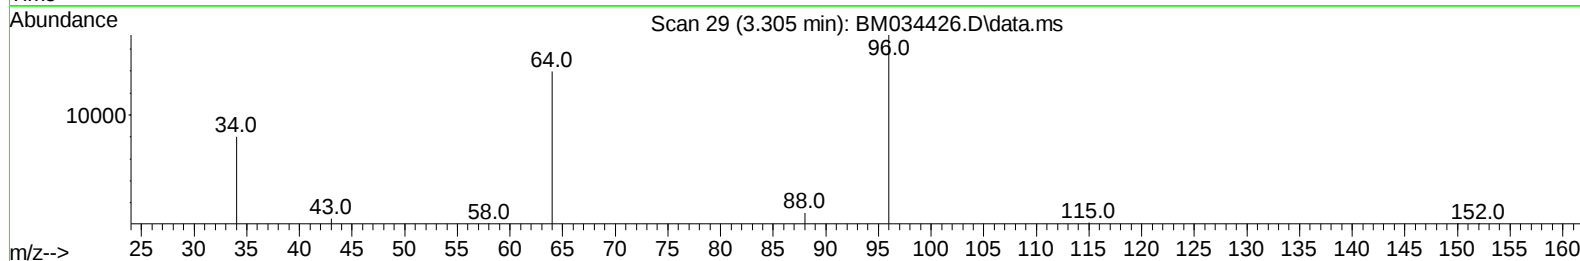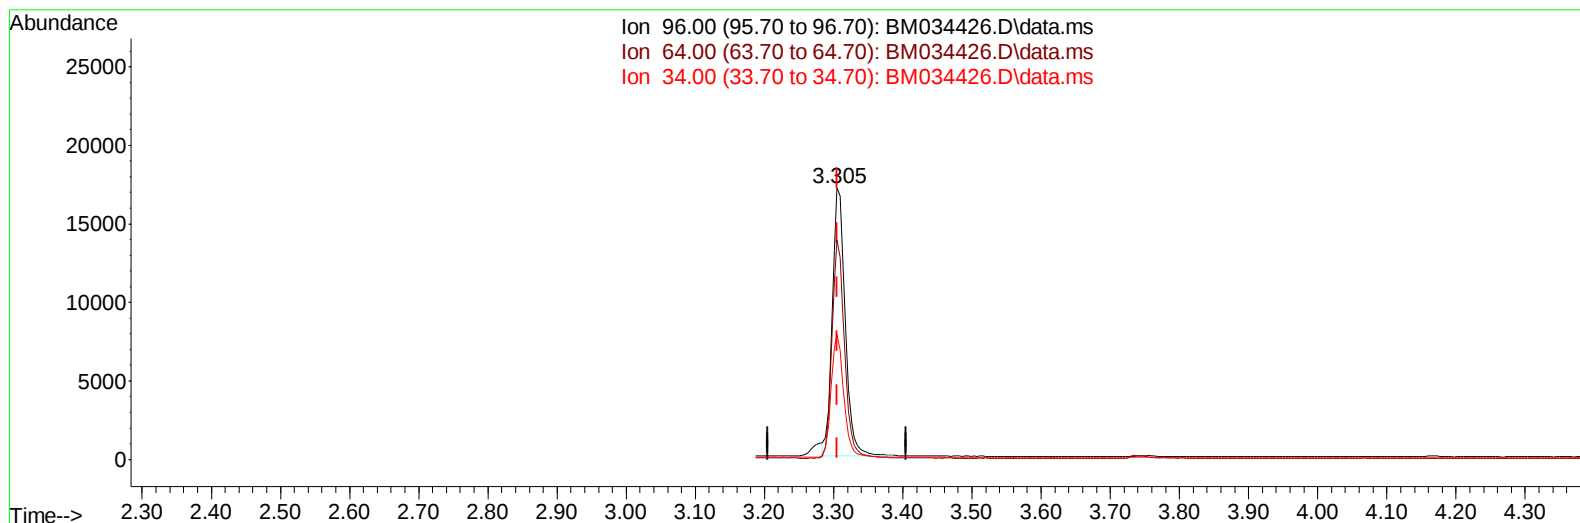

TIC: BM034426.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.305min (+ 0.000) 5.16 ng/ul m

response 22352

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	80.66
34.00	243.00	46.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034426.D
 Acq On : 30 Mar 2022 03:05
 Operator : CG/JU
 Sample : N2082-12
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW604

Manual IntegrationsAPPROVED

Quant Time: Mar 30 03:53:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

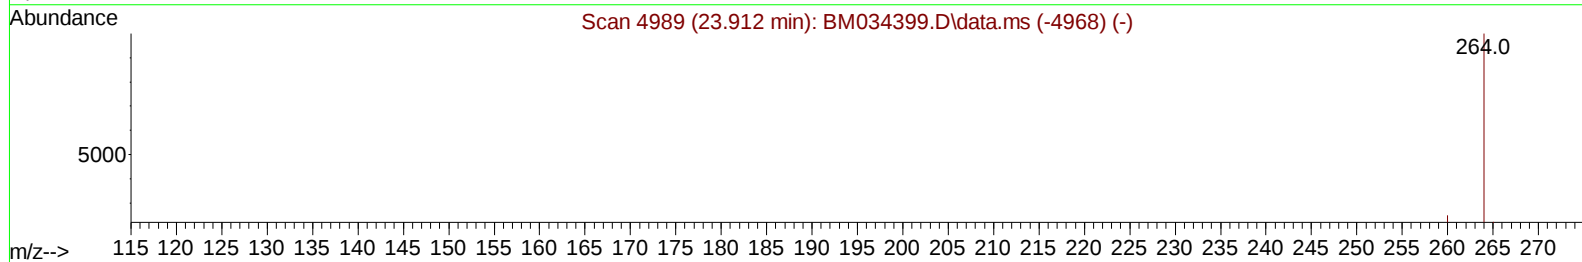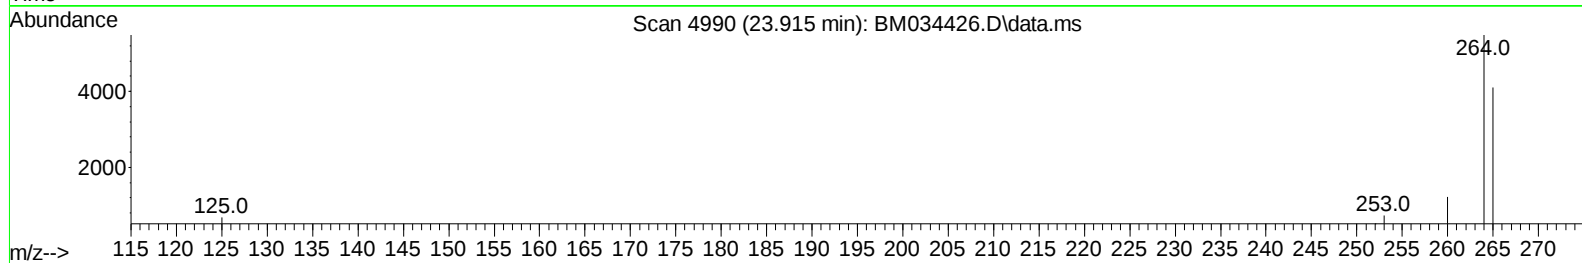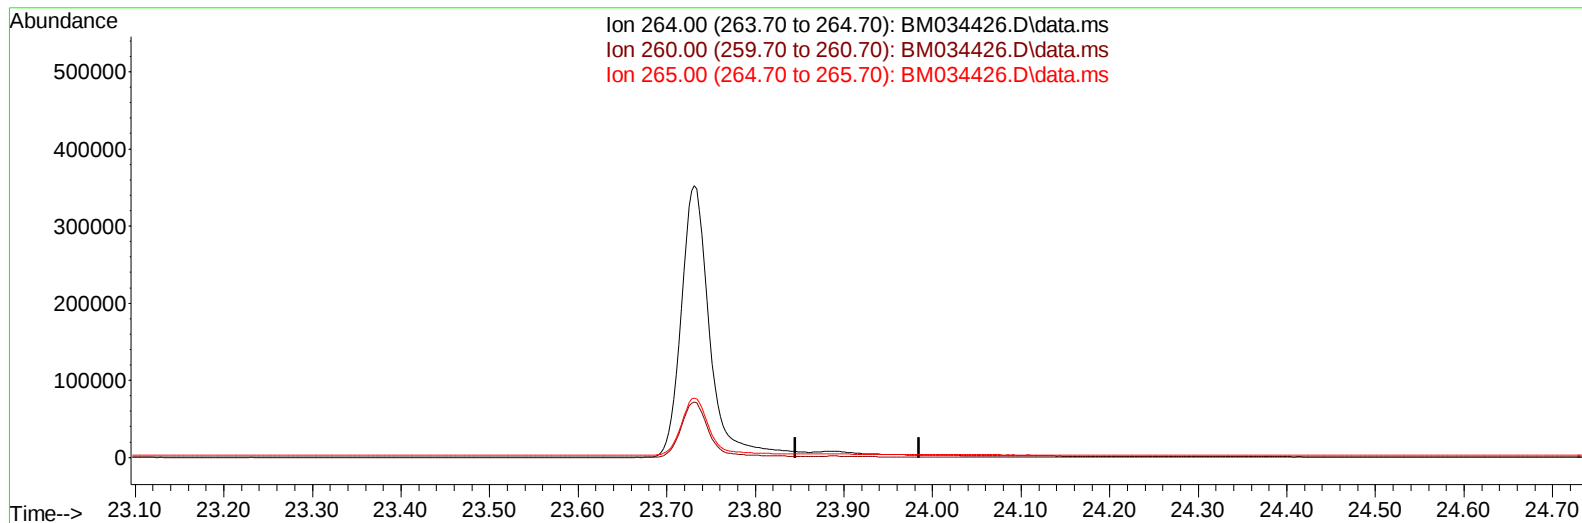

TIC: BM034426.D\data.ms

(23) Perylene-d12 (I)

23.915min (-23.915) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034426.D
 Acq On : 30 Mar 2022 03:05
 Operator : CG/JU
 Sample : N2082-12
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW604

Manual IntegrationsAPPROVED

Quant Time: Mar 30 03:53:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

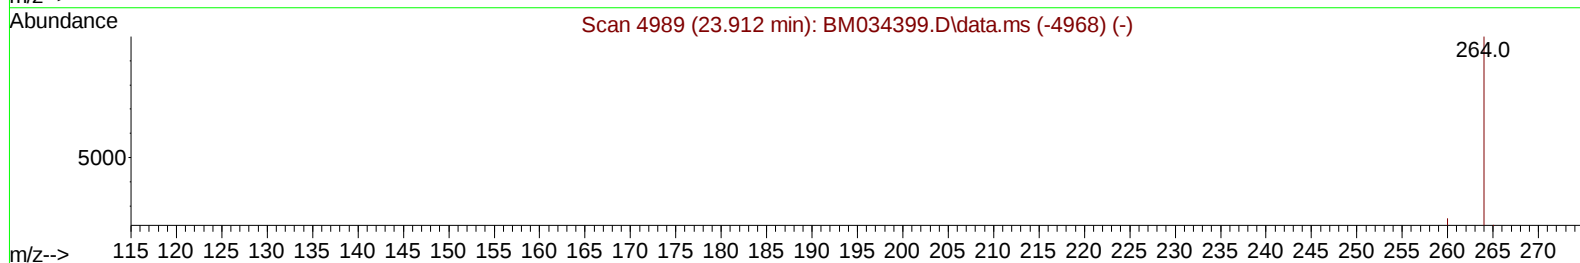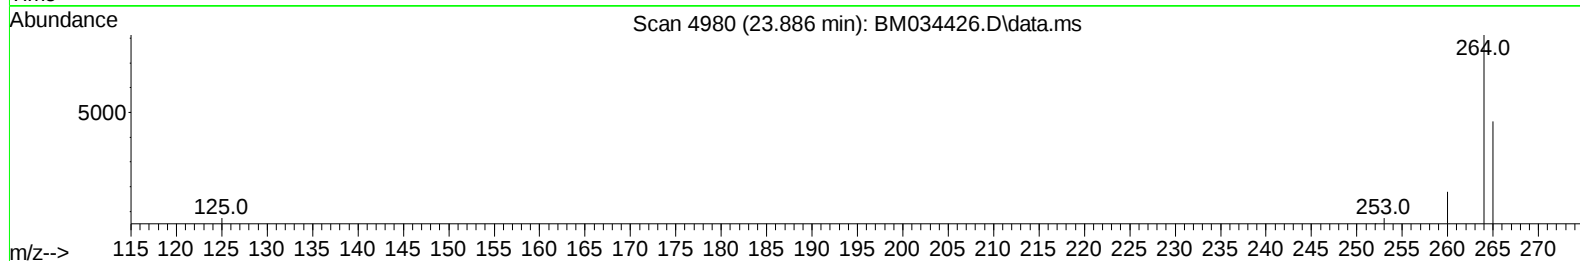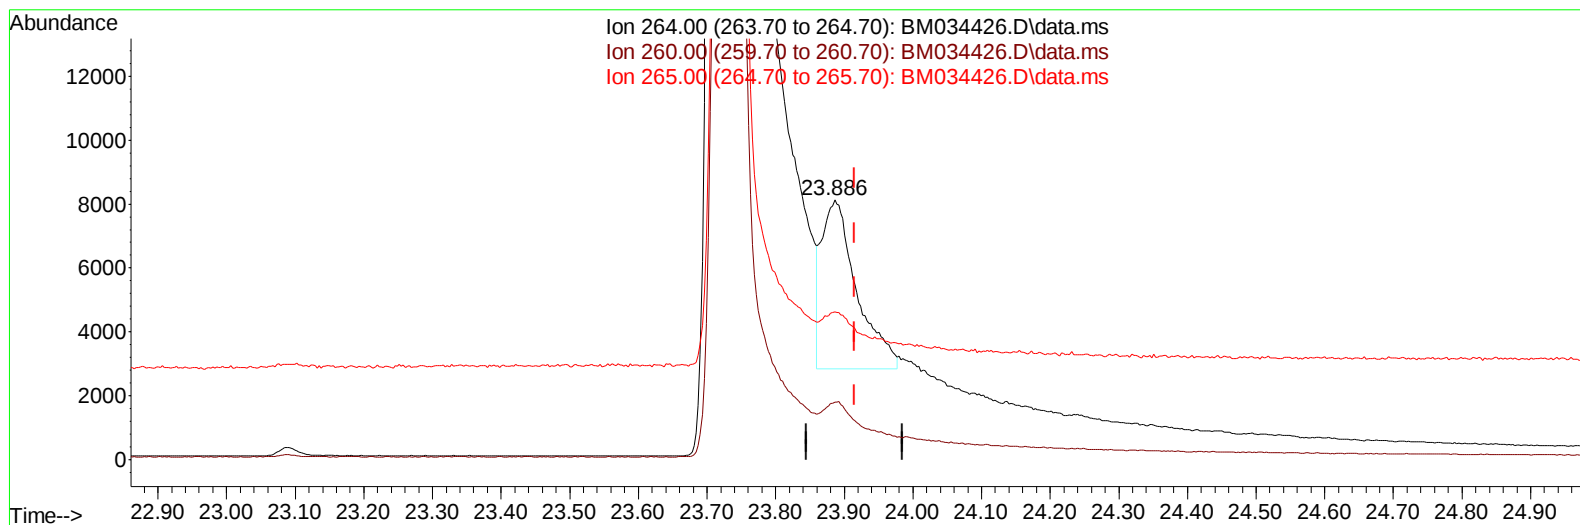

TIC: BM034426.D\data.ms

(23) Perylene-d12 (I)

23.886min (-0.029) 0.40 ng/ul m

response 18628

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	22.06#
265.00	95.30	56.98#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034426.D
 Acq On : 30 Mar 2022 03:05
 Operator : CG/JU
 Sample : N2082-12
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW604

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 03:53:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.929	152		2911	0.400	ng/ul	0.00
4) Naphthalene-d8	10.735	136		7484	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.569	164		4078	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.308	188		7550	0.400	ng/ul	-0.02
17) Chrysene-d12	21.495	240		5575	0.400	ng/ul	# 0.00
23) Perylene-d12	23.886	264		18628m	0.400	ng/ul	-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.305	96		22352m	5.162	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152		3727	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.334	212		8510	0.489	ng/ul	-0.01
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.343	88		2671	0.558	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034426.D
Acq On : 30 Mar 2022 03:05
Operator : CG/JU
Sample : N2082-12
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW604

Manual IntegrationsAPPROVED

Quant Time: Mar 30 03:53:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

