

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034441.D
 Acq On : 30 Mar 2022 15:23
 Operator : CG/JU
 Sample : PB143666BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 SBLK666

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:21:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

03/31/2022
 Supervised By :Yogesh
 Patel

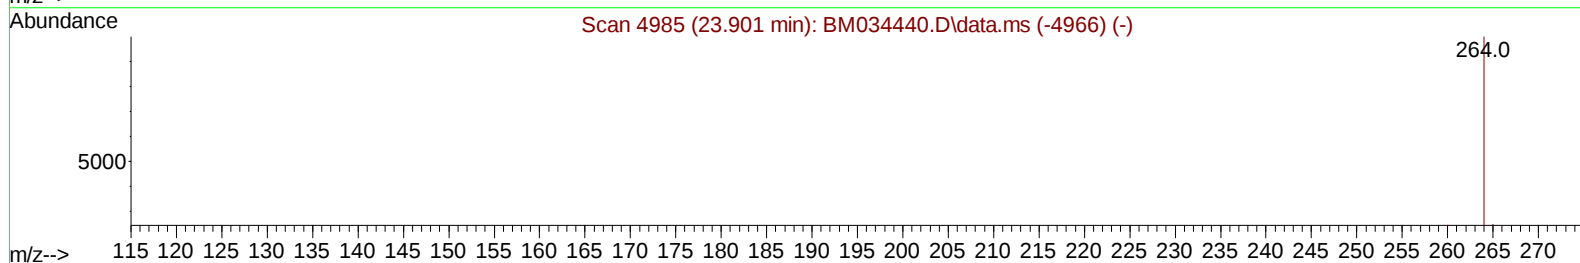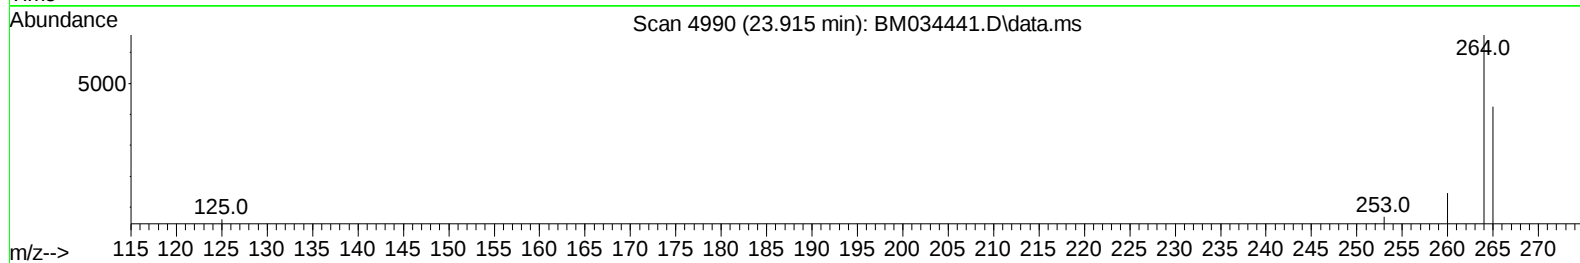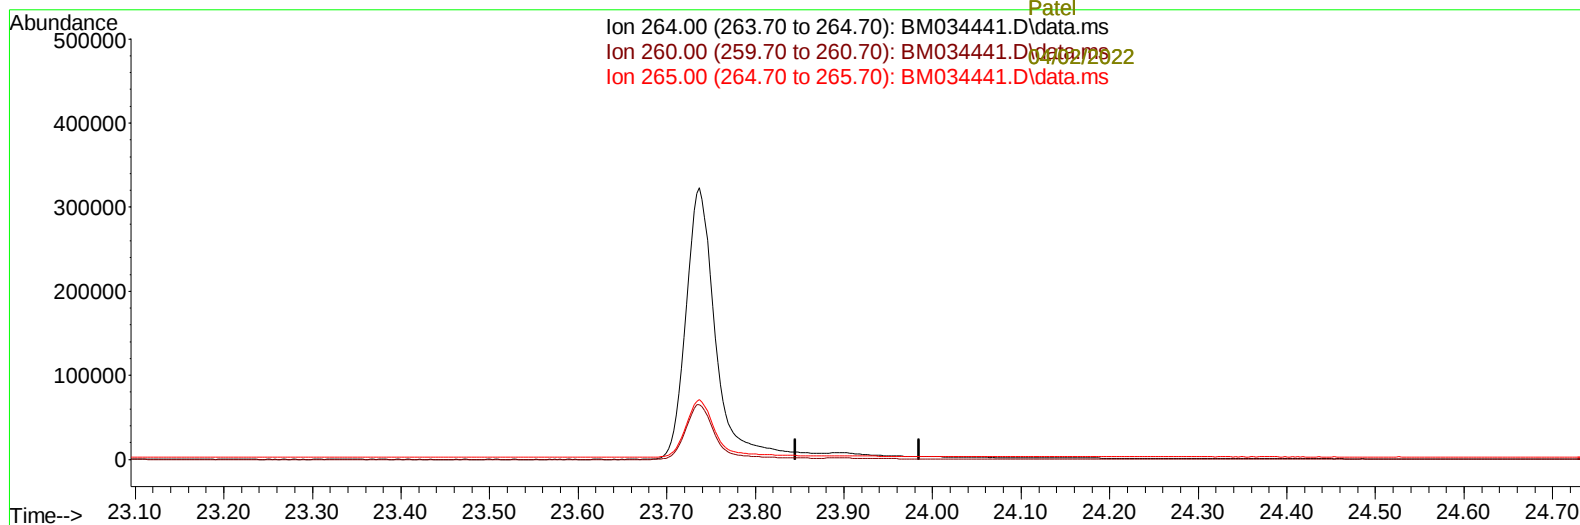

TIC: BM034441.D\data.ms

(23) Perylene-d12 (I)

23.915min (-23.915) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034441.D
 Acq On : 30 Mar 2022 15:23
 Operator : CG/JU
 Sample : PB143666BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 SBLK666

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:21:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

03/31/2022
 Supervised By :Yogesh
 Patel

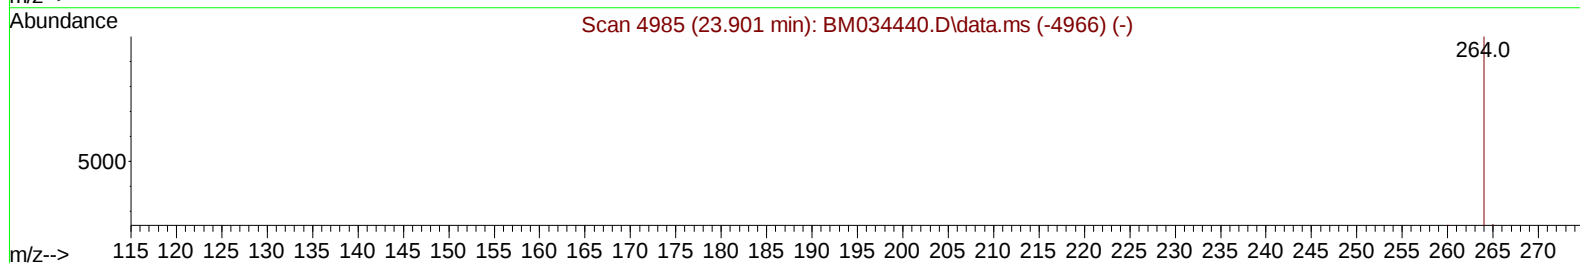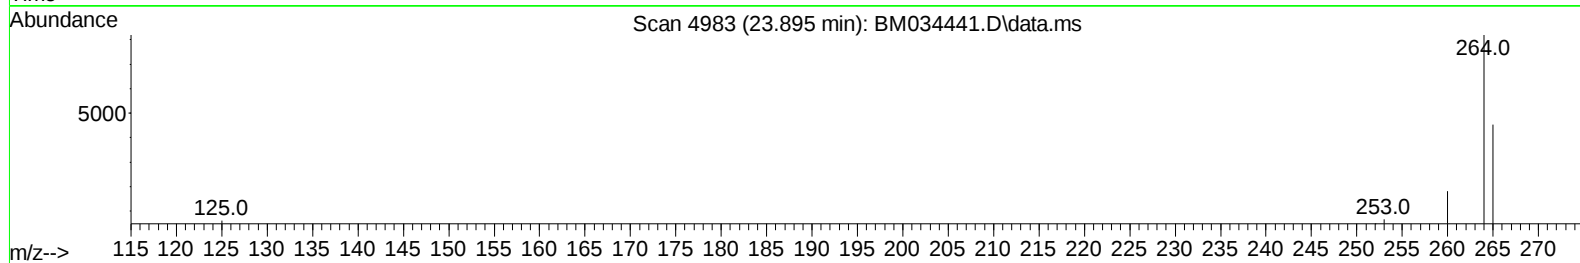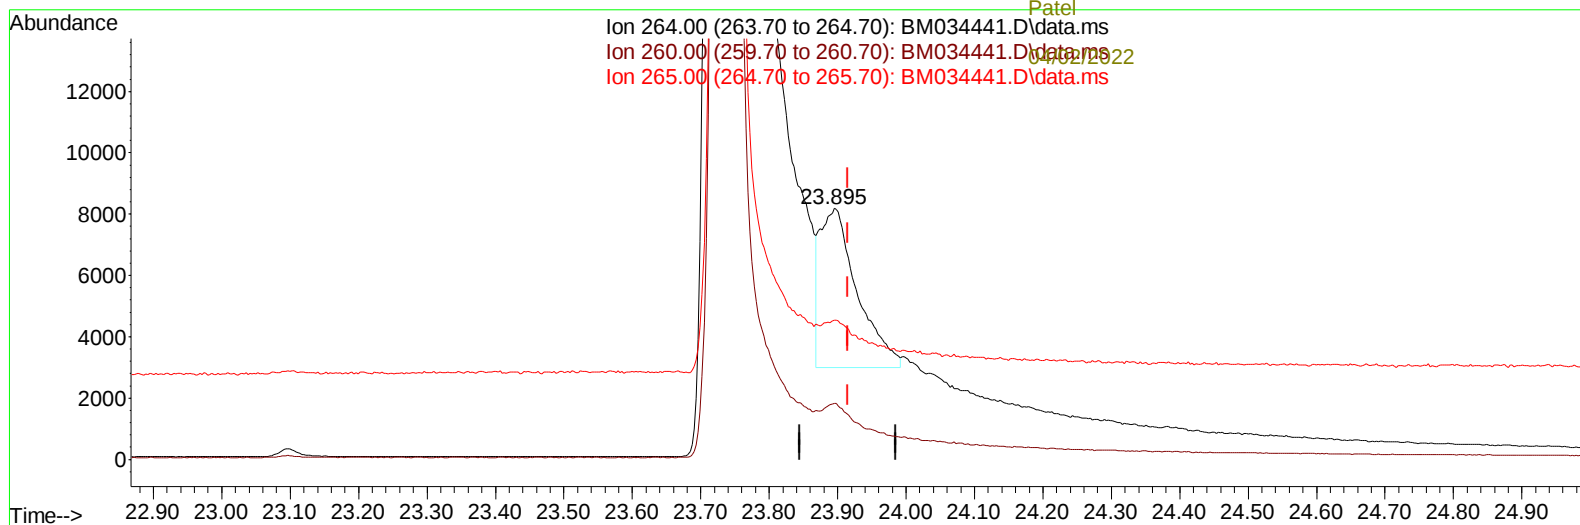

TIC: BM034441.D\data.ms

(23) Perylene-d12 (I)

23.895min (-0.020) 0.40 ng/ul m

response 19400

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	22.23#
265.00	95.30	55.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034441.D
 Acq On : 30 Mar 2022 15:23
 Operator : CG/JU
 Sample : PB143666BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK666

Manual IntegrationsAPPROVED

Reviewed By :Jagrut
 Upadhyay

03/31/2022
 Supervised By :Yogesh
 Patel

Quant Time: Mar 31 02:21:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/02/2022						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	3478	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.735	136	9238	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.569	164	5153	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.308	188	9429	0.400	ng/ul	-0.02
17) Chrysene-d12	21.507	240	5951	0.400	ng/ul	# 0.00
23) Perylene-d12	23.895	264	19400m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	32109	6.206	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	4931	0.396	ng/ul	0.00
18) Fluoranthene-d10	19.339	212	8923	0.481	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034441.D
Acq On : 30 Mar 2022 15:23
Operator : CG/JU
Sample : PB143666BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK666

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:21:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

03/31/2022
Supervised By :Yogesh
Patel

04/02/2022

