




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034459.D
 Acq On : 31 Mar 2022 02:48
 Operator : CG/JU
 Sample : N2097-20
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 03:23:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

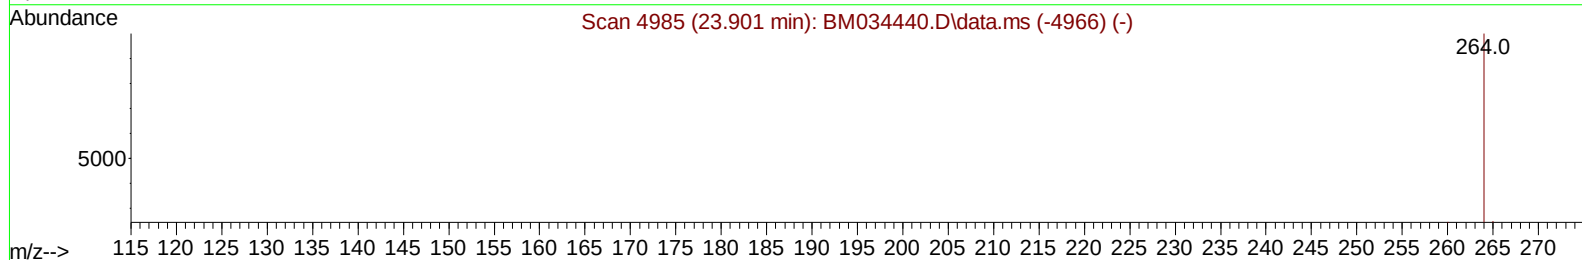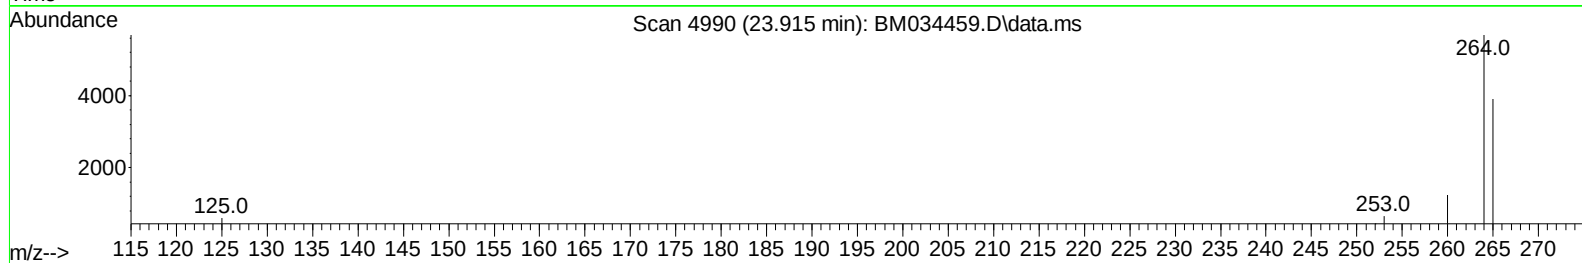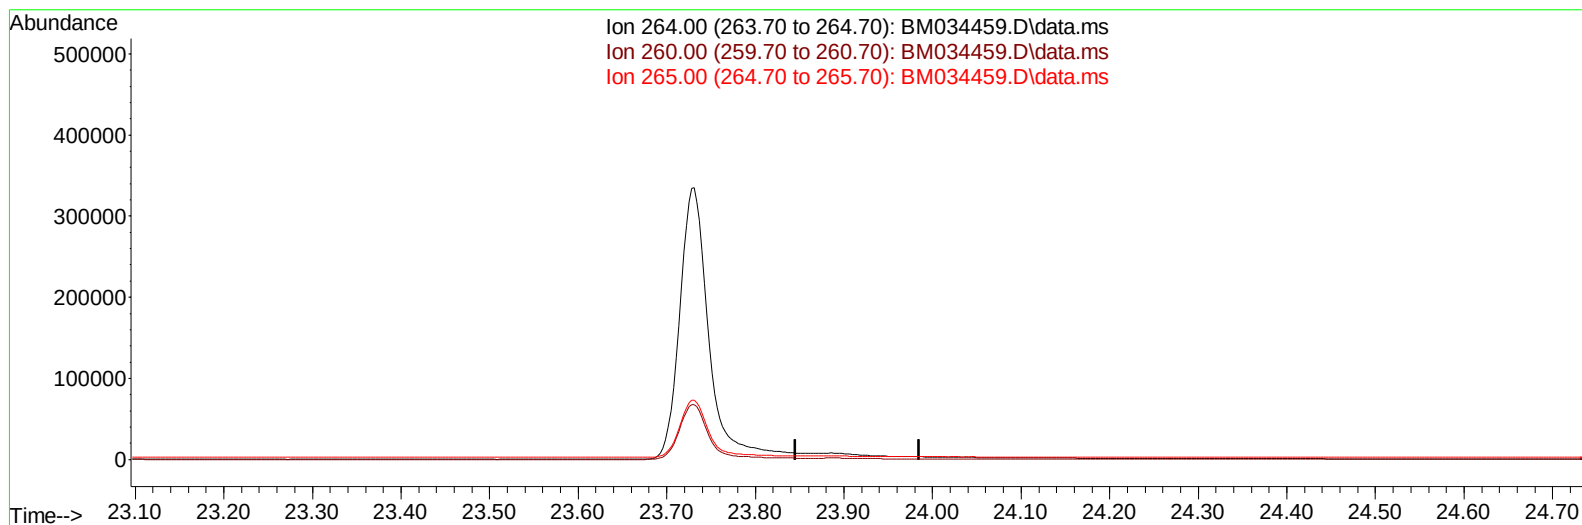

TIC: BM034459.D\data.ms

(23) Perylene-d12 (I)

23.915min (-23.915) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034459.D
 Acq On : 31 Mar 2022 02:48
 Operator : CG/JU
 Sample : N2097-20
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 03:23:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

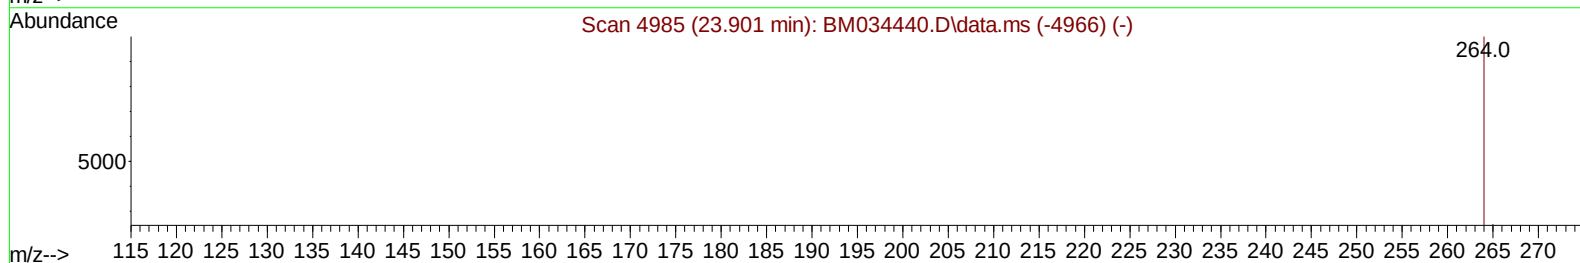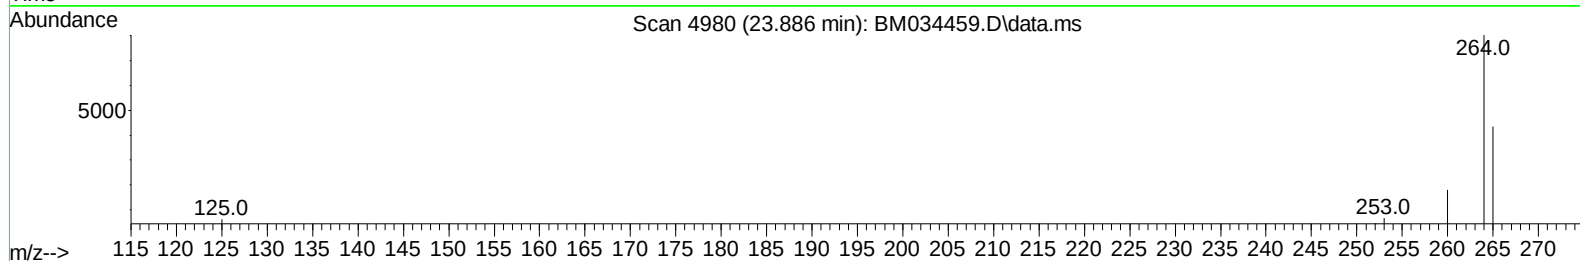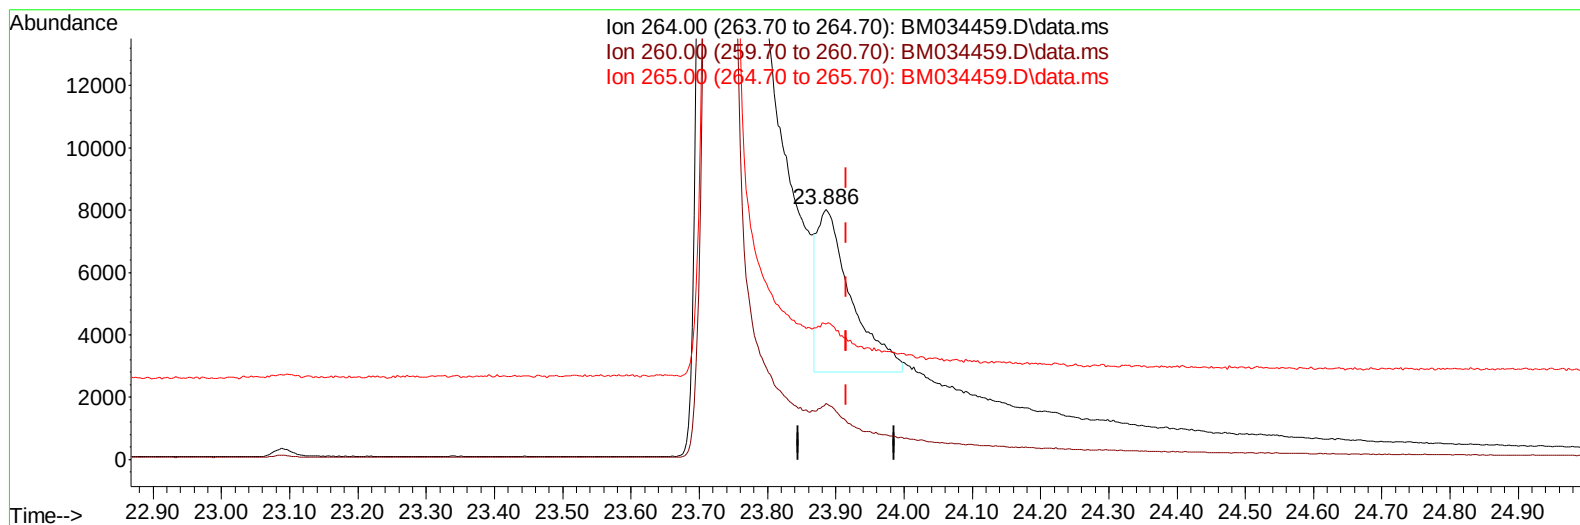

TIC: BM034459.D\data.ms

(23) Perylene-d12 (I)

23.886min (-0.029) 0.40 ng/ul m

response 18127

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	22.39
265.00	95.30	54.17#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034459.D
 Acq On : 31 Mar 2022 02:48
 Operator : CG/JU
 Sample : N2097-20
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 31 03:23:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.925	152		2582	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.729	136		7027	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.564	164		3935	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.307	188		7509	0.400	ng/ul	-0.02
17) Chrysene-d12	21.498	240		5352	0.400	ng/ul	# 0.00
23) Perylene-d12	23.886	264		18127m	0.400	ng/ul	-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.301	96		20170	5.252	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152		3579	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.334	212		8480	0.508	ng/ul	-0.01
Target Compounds							
2) 1,4-Dioxane	3.338	88		2211	0.521	ng/ul#	Qvalue 73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034459.D
Acq On : 31 Mar 2022 02:48
Operator : CG/JU
Sample : N2097-20
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 03:23:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

