

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034412.D
 Acq On : 29 Mar 2022 18:05
 Operator : CG/JU
 Sample : N2079-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Z7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 02:31:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	2500	0.400	ng/ul	0.00
4) Naphthalene-d8	10.741	136	6848	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.574	164	3745	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.312	188	7033	0.400	ng/ul	-0.01
17) Chrysene-d12	21.504	240	5023	0.400	ng/ul	# 0.00
23) Perylene-d12	23.901	264	15158m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	14687	3.949	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	2432	0.263	ng/ul	0.02
18) Fluoranthene-d10	19.343	212	5537	0.353	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.339	88	3424	0.834	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034412.D
Acq On : 29 Mar 2022 18:05
Operator : CG/JU
Sample : N2079-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW5Z7


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 02:31:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

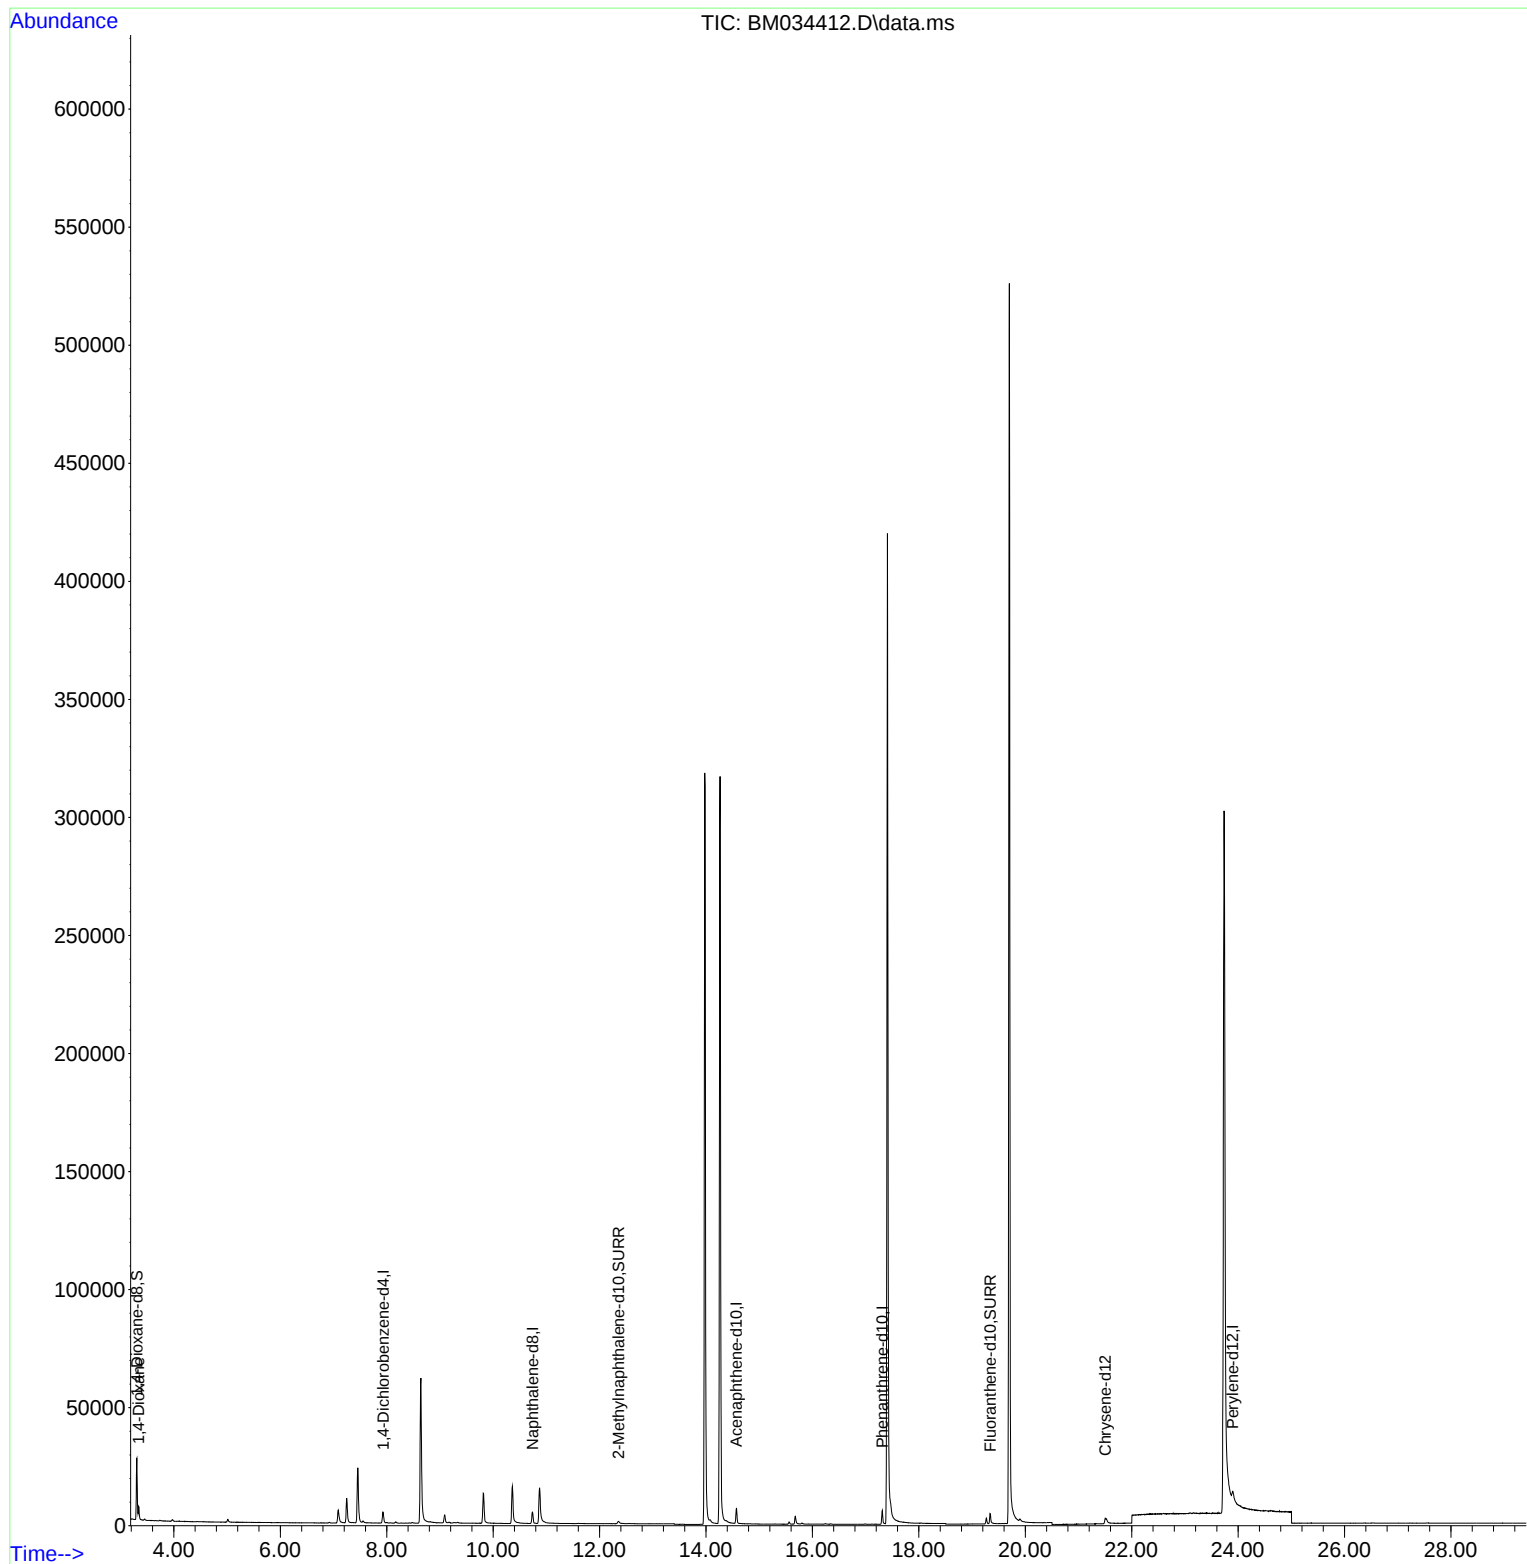


Abundance Scan 38 (3.343 min): BM034399.D\data.ms (-31)

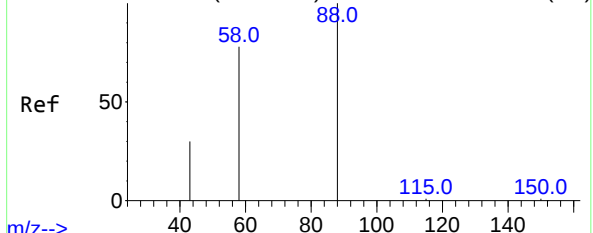


m/z-->

Abundance Scan 37 (3.339 min): BM034412.D\data.ms

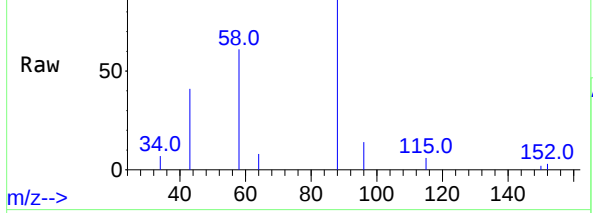

m/z-->

Abundance Scan 37 (3.339 min): BM034412.D\data.ms (-26)

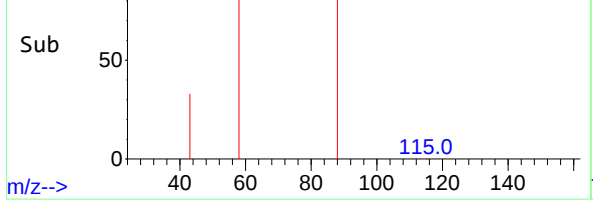

m/z-->

#2
1,4-Dioxane
Concen: 0.834 ng/ul
RT: 3.339 min Scan# 31
Delta R.T. -0.004 min
Lab File: BM034412.D
Acq: 29 Mar 2022 18:05

Instrument :
BNA_M
ClientSampleId :
EW5Z7

Tgt Ion: 88	Resp: 3424
Ion Ratio	Lower Upper
88	100
43	40.9 49.7 74.5
58	61.2 52.5 78.7

Manual Integrations
APPROVED
Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

