

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034423.D
 Acq On : 30 Mar 2022 01:17
 Operator : CG/JU
 Sample : N2079-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Y6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 02:33:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	2654	0.400	ng/ul	0.00
4) Naphthalene-d8	10.735	136	6962	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.569	164	3844	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.307	188	7166	0.400	ng/ul	-0.02
17) Chrysene-d12	21.498	240	5269	0.400	ng/ul	# 0.00
23) Perylene-d12	23.889	264	14188m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.309	96	18824	4.768	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	3640	0.388	ng/ul	0.01
18) Fluoranthene-d10	19.338	212	8966	0.545	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.343	88	5343	1.225	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034423.D
Acq On : 30 Mar 2022 01:17
Operator : CG/JU
Sample : N2079-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW5Y6


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 02:33:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

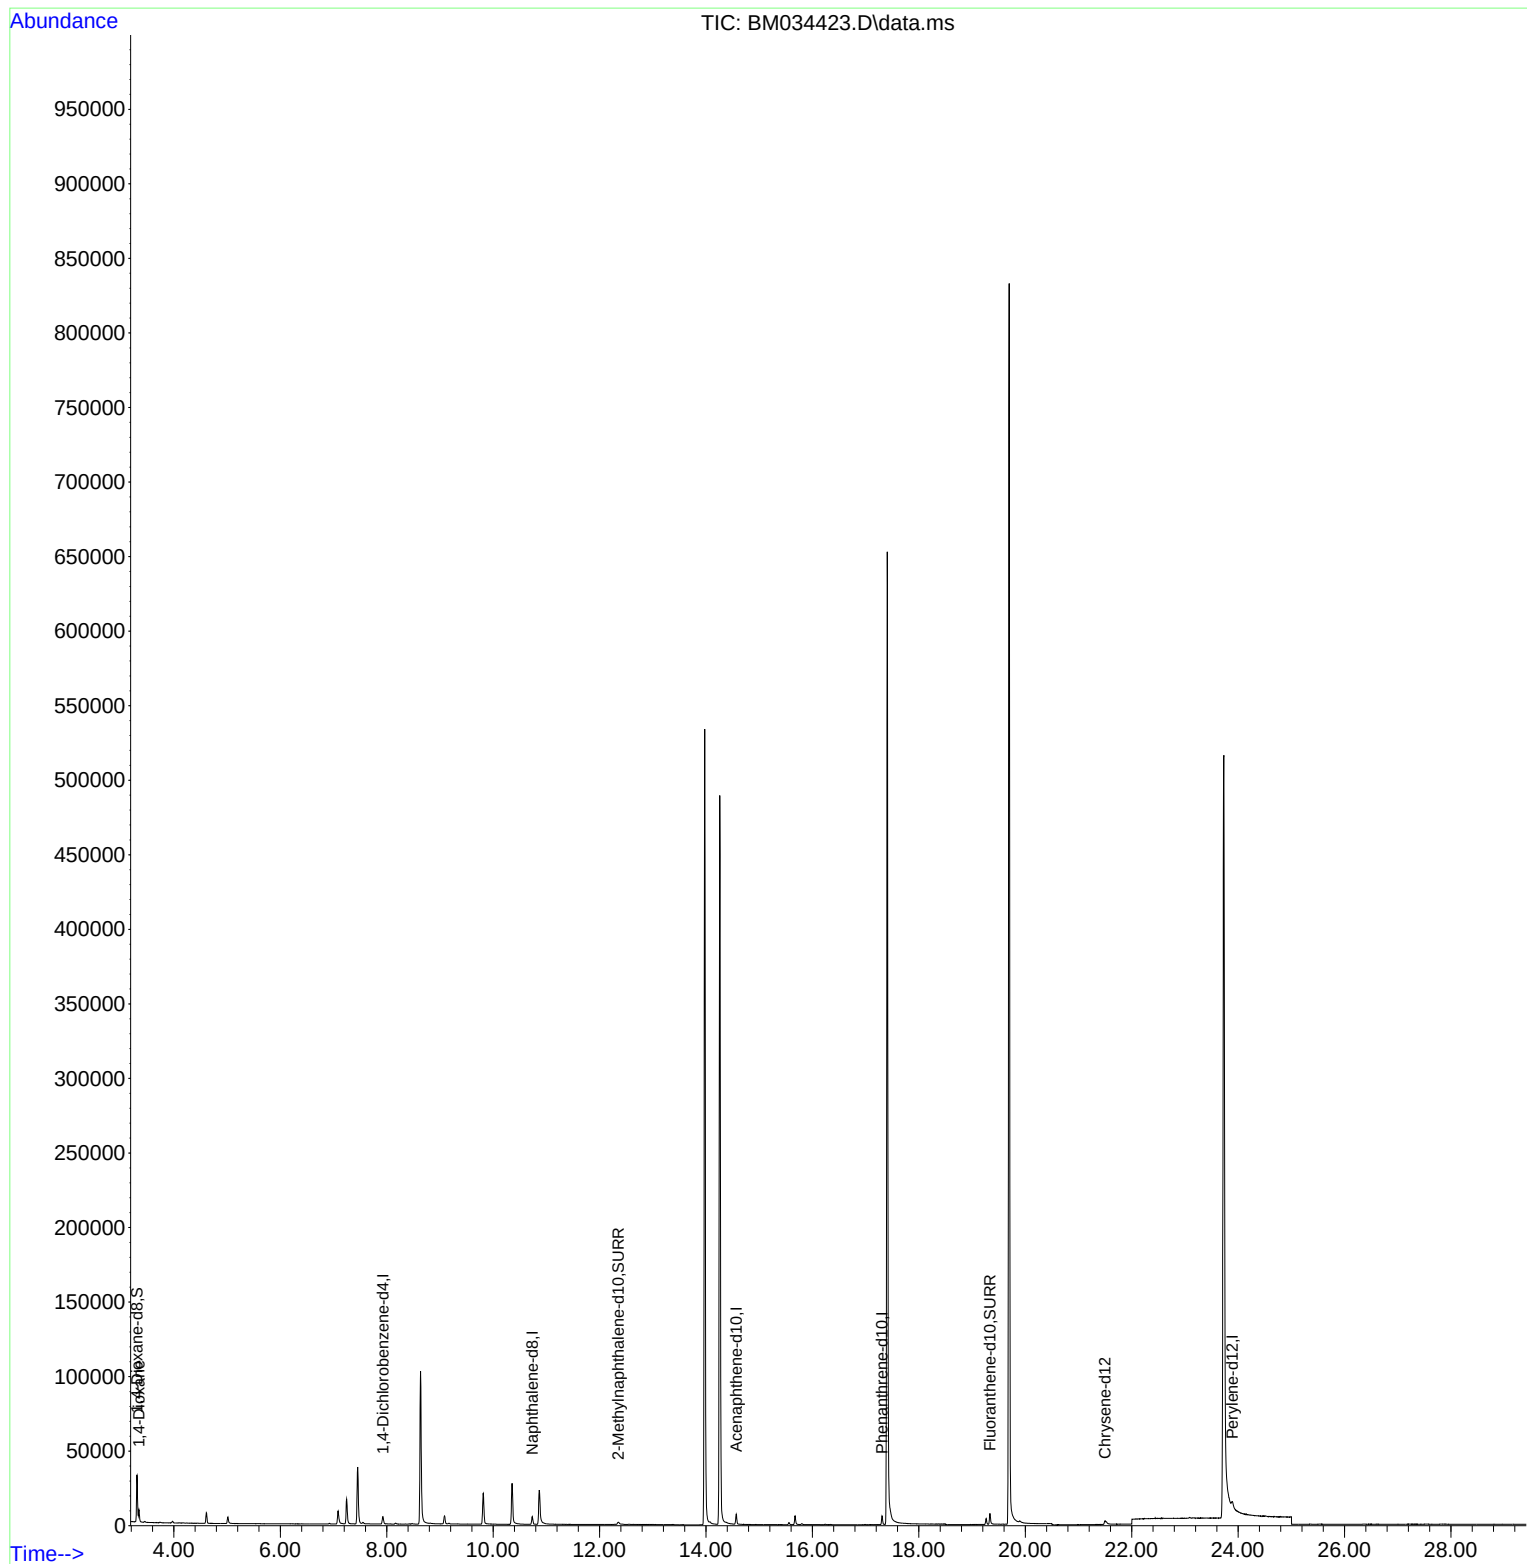


Abundance Scan 38 (3.343 min): BM034416.D\data.ms (-32)

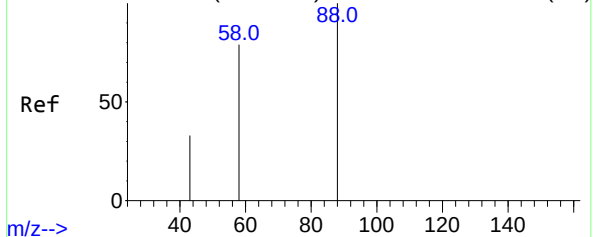

#2
1,4-Dioxane
Concen: 1.225 ng/ul
RT: 3.343 min Scan# 30
Delta R.T. -0.000 min
Lab File: BM034423.D
Acq: 30 Mar 2022 01:17

Instrument :
BNA_M
ClientSampleId :
EW5Y6

Abundance Scan 38 (3.343 min): BM034423.D\data.ms

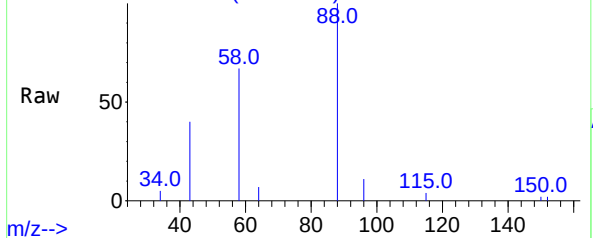

Tgt Ion: 88 Resp: 534
Ion Ratio Lower Upper
88 100
43 40.2 49.7 74.5
58 66.7 52.5 78.7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

Abundance Scan 38 (3.343 min): BM034423.D\data.ms (-26)

