

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034426.D
 Acq On : 30 Mar 2022 03:05
 Operator : CG/JU
 Sample : N2082-12
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW604

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 03:53:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	2911	0.400	ng/u1	0.00
4) Naphthalene-d8	10.735	136	7484	0.400	ng/u1	#-0.02
9) Acenaphthene-d10	14.569	164	4078	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.308	188	7550	0.400	ng/u1	-0.02
17) Chrysene-d12	21.495	240	5575	0.400	ng/u1	# 0.00
23) Perylene-d12	23.886	264	18628m	0.400	ng/u1	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	22352m	5.162	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.346	152	3727	0.369	ng/u1	0.00
18) Fluoranthene-d10	19.334	212	8510	0.489	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.343	88	2671	0.558	ng/u1#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034426.D
Acq On : 30 Mar 2022 03:05
Operator : CG/JU
Sample : N2082-12
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW604


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 03:53:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

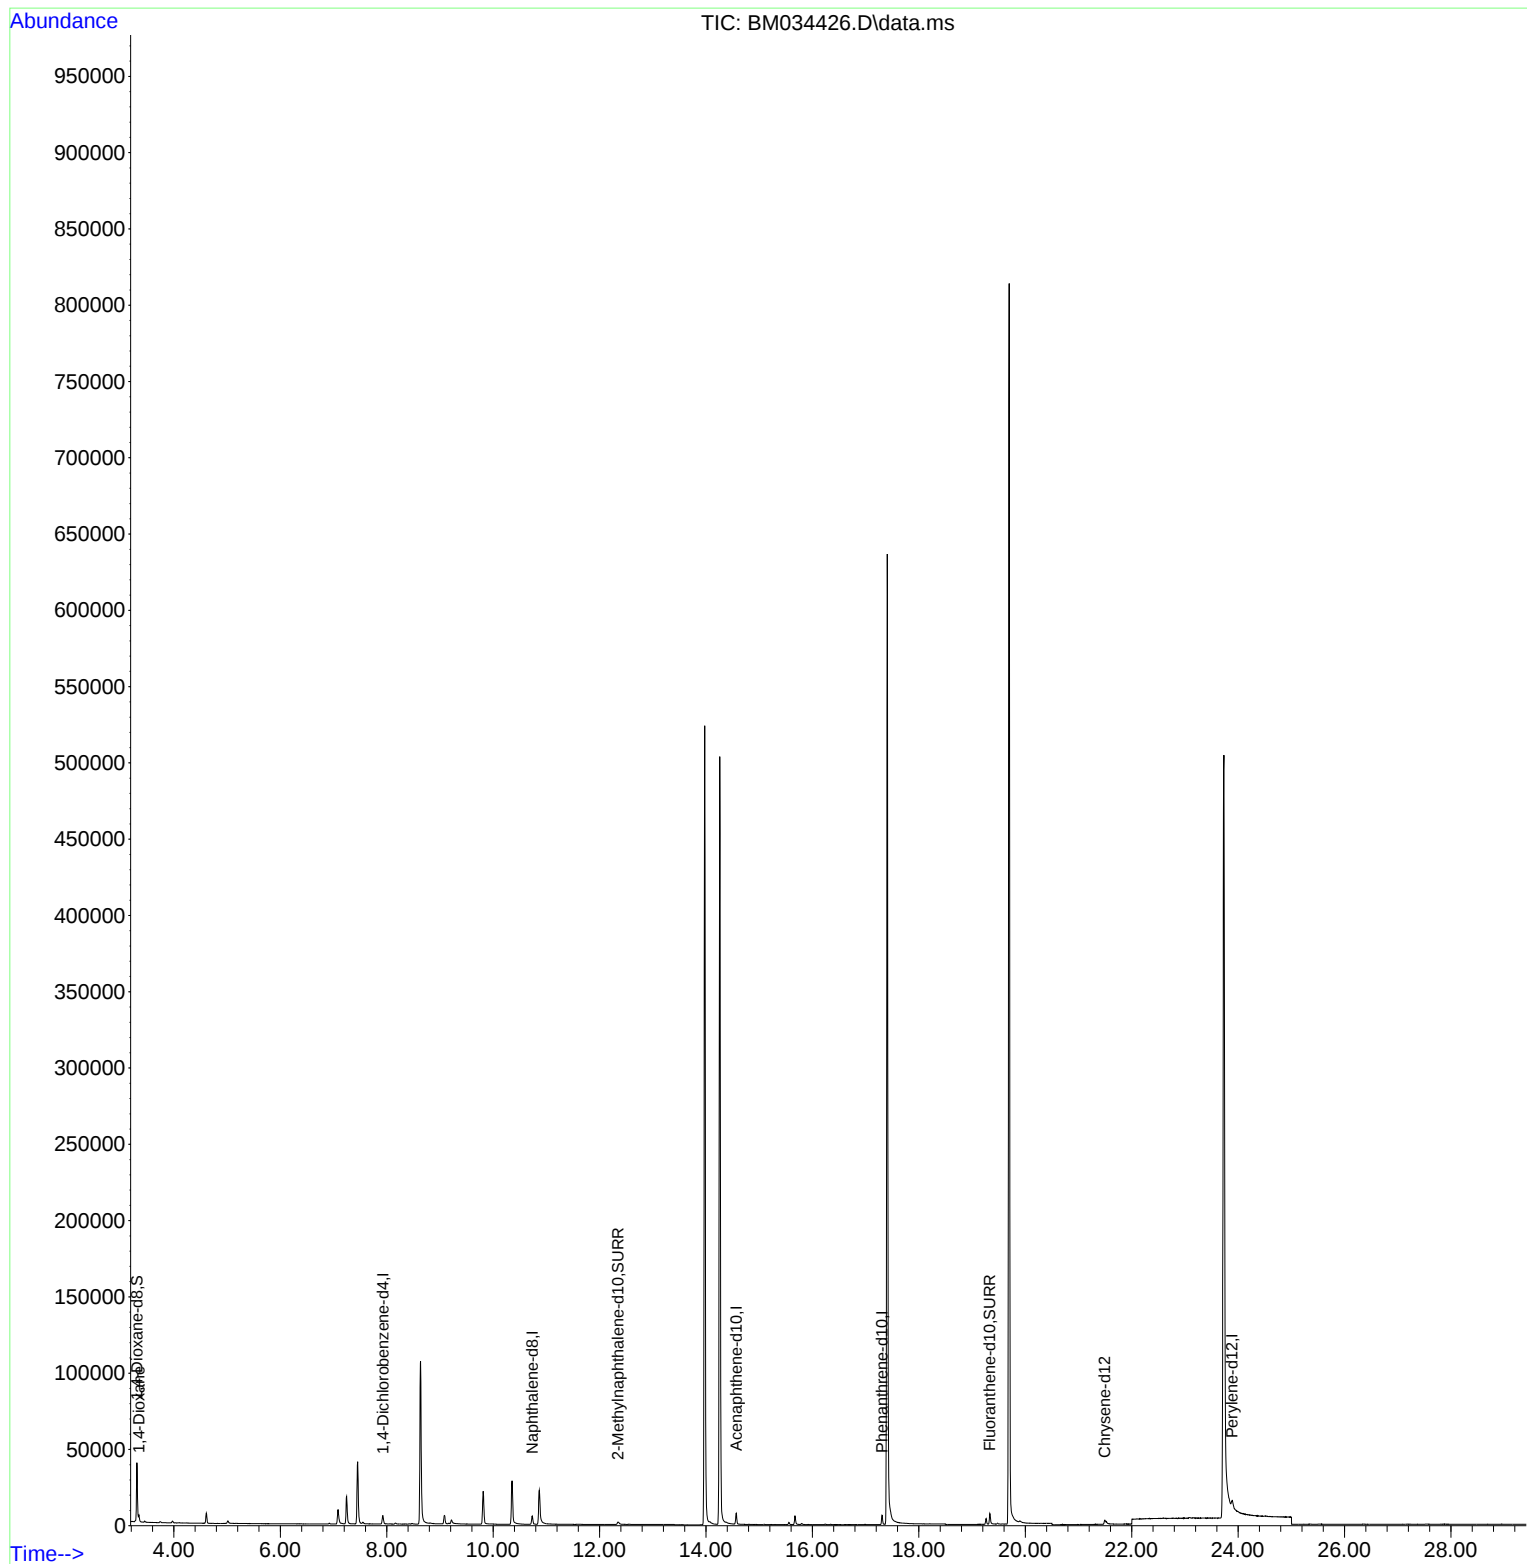


Abundance Scan 38 (3.343 min): BM034416.D\data.ms (-32)

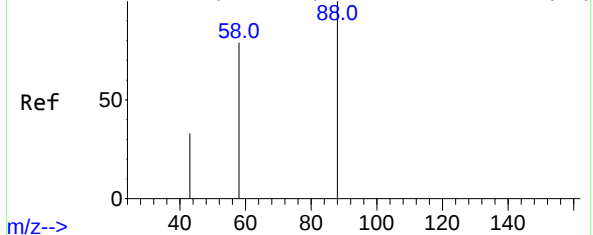

#2
1,4-Dioxane
Concen: 0.558 ng/ul
RT: 3.343 min Scan# 31
Delta R.T. 0.000 min
Lab File: BM034426.D
Acq: 30 Mar 2022 03:05

Instrument :
BNA_M
ClientSampleId :
EW604

Abundance Scan 38 (3.343 min): BM034426.D\data.ms

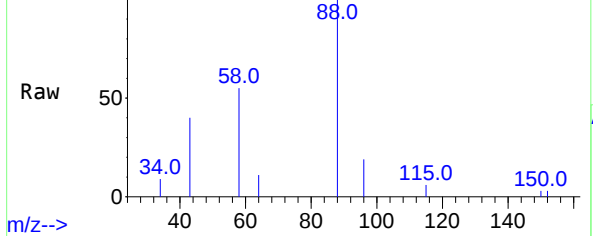

Tgt Ion: 88 Resp: 267
Ion Ratio Lower Upper
88 100
43 39.9 49.7 74.5
58 54.7 52.5 78.7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

Abundance Scan 38 (3.343 min): BM034426.D\data.ms (-26)

