

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034436.D
 Acq On : 30 Mar 2022 09:38
 Operator : CG/JU
 Sample : N2082-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW605

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 31 02:19:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	2913	0.400	ng/ul	0.00
4) Naphthalene-d8	10.735	136	7608	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.569	164	4082	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.308	188	7691	0.400	ng/ul	-0.02
17) Chrysene-d12	21.501	240	5310	0.400	ng/ul	# 0.00
23) Perylene-d12	23.886	264	17945m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	18445m	4.257	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	2984	0.291	ng/ul	0.01
18) Fluoranthene-d10	19.334	212	7371	0.445	ng/ul	-0.01
Target Compounds						
19) Fluoranthene	19.362	202	600	0.025	ng/ul#	Qvalue 56

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034436.D
Acq On : 30 Mar 2022 09:38
Operator : CG/JU
Sample : N2082-13
Misc :
ALS Vial : 40 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW605

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022


Quant Time: Mar 31 02:19:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

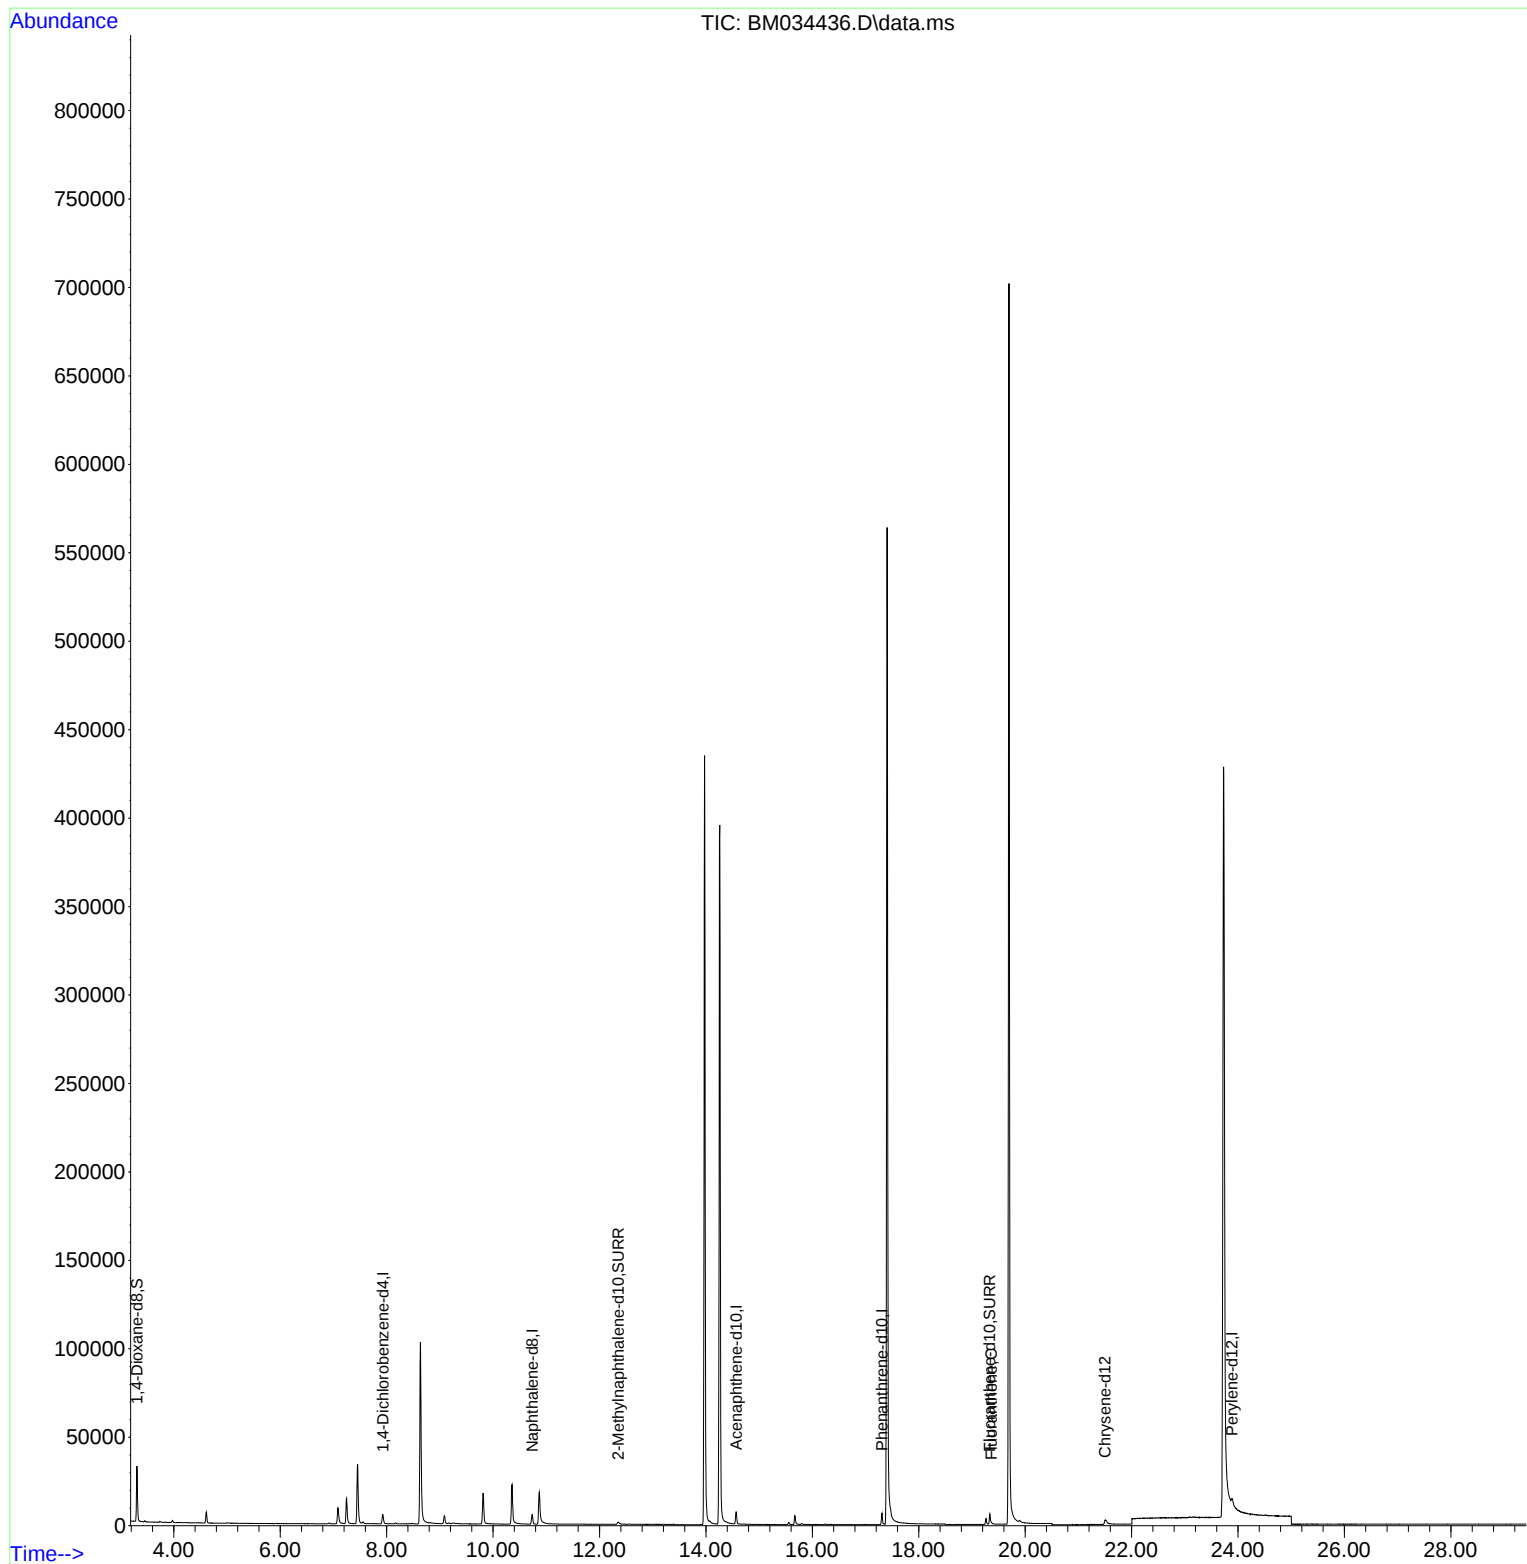

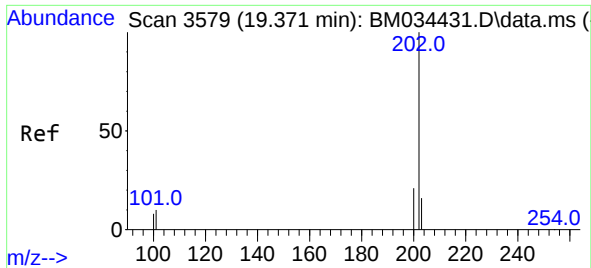

#19
Fluoranthene
Concen: 0.025 ng/ul
RT: 19.362 min Scan# 3577
Delta R.T. -0.014 min
Lab File: BM034436.D
Acq: 30 Mar 2022 09:38

Instrument :
BNA_M
ClientSampleId :
EW605

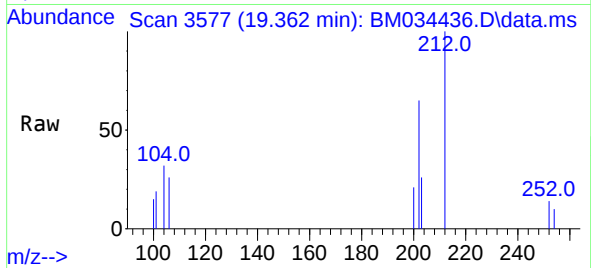

Tgt Ion:	202	Resp:	600
Ion	Ratio	Lower	Upper
202	100		
101	29.4	9.2	13.8
100	23.6	7.2	10.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

