

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034457.D
 Acq On : 31 Mar 2022 01:36
 Operator : CG/JU
 Sample : N2097-15
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 31 02:23:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	3138	0.400	ng/u1	-0.01
4) Naphthalene-d8	10.729	136	8399	0.400	ng/u1	#-0.02
9) Acenaphthene-d10	14.564	164	4541	0.400	ng/u1	-0.01
13) Phenanthrene-d10	17.303	188	8733	0.400	ng/u1	-0.02
17) Chrysene-d12	21.495	240	6384	0.400	ng/u1	# 0.00
23) Perylene-d12	23.889	264	20292m	0.400	ng/u1	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	18354	3.932	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.352	152	3300	0.291	ng/u1	0.01
18) Fluoranthene-d10	19.334	212	7941	0.399	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.338	88	992	0.192	ng/u1#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034457.D
Acq On : 31 Mar 2022 01:36
Operator : CG/JU
Sample : N2097-15
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE4


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 31 02:23:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

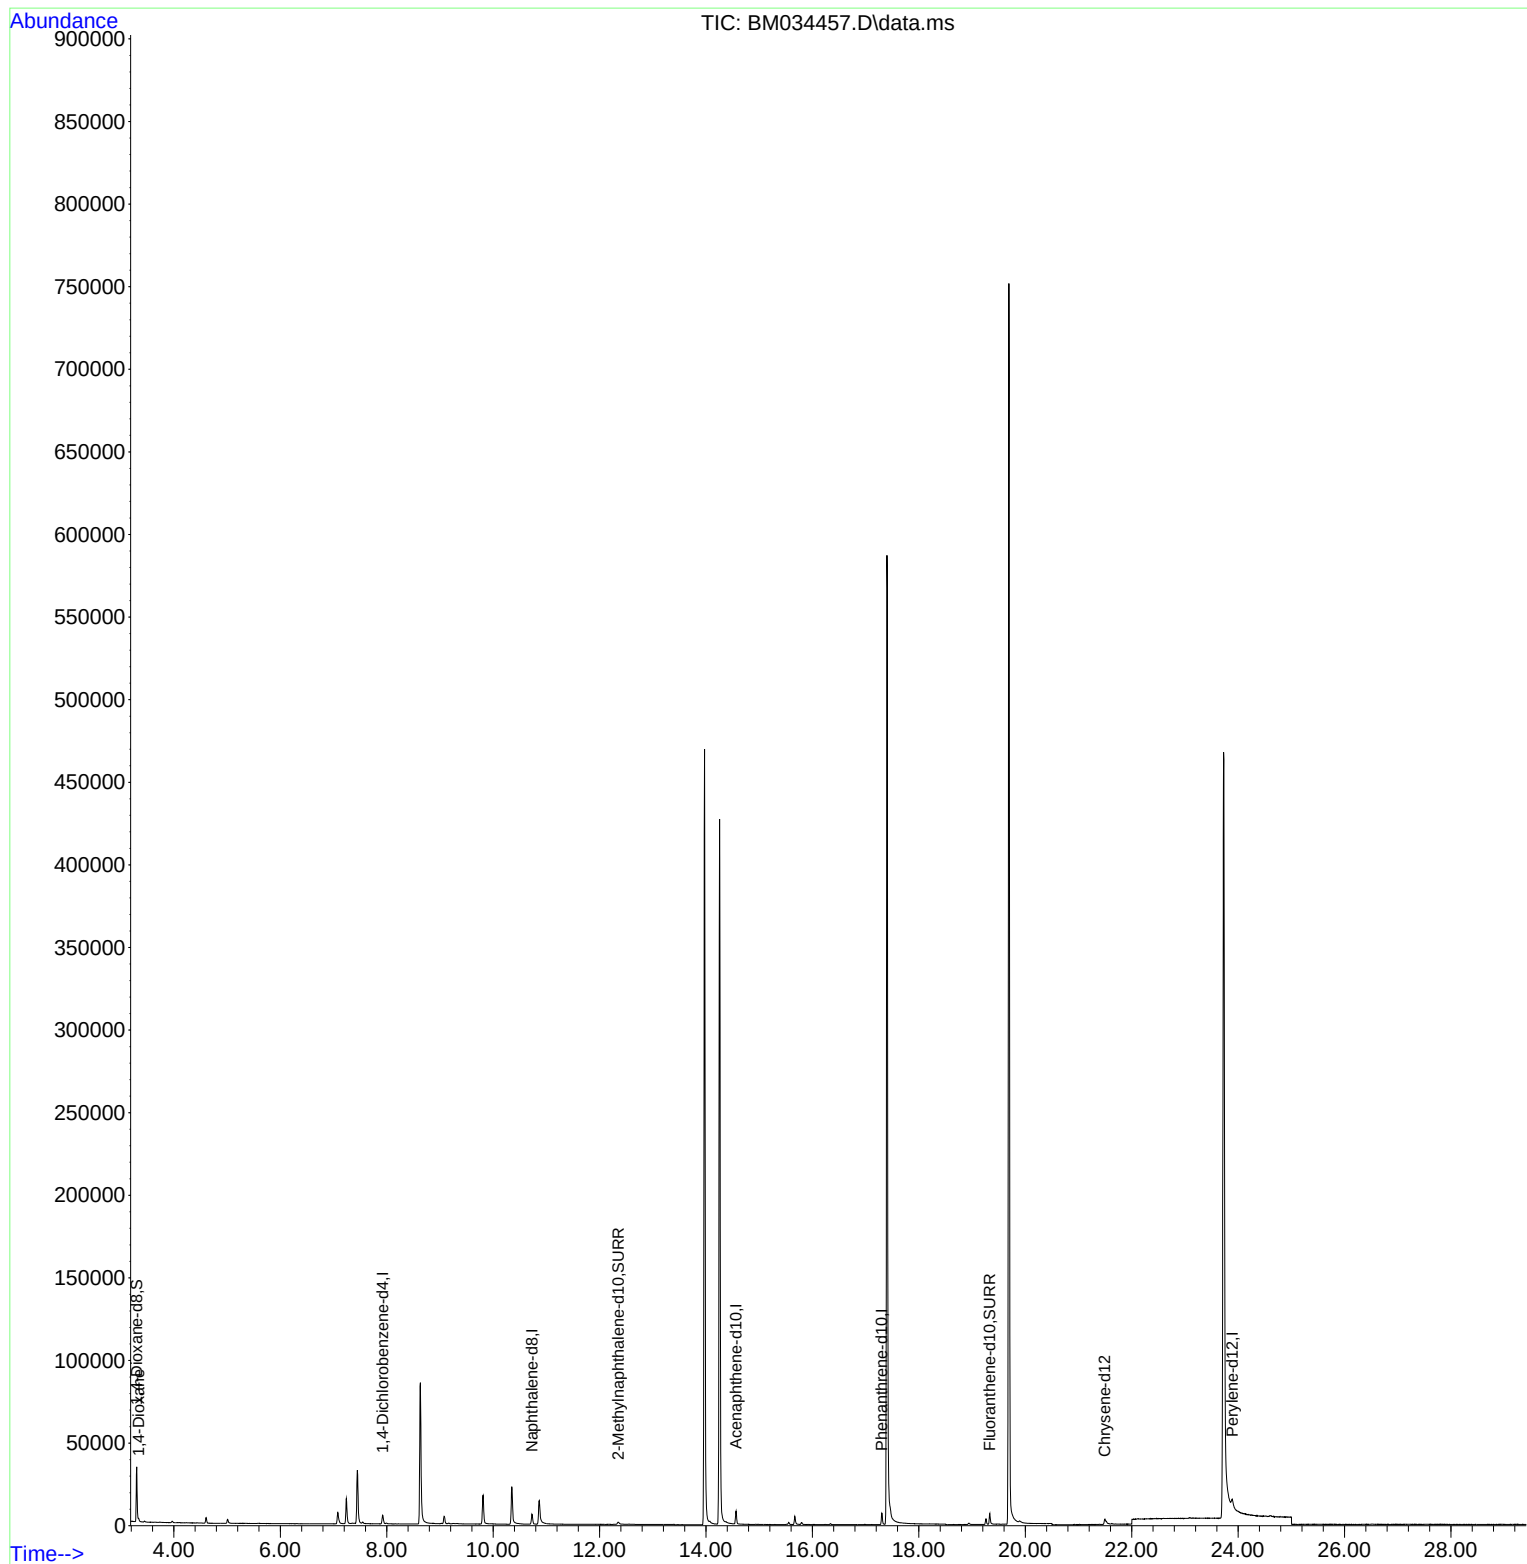


Abundance Scan 37 (3.338 min): BM034453.D\data.ms (-32)

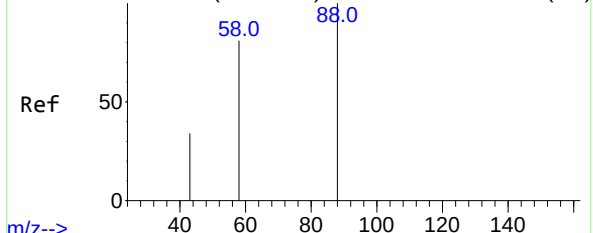

#2
1,4-Dioxane
Concen: 0.192 ng/ul
RT: 3.338 min Scan# 31
Delta R.T. -0.004 min
Lab File: BM034457.D
Acq: 31 Mar 2022 01:36

Instrument :
BNA_M
ClientSampleId :
C0AE4

Abundance Scan 37 (3.338 min): BM034457.D\data.ms

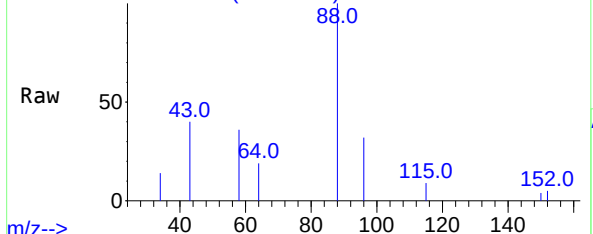

Tgt Ion: 88 Resp: 992

Ion	Ratio	Lower	Upper
88	100		
43	39.9	49.7	74.5
58	36.4	52.5	78.7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/02/2022

Abundance Scan 37 (3.338 min): BM034457.D\data.ms (-26)

