

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
 Data File : BM034483.D
 Acq On : 31 Mar 2022 17:55
 Operator : CG/JU
 Sample : N2100-04
 Misc :
 ALS Vial : 89 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Apr 01 02:58:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 18:27:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	2539	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.730	136	7150	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.564	164	3957	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.308	188	7616	0.400	ng/ul	-0.02
17) Chrysene-d12	21.501	240	5386	0.400	ng/ul	# 0.00
23) Perylene-d12	23.886	264	15081m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	19889	5.266	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	3285	0.341	ng/ul	0.01
18) Fluoranthene-d10	19.334	212	8562	0.510	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.343	88	2724	0.653	ng/ul#	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032922\
Data File : BM034483.D
Acq On : 31 Mar 2022 17:55
Operator : CG/JU
Sample : N2100-04
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6




Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/02/2022

Quant Time: Apr 01 02:58:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM032822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:27:40 2022
Response via : Initial Calibration

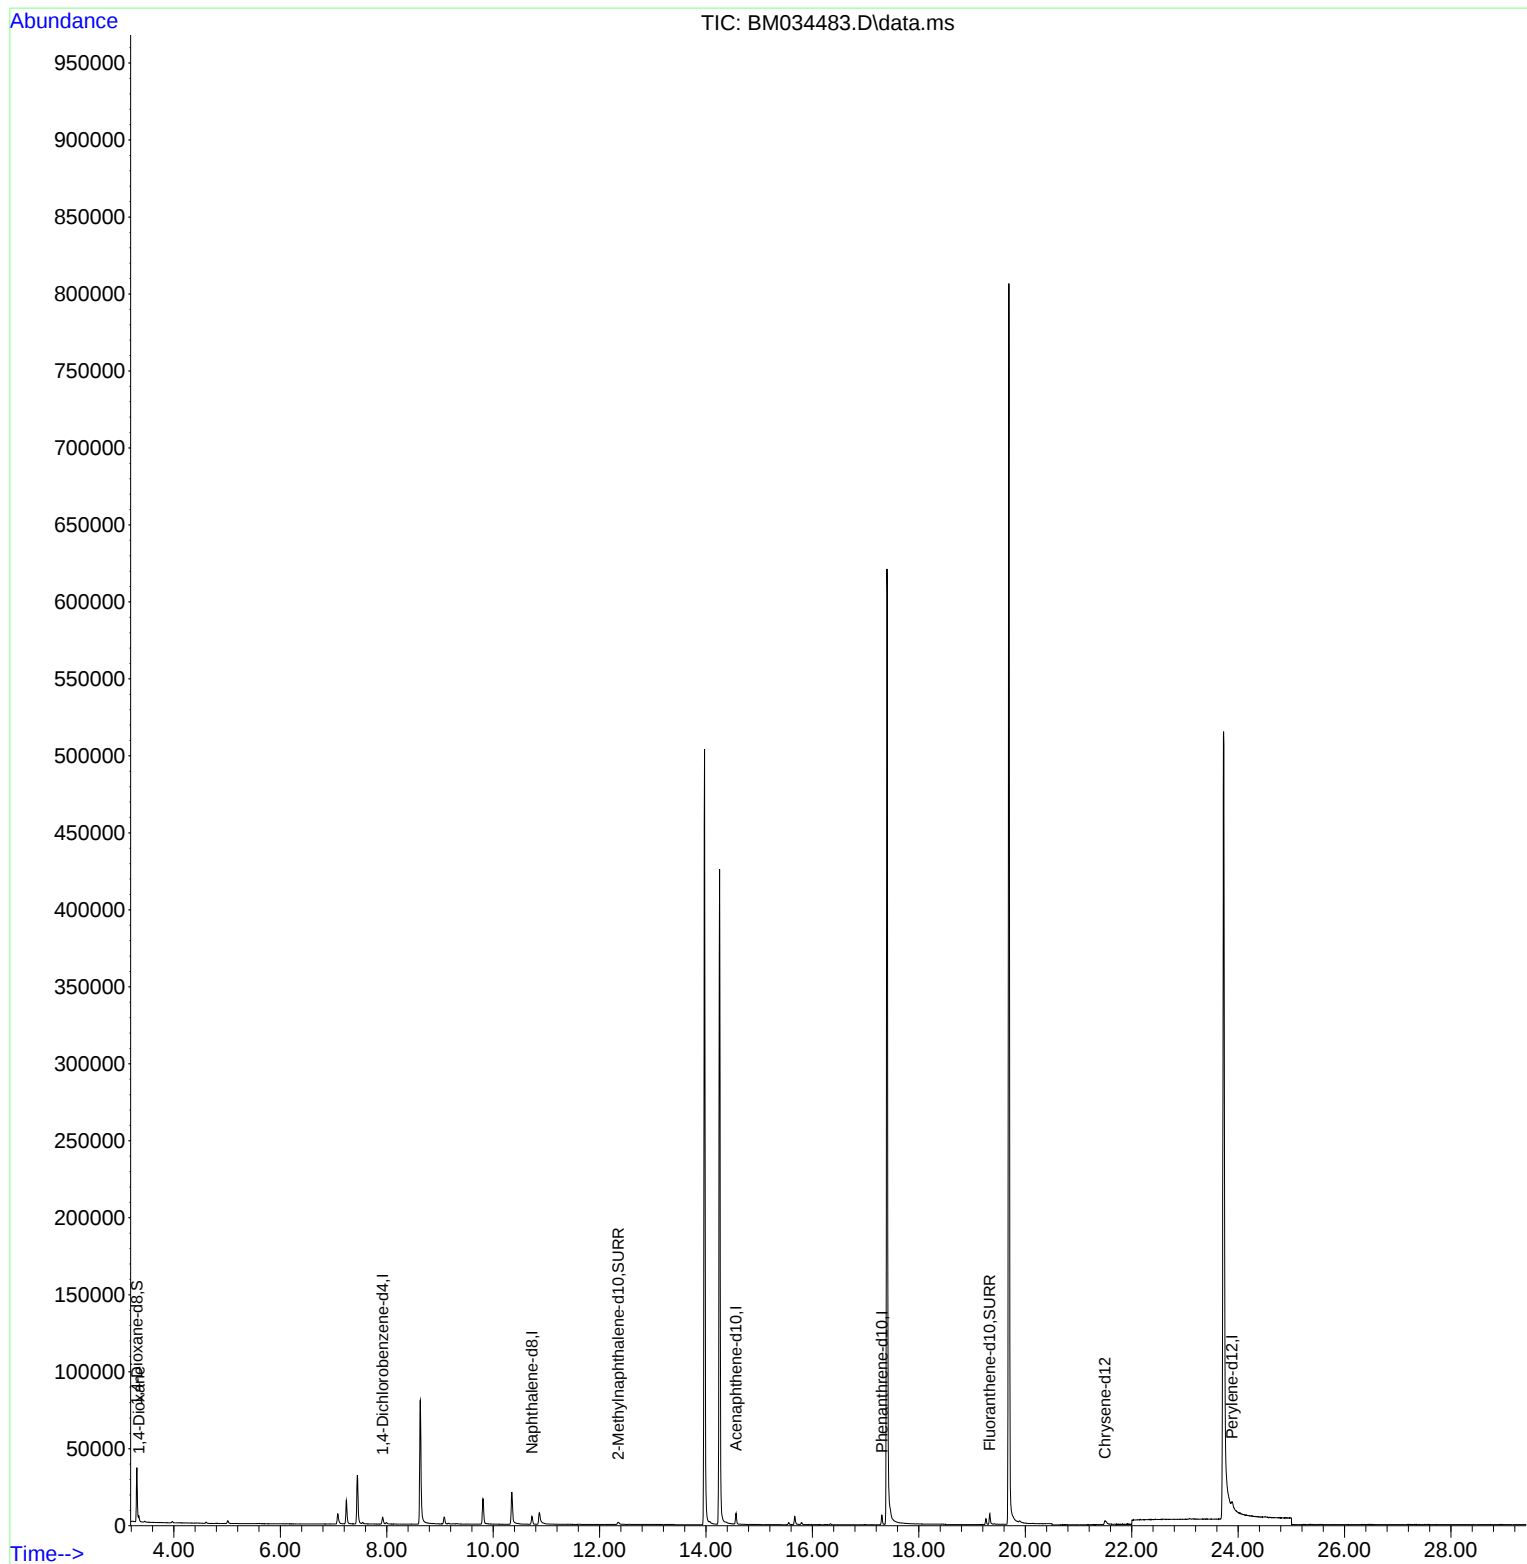

Abundance Scan 38 (3.343 min): BM034470.D\data.ms (-31)

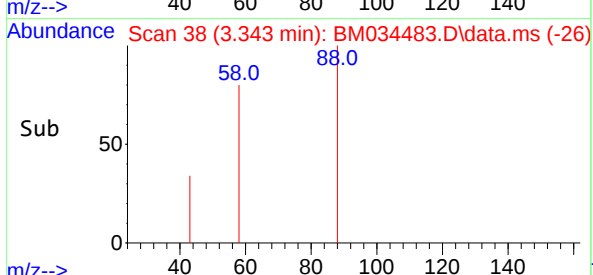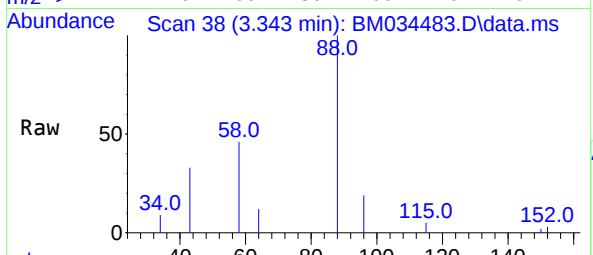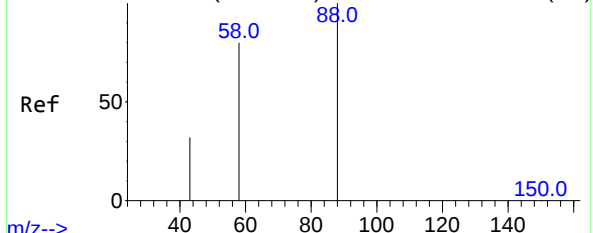

#2
1,4-Dioxane
Concen: 0.653 ng/ul
RT: 3.343 min Scan# 31
Delta R.T. 0.000 min
Lab File: BM034483.D
Acq: 31 Mar 2022 17:55

Instrument :
BNA_M
ClientSampleId :
C0AF6

Tgt Ion: 88 Resp: 2724

Ion	Ratio	Lower	Upper
88	100		
43	33.5	49.7	74.5
58	46.0	52.5	78.7

Manual Integrations
APPROVED
Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/02/2022

