
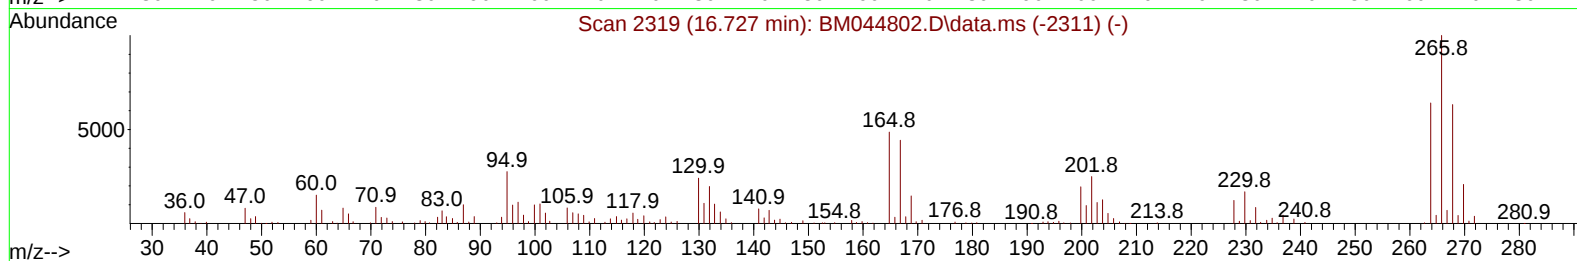
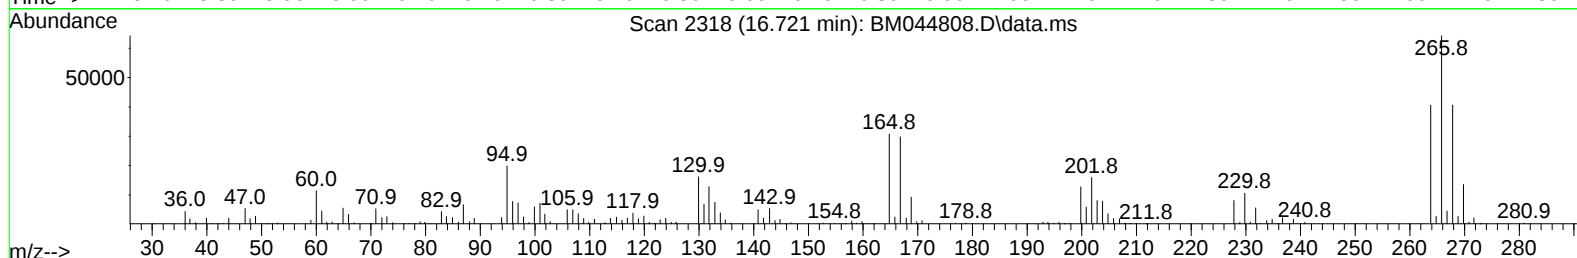


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032924\
Data File : BM044808.D
Acq On : 29 Mar 2024 09:28
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 12:40:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 29 01:24:21 2024
Response via : Initial Calibration

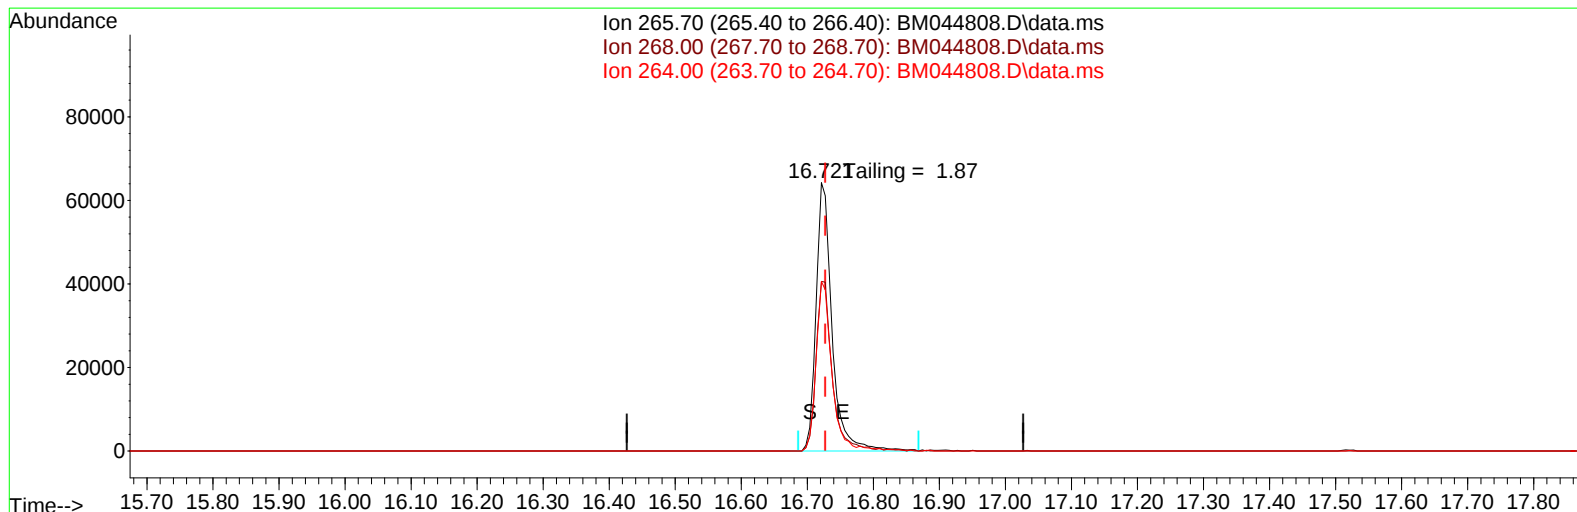

TIC: BM044808.D\data.ms

(70) Pentachlorophenol (C)




16.721min (-0.006) 0.00 ng

response 108737

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.18
264.00	64.10	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032924\
Data File : BM044808.D
Acq On : 29 Mar 2024 09:28
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 12:40:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 29 01:24:21 2024
Response via : Initial Calibration

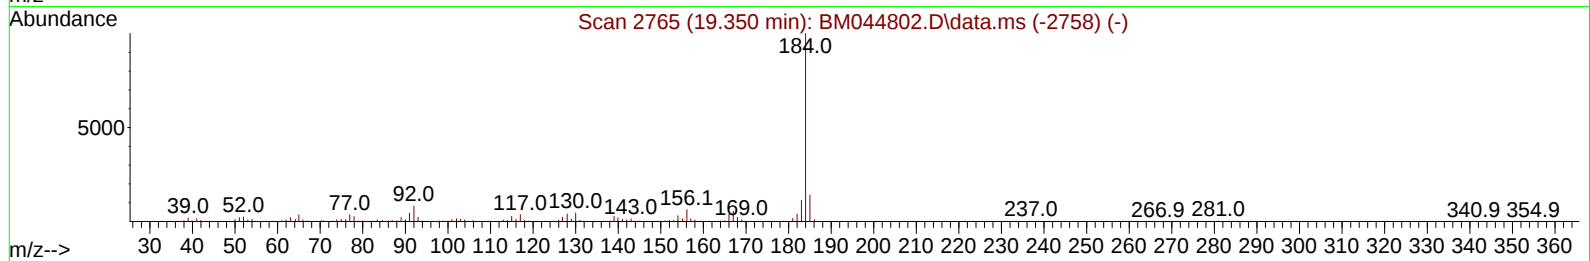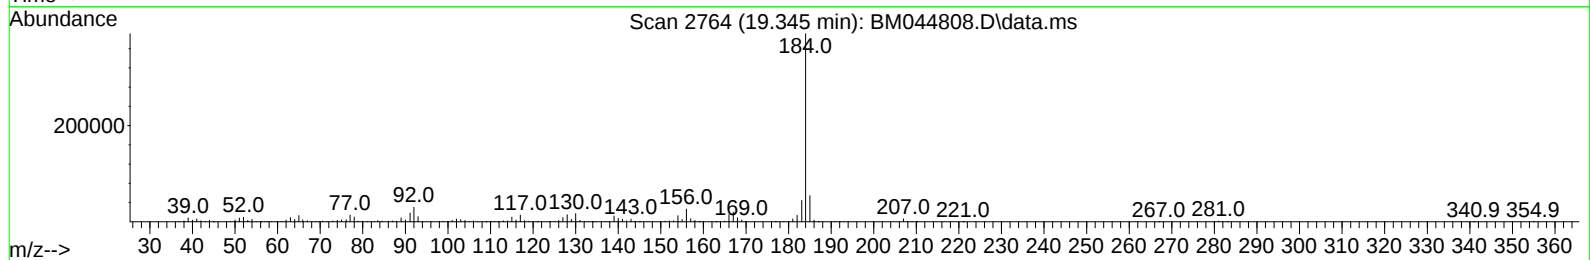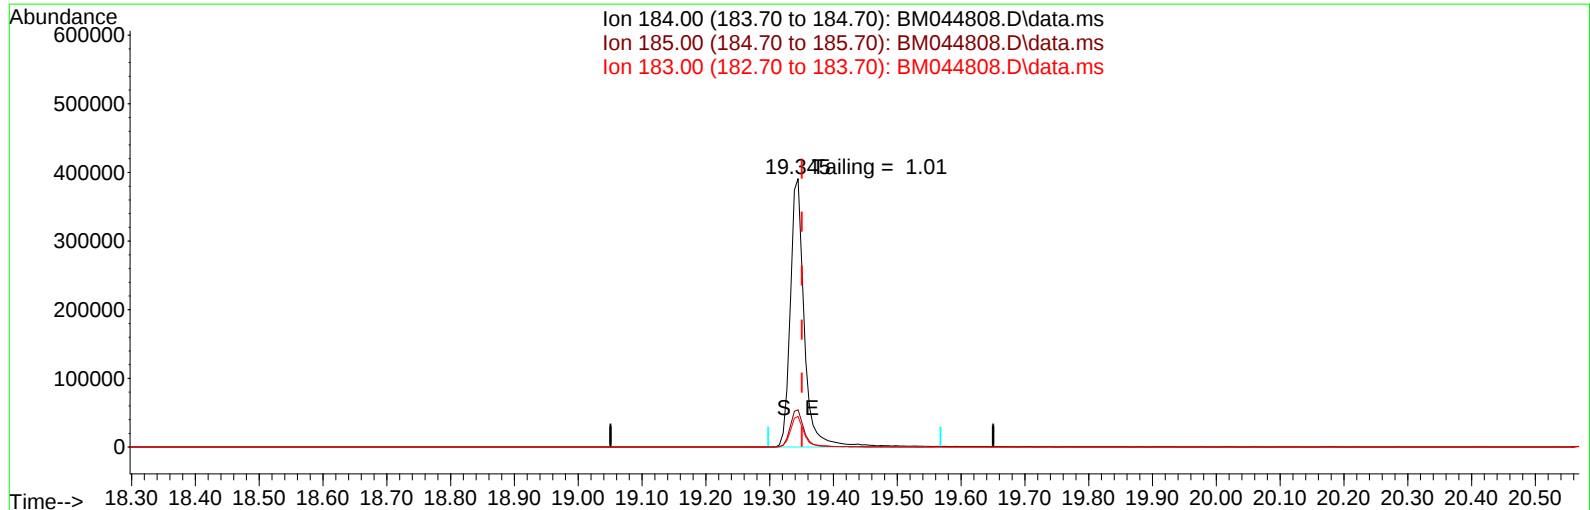

TIC: BM044808.D\data.ms

(77) Benzidine**19.345min (-0.006) 183066.95 ng****response 599971**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.93
183.00	11.30	11.39
0.00	0.00	0.00