


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032924\
Data File : BM044808.D
Acq On : 29 Mar 2024 09:28
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 29 01:24:21 2024

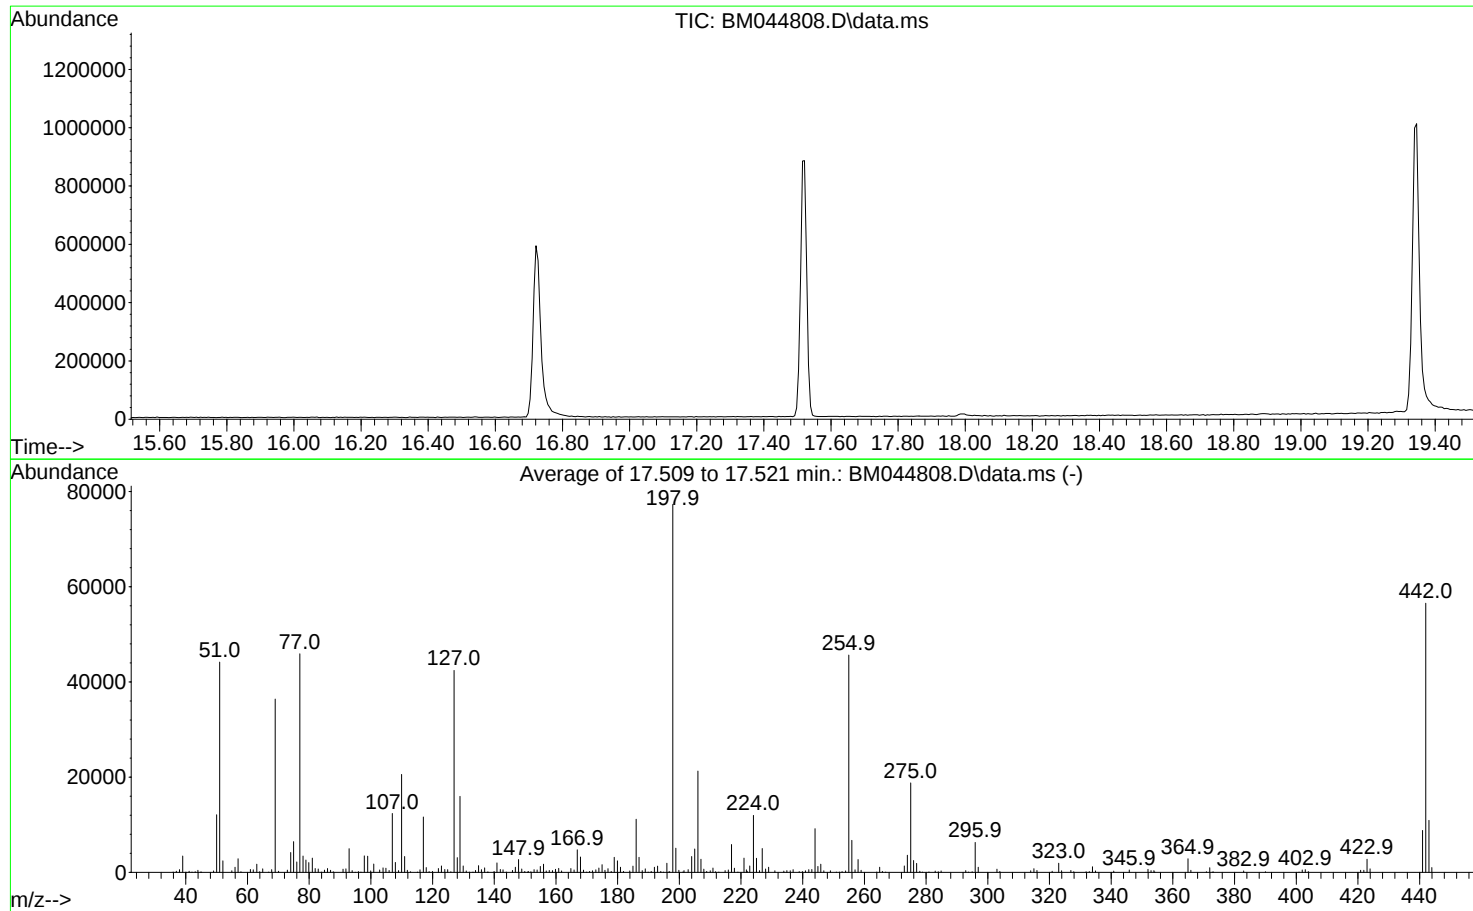




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	44153	PASS
68	69	0.00	2	1.6	578	PASS
69	198	0.00	100	47.1	36419	PASS
70	69	0.00	2	0.7	241	PASS
127	198	10	80	54.9	42427	PASS
197	198	0.00	2	0.2	169	PASS
198	198	100	100	100.0	77275	PASS
199	198	5	9	6.6	5067	PASS
275	198	10	60	24.3	18777	PASS
365	198	1	100	3.7	2866	PASS
441	198	0.01	100	11.4	8802	PASS
442	442	50	100	100.0	56525	PASS
443	442	15	24	19.3	10913	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032924\
Data File : BM044808.D
Acq On : 29 Mar 2024 09:28
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 29 12:40:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 29 01:24:21 2024
Response via : Initial Calibration

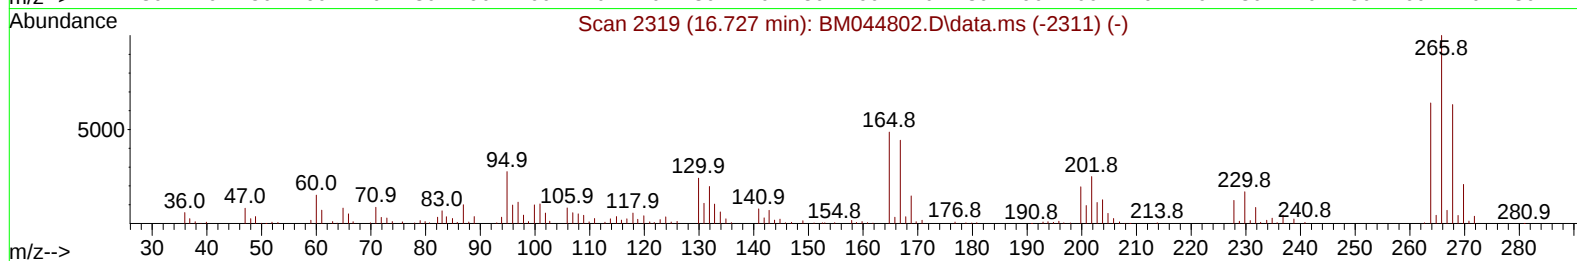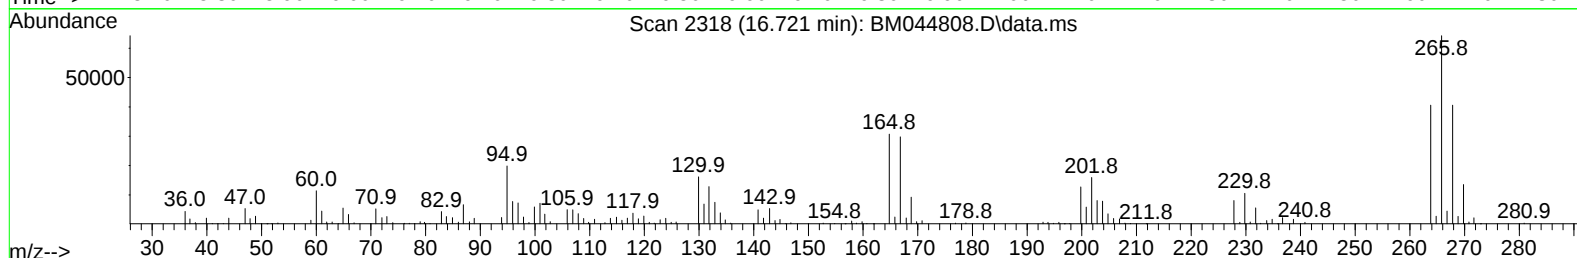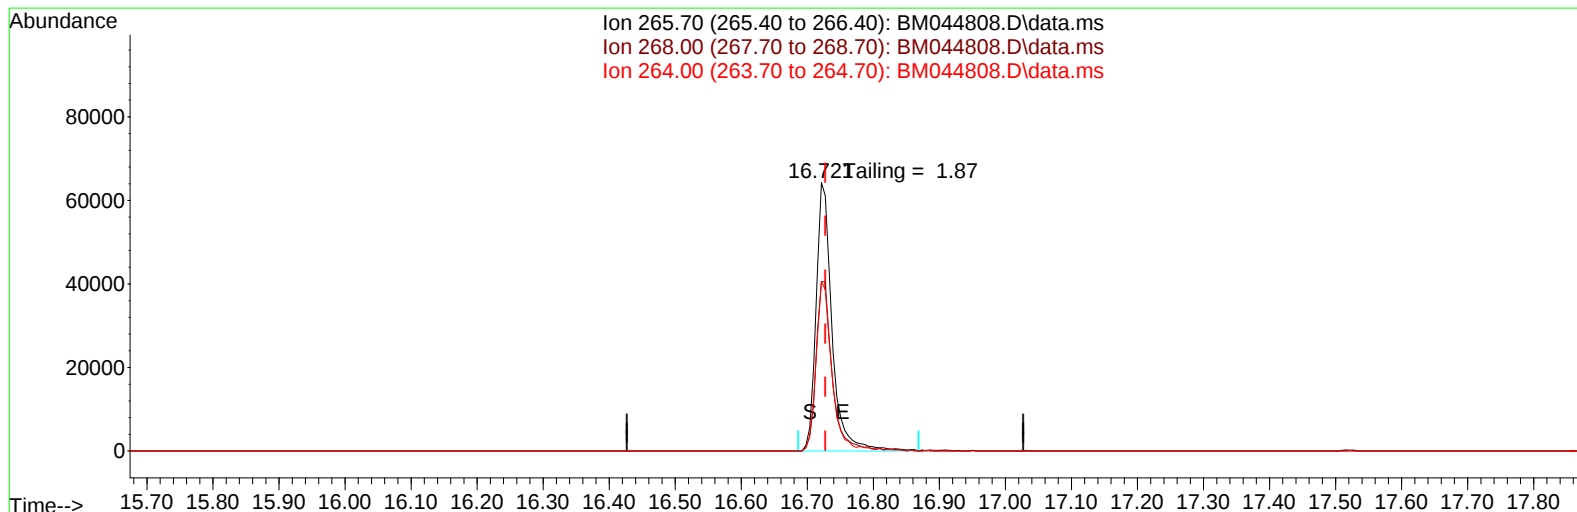

TIC: BM044808.D\data.ms

(70) Pentachlorophenol (C)

16.721min (-0.006) 0.00 ng




response 108737

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.18
264.00	64.10	63.13
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM03292\  
Data File : BM044808.D  
Acq On    : 29 Mar 2024  09:28  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 29 12:40:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 29 01:24:21 2024
Response via : Initial Calibration

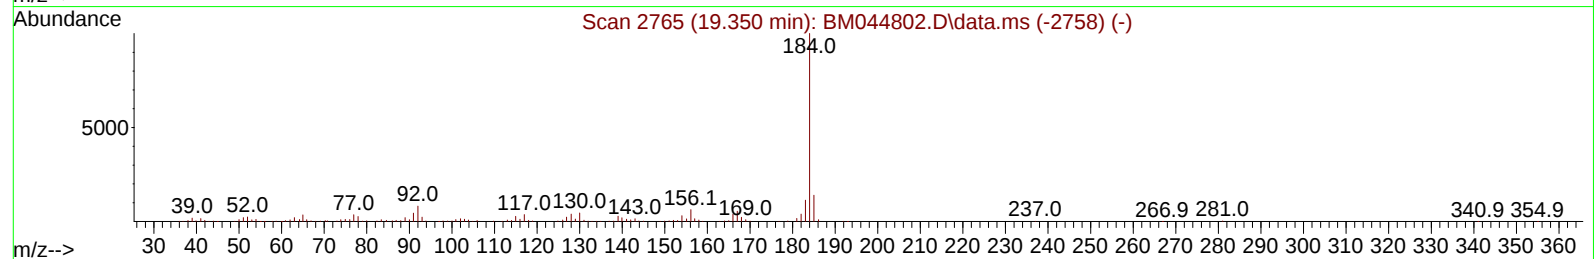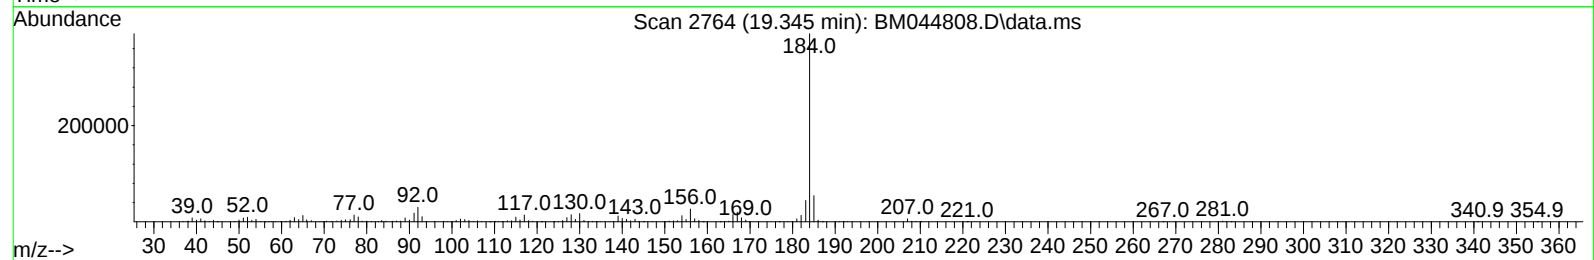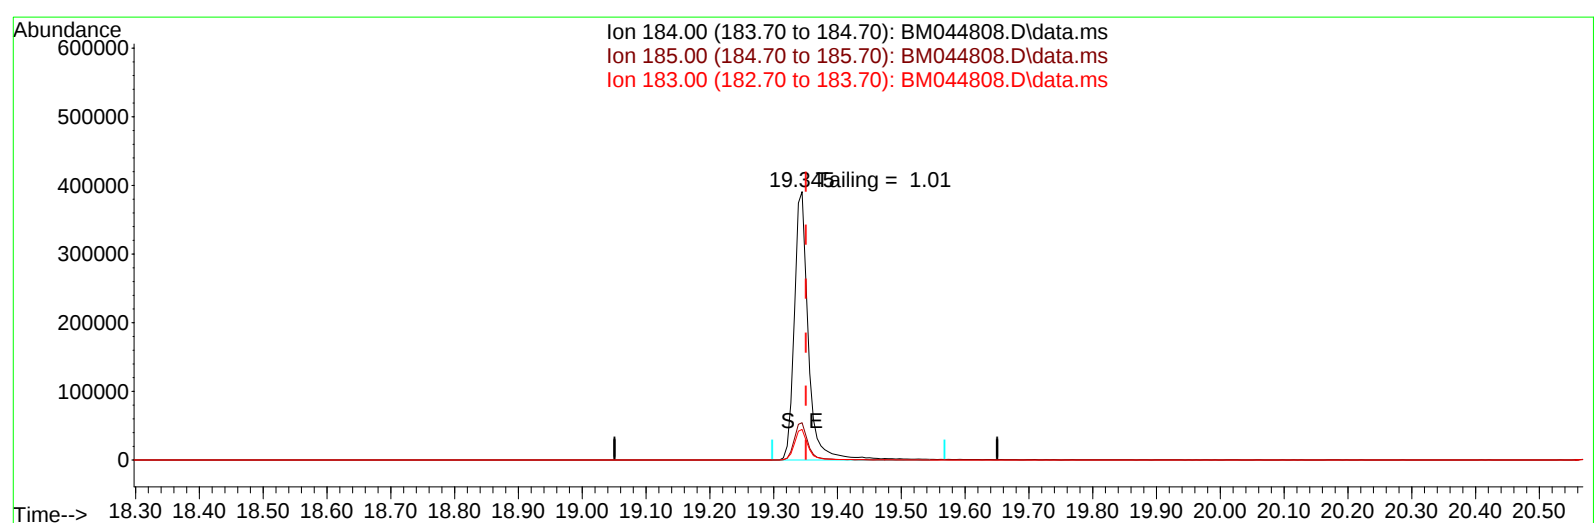

TIC: BM044808.D\data.ms

(77) Benzidine

19.345min (-0.006) 183066.95 ng

response **599971**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.00	13.93
--------	-------	-------

183.00	11.30	11.39
--------	-------	-------

0.00 0.00 0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/29/2024	BNA_M	<u>BM044808.D</u>
Compound Name	Response	Retention Time
DDT	271178	20.574
DDD	4870	20.139
DDE	54	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4924	276102	1.78

Instrument :
BNA_M
ClientSampleId :
DFTPP