


Data Path : Z:\HPCHEM1\BNA M\DATA\BM033017\
 Data File : BM009450.D
 Acq On : 30 Mar 2017 14:29
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 31 12:10:26 2017

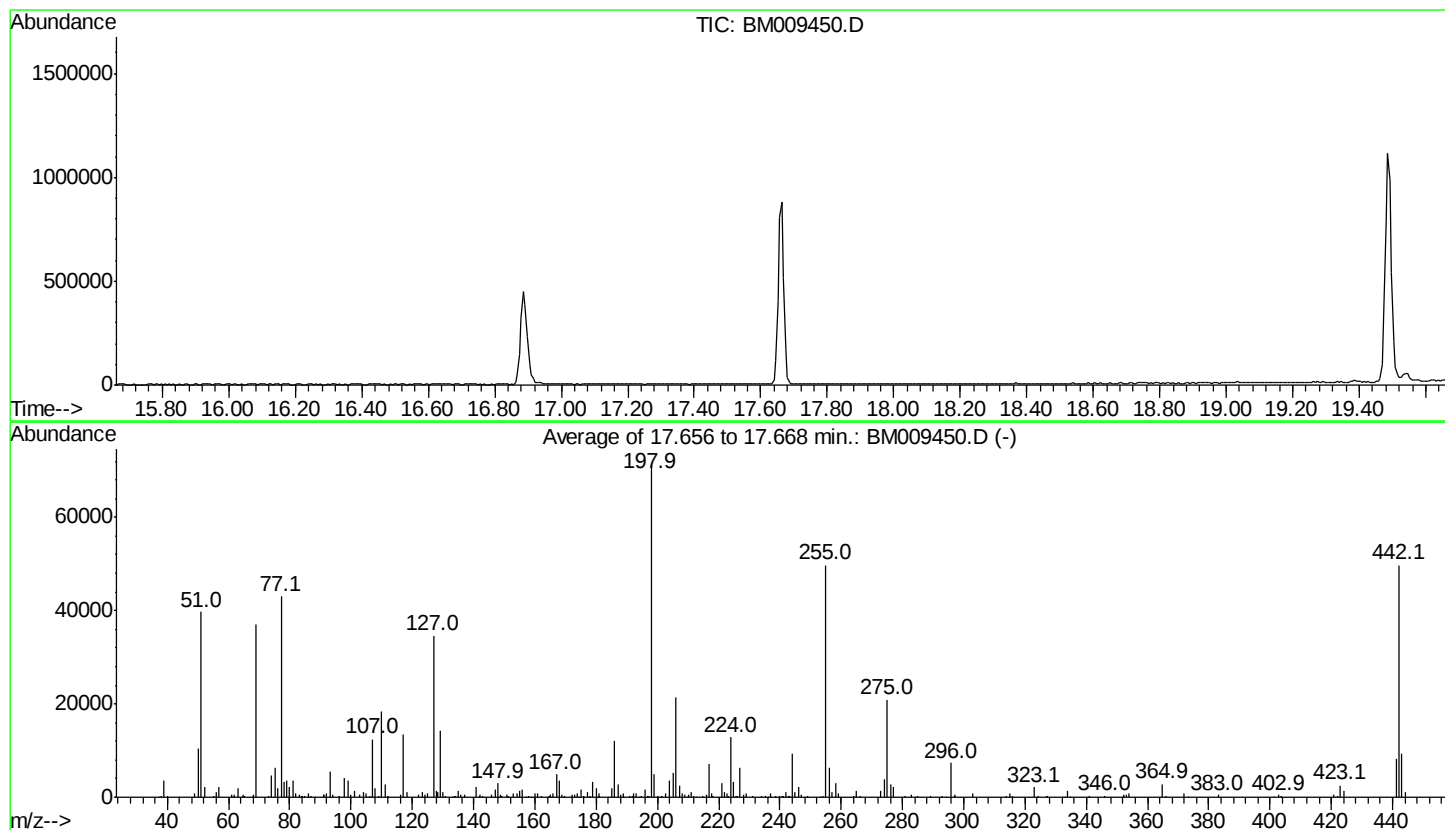

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.0	39773	PASS
68	69	0.00	2	1.3	463	PASS
69	198	0.00	100	52.0	36960	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	34650	PASS
197	198	0.00	2	0.3	234	PASS
198	198	100	100	100.0	71058	PASS
199	198	5	9	7.0	4971	PASS
275	198	10	60	29.4	20874	PASS
365	198	1	100	3.9	2784	PASS
441	442	0.01	24	16.3	8109	PASS
442	198	50	100	70.0	49741	PASS
443	442	15	24	19.0	9437	PASS