


Data Path : Z:\HPCHEM1\BNA M\DATA\BM033017\
 Data File : BM009465.D
 Acq On : 31 Mar 2017 01:34
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 31 12:10:26 2017

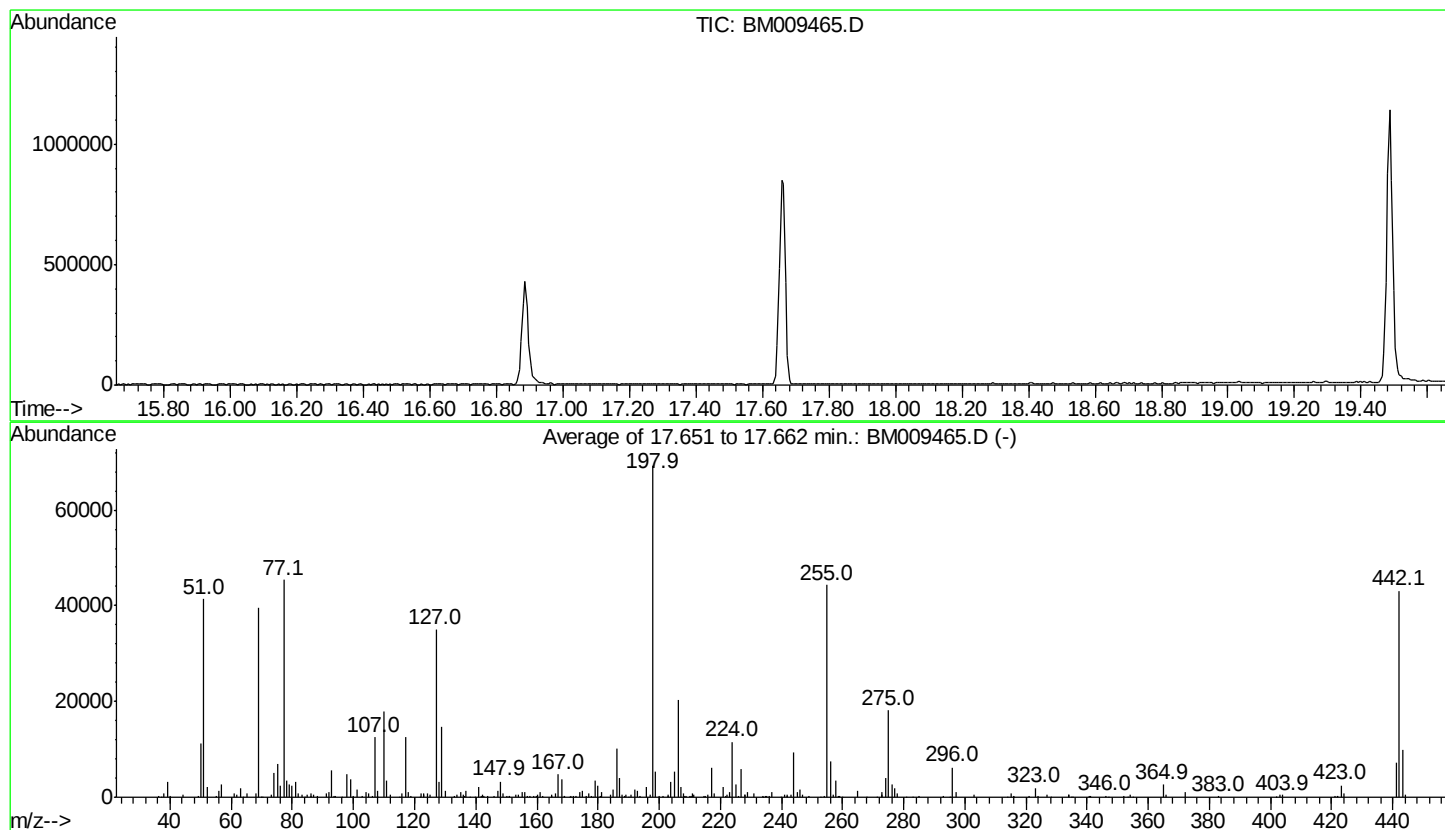

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.7	41320	PASS
68	69	0.00	2	1.8	719	PASS
69	198	0.00	100	57.1	39538	PASS
70	69	0.00	2	0.3	110	PASS
127	198	10	80	50.6	35018	PASS
197	198	0.00	2	0.7	457	PASS
198	198	100	100	100.0	69250	PASS
199	198	5	9	7.7	5332	PASS
275	198	10	60	26.1	18105	PASS
365	198	1	100	3.7	2558	PASS
441	442	0.01	24	17.0	7325	PASS
442	198	50	100	62.2	43098	PASS
443	442	15	24	23.0	9918	PASS