
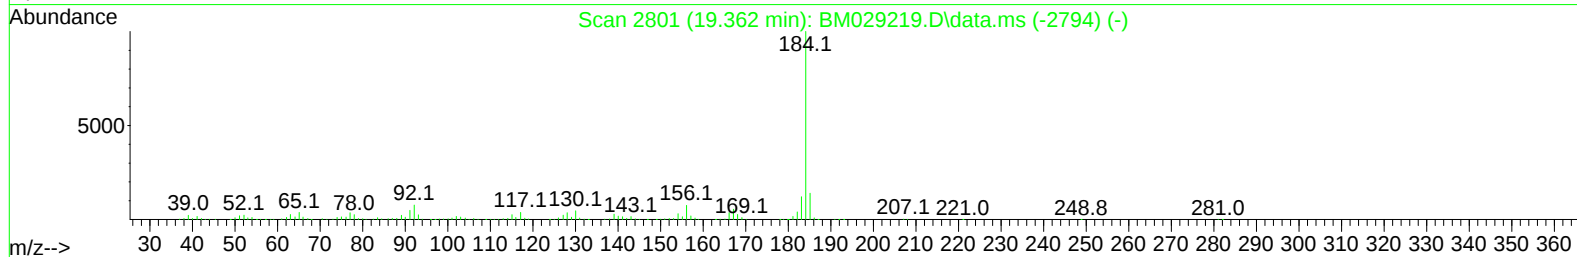
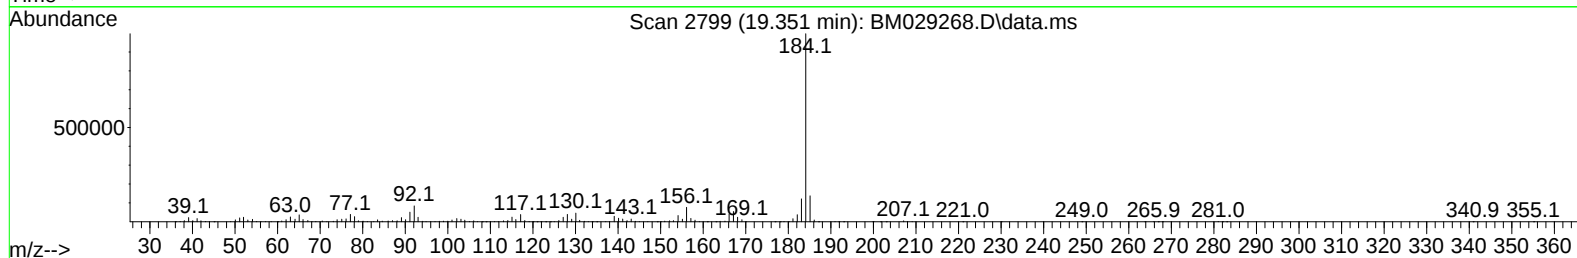


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM033021\  
 Data File : BM029268.D  
 Acq On : 30 Mar 2021 13:09  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 14:21:07 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM032621.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Mar 29 11:14:33 2021  
 Response via : Initial Calibration

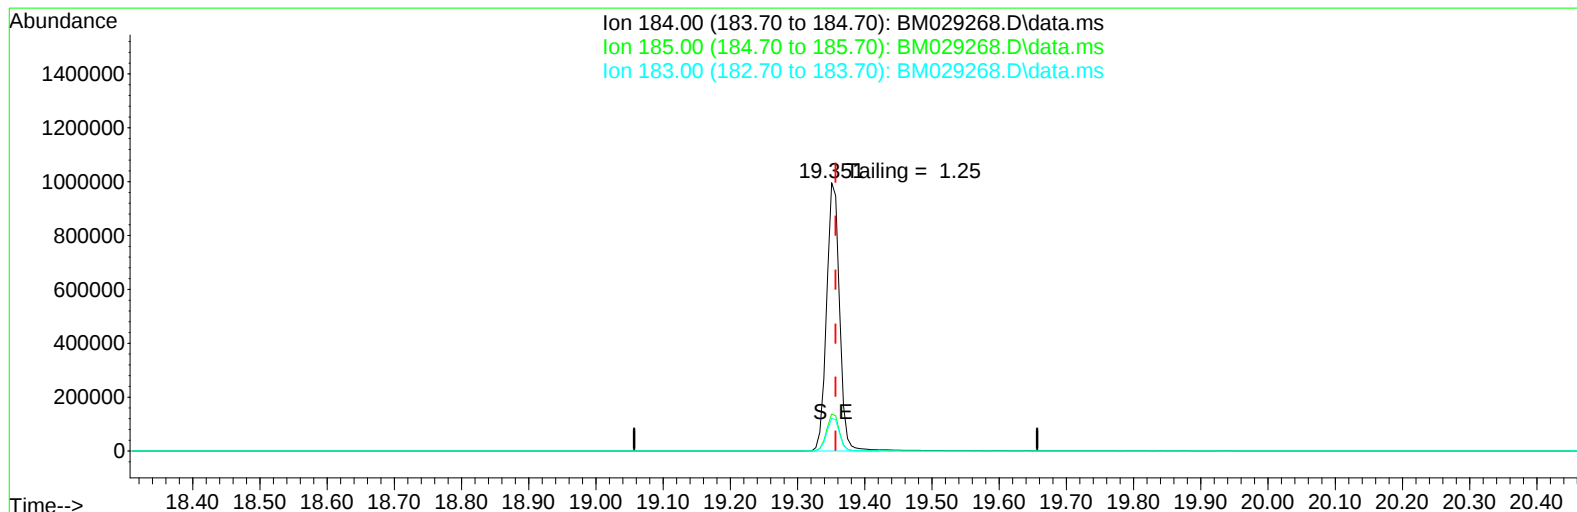




TIC: BM029268.D\data.ms

**(77) Benzidine****19.351min (-0.006) 64912.04 ng****response 1335243**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 13.80  |
| 183.00 | 12.20  | 12.23  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM033021\  
Data File : BM029268.D  
Acq On : 30 Mar 2021 13:09  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 14:21:07 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM032621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 29 11:14:33 2021  
Response via : Initial Calibration

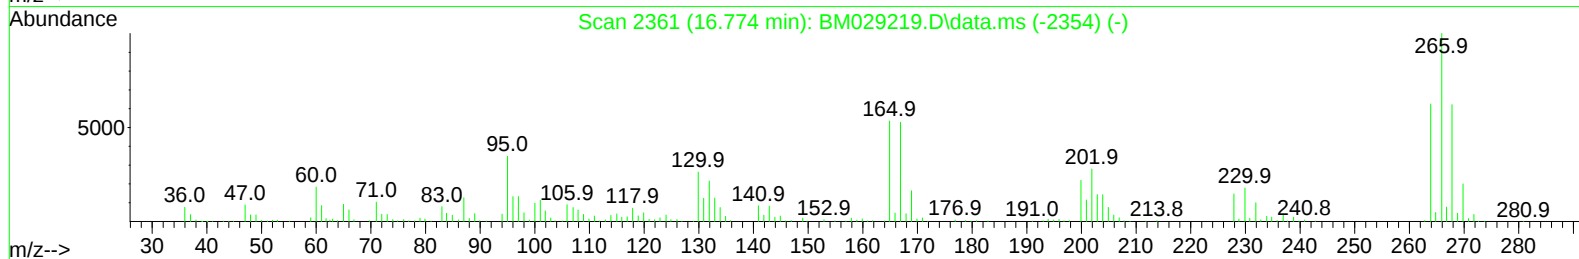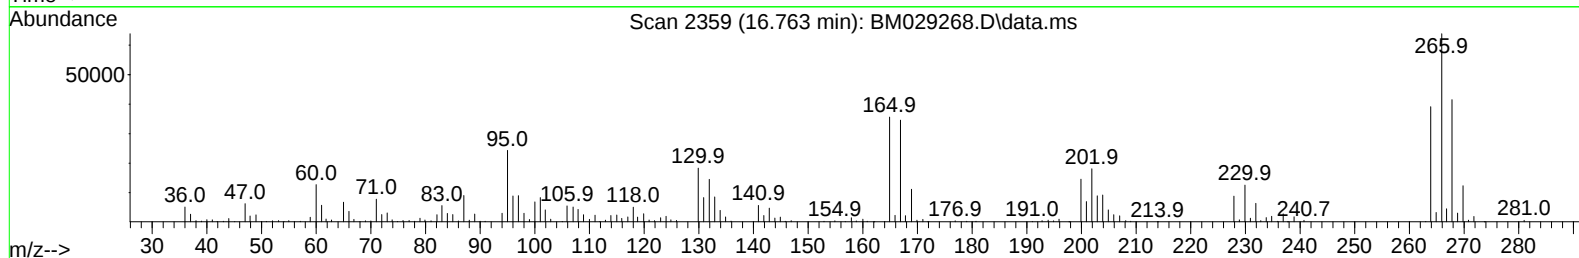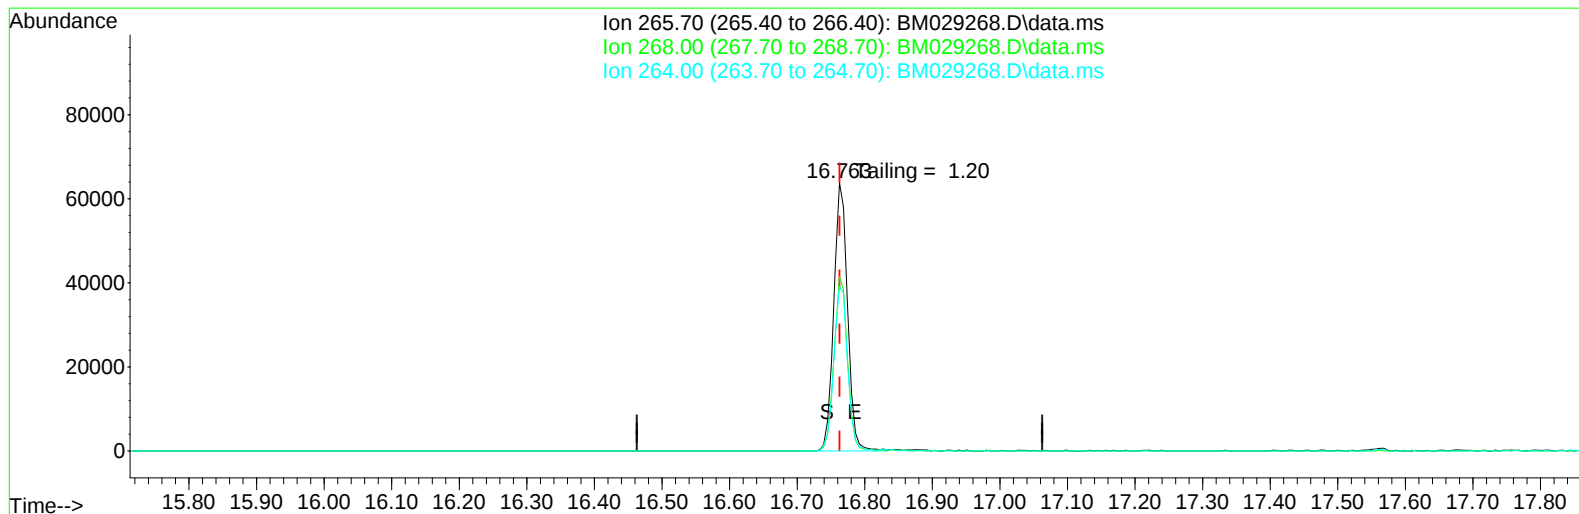

TIC: BM029268.D\data.ms

**(70) Pentachlorophenol (C)**

16.763min (-0.000) 200460.39 ng

response 90570

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.20  | 65.06  |
| 264.00 | 63.60  | 61.33  |
| 0.00   | 0.00   | 0.00   |