

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
 Data File : BM029270.D
 Acq On : 30 Mar 2021 14:59
 Operator : CG/JU
 Sample : PB135411BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135411BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.893	336	341	351	rBV	185046	260162	3.83%	0.793%
2	5.346	411	418	431	rBV	2636244	3726261	54.92%	11.358%
3	6.916	678	685	695	rBV	2463727	3878569	57.16%	11.822%
4	7.746	820	826	834	rVB	476141	734637	10.83%	2.239%
5	8.898	1014	1022	1035	rBV	1524306	2533200	37.33%	7.722%
6	10.528	1291	1299	1309	rBV	572667	973150	14.34%	2.966%
7	12.998	1712	1719	1730	rBV	3643183	5305289	78.19%	16.171%
8	14.375	1944	1953	1966	rBV	837921	1235335	18.21%	3.765%
9	15.857	2198	2205	2215	rBV	2457697	3433943	50.61%	10.467%
10	17.110	2412	2418	2426	rBV	937846	1326611	19.55%	4.044%
11	19.733	2858	2864	2872	rBV	5623498	6785231	100.00%	20.682%
12	21.062	3087	3090	3096	rBV	53286	83290	1.23%	0.254%
13	21.280	3122	3127	3135	rBV	978707	1262548	18.61%	3.848%
14	23.515	3501	3507	3515	rVB2	655486	1268786	18.70%	3.867%




Sum of corrected areas: 32807012

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
Data File : BM029270.D
Acq On : 30 Mar 2021 14:59
Operator : CG/JU
Sample : PB135411BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135411BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

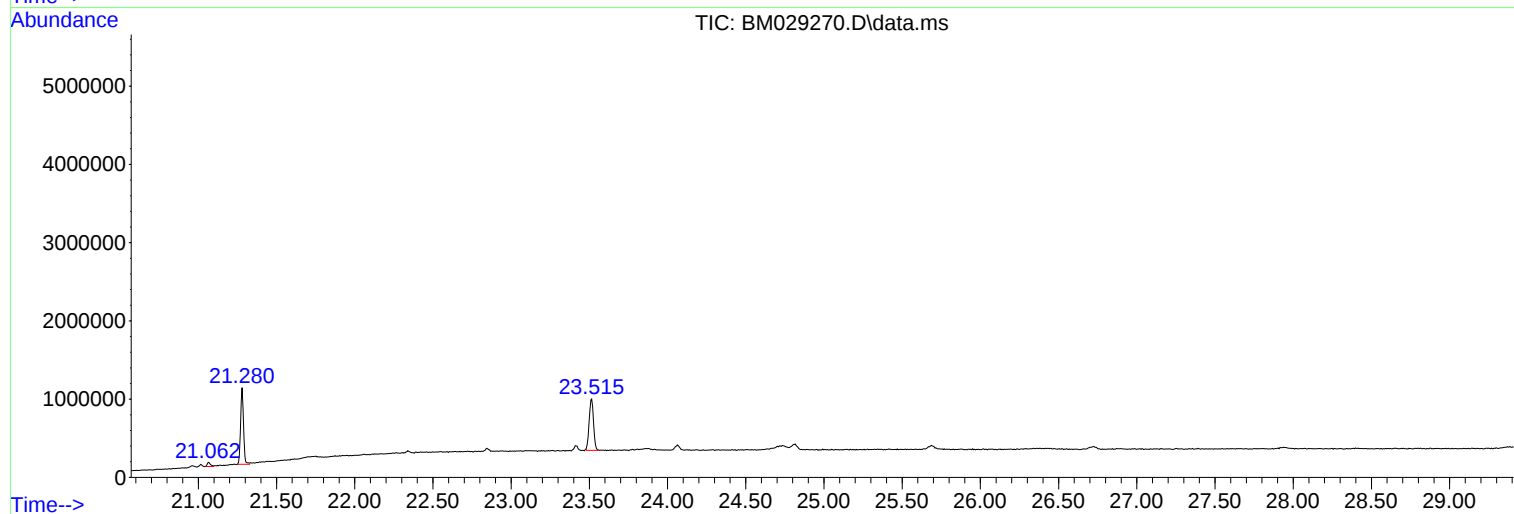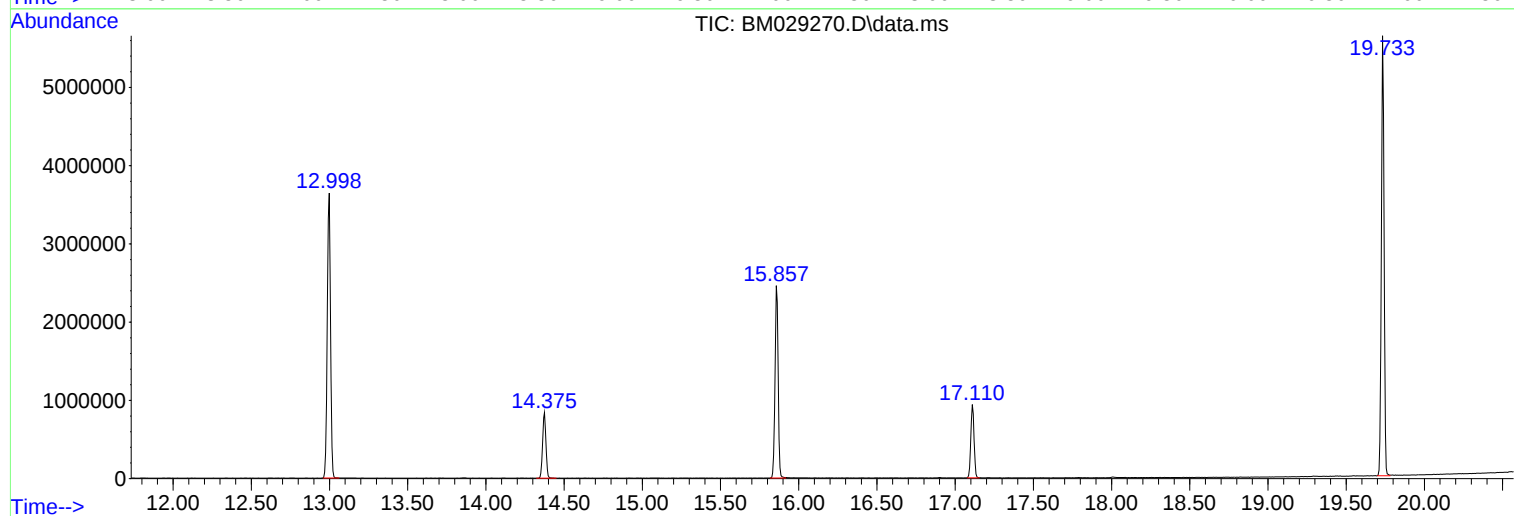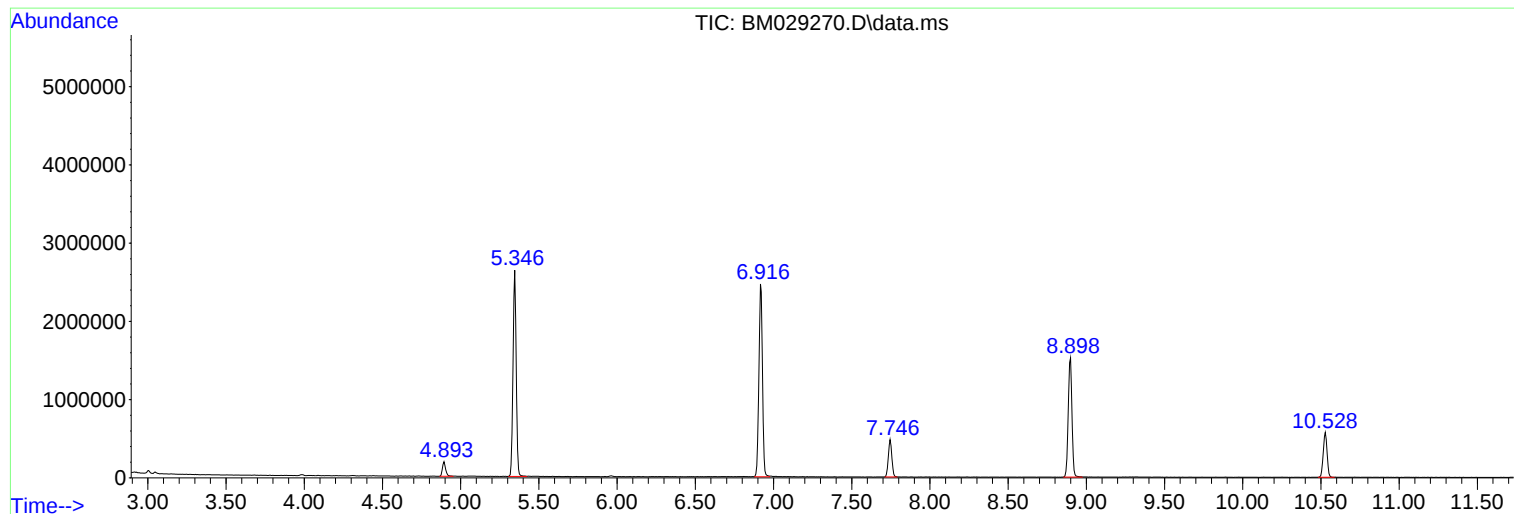

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
Data File : BM029270.D
Acq On : 30 Mar 2021 14:59
Operator : CG/JU
Sample : PB135411BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135411BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
Data File : BM029270.D
Acq On : 30 Mar 2021 14:59
Operator : CG/JU
Sample : PB135411BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135411BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------