

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
 Data File : BM029273.D
 Acq On : 30 Mar 2021 16:59
 Operator : CG/JU
 Sample : PB135399BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135399BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.004	16	20	25	rVB	60455	72103	1.05%	0.210%
2	4.892	336	341	350	rBV	266625	383451	5.60%	1.118%
3	5.345	411	418	428	rBV	2739744	3915752	57.15%	11.413%
4	6.916	677	685	696	rBV	2641133	4074080	59.46%	11.875%
5	7.745	819	826	833	rBV	496680	767986	11.21%	2.238%
6	8.898	1014	1022	1037	rBV	1578062	2664024	38.88%	7.765%
7	10.527	1292	1299	1307	rBV	600374	1034002	15.09%	3.014%
8	12.998	1710	1719	1730	rBV	3757264	5516661	80.52%	16.079%
9	14.374	1946	1953	1964	rBV	862845	1302201	19.01%	3.795%
10	15.856	2198	2205	2219	rBV	2556877	3548841	51.80%	10.344%
11	17.109	2412	2418	2428	rBV	956201	1389284	20.28%	4.049%
12	19.733	2858	2864	2872	rBV	5553600	6851590	100.00%	19.970%
13	21.068	3087	3091	3094	rBV	78602	97615	1.42%	0.285%
14	21.280	3122	3127	3132	rBV	1074599	1328271	19.39%	3.871%
15	23.515	3501	3507	3516	rVB2	698660	1363254	19.90%	3.973%

Sum of corrected areas: 34309115

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
Data File : BM029273.D
Acq On : 30 Mar 2021 16:59
Operator : CG/JU
Sample : PB135399BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135399BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.892	9.99 ng	383451	1,4-Dichlorobenzene-d4	7.745

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27		
3	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	23		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

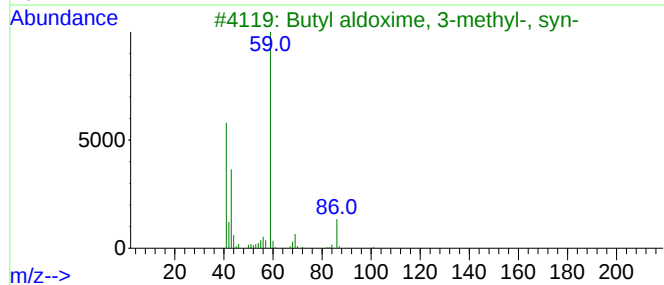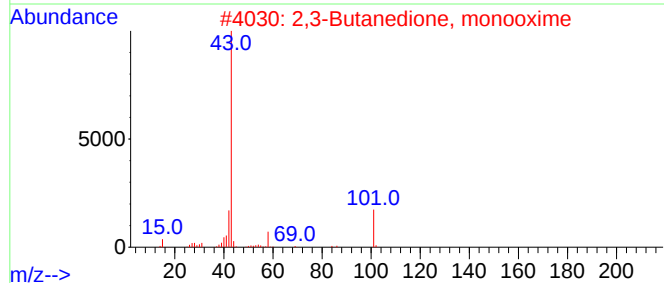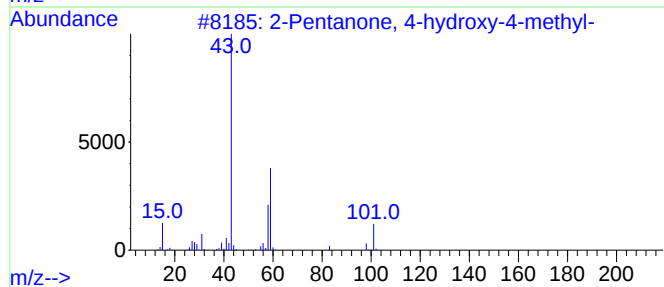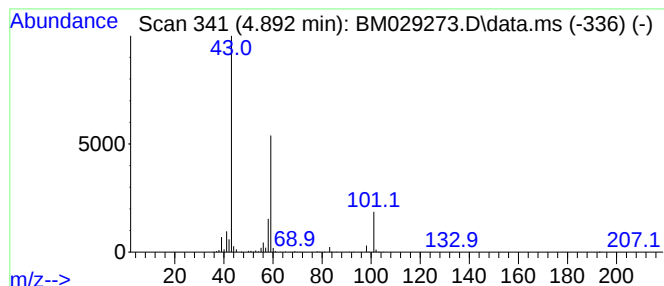

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
Data File : BM029273.D
Acq On : 30 Mar 2021 16:59
Operator : CG/JU
Sample : PB135399BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135399BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.892	10.0	ng	383451	1	7.745	767986	20.0