
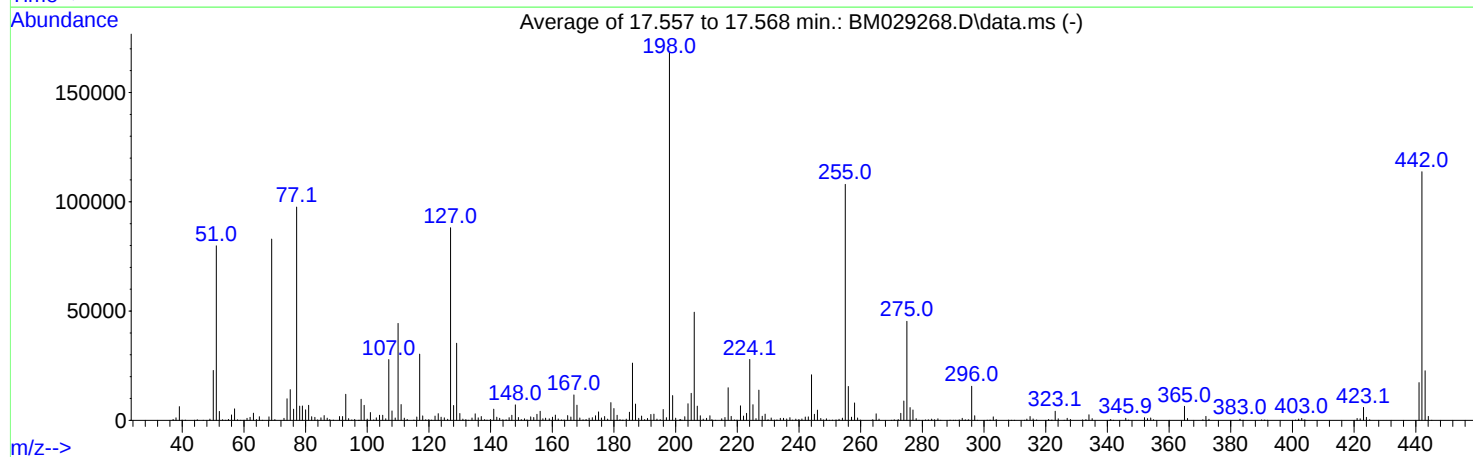


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
 Data File : BM029268.D
 Acq On : 30 Mar 2021 13:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 29 11:14:33 2021

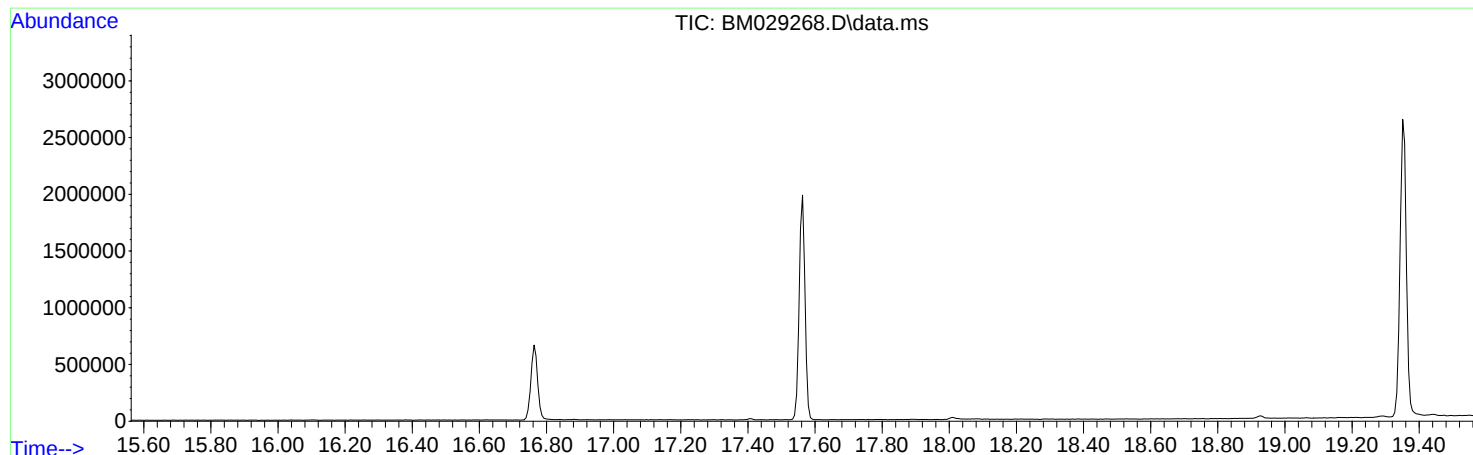




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	79896	PASS
68	69	0.00	2	2.0	1634	PASS
69	198	0.00	100	49.3	82975	PASS
70	69	0.00	2	0.5	399	PASS
127	198	10	80	52.3	88104	PASS
197	198	0.00	2	0.7	1238	PASS
198	198	100	100	100.0	168299	PASS
199	198	5	9	6.7	11359	PASS
275	198	10	60	26.9	45339	PASS
365	198	1	100	3.8	6434	PASS
441	198	0.01	100	10.3	17303	PASS
442	442	50	100	100.0	113776	PASS
443	442	15	24	19.9	22691	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
 Data File : BM029268.D
 Acq On : 30 Mar 2021 13:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 30 14:21:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 29 11:14:33 2021
 Response via : Initial Calibration

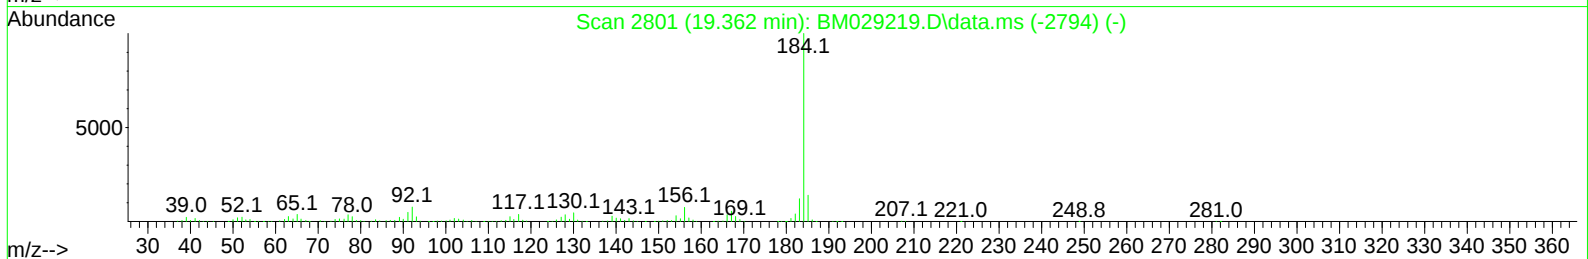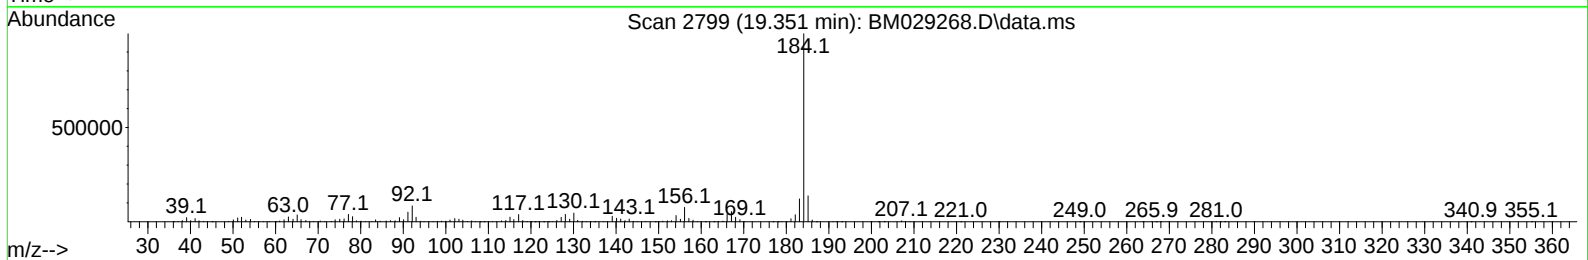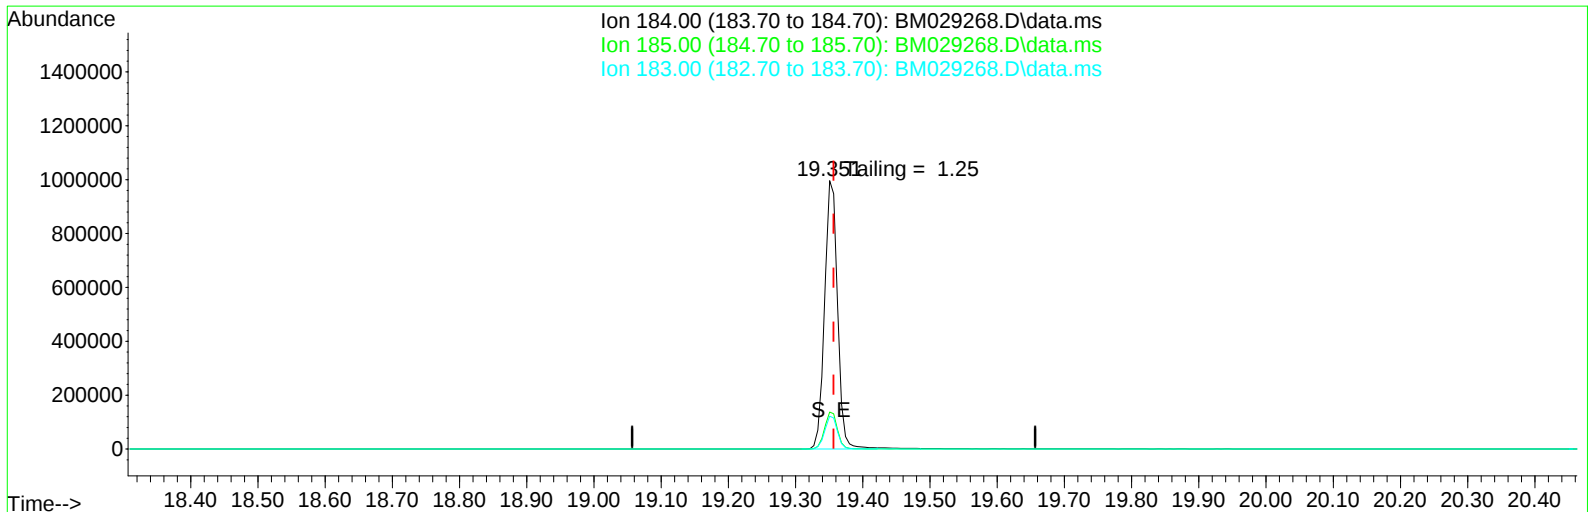

TIC: BM029268.D\data.ms

(77) Benzidine

19.351min (-0.006) 64912.04 ng




response 1335243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.80
183.00	12.20	12.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033021\
Data File : BM029268.D
Acq On : 30 Mar 2021 13:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 30 14:21:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 29 11:14:33 2021
Response via : Initial Calibration

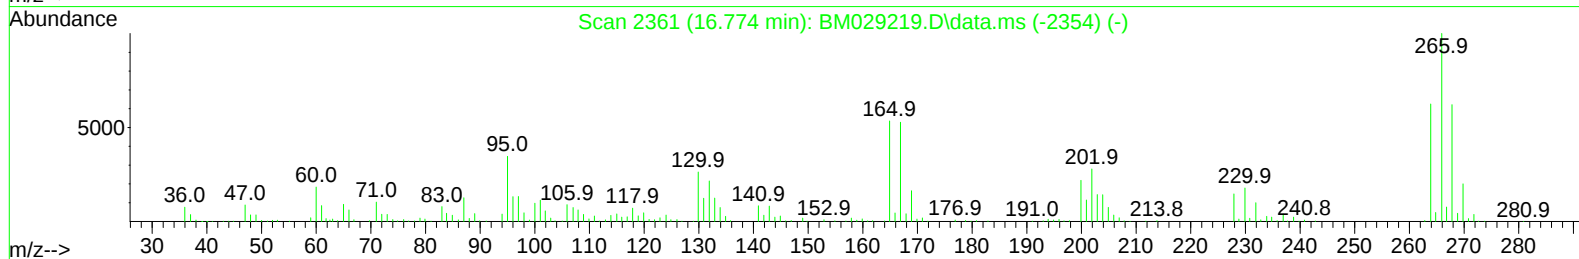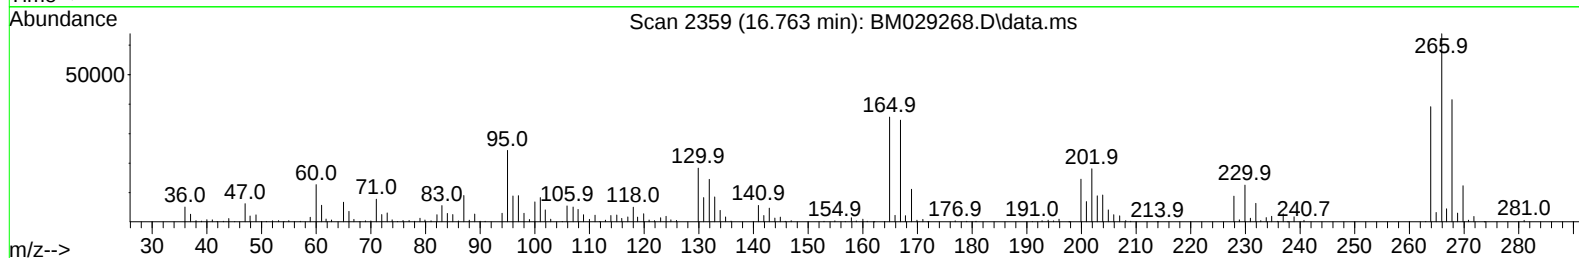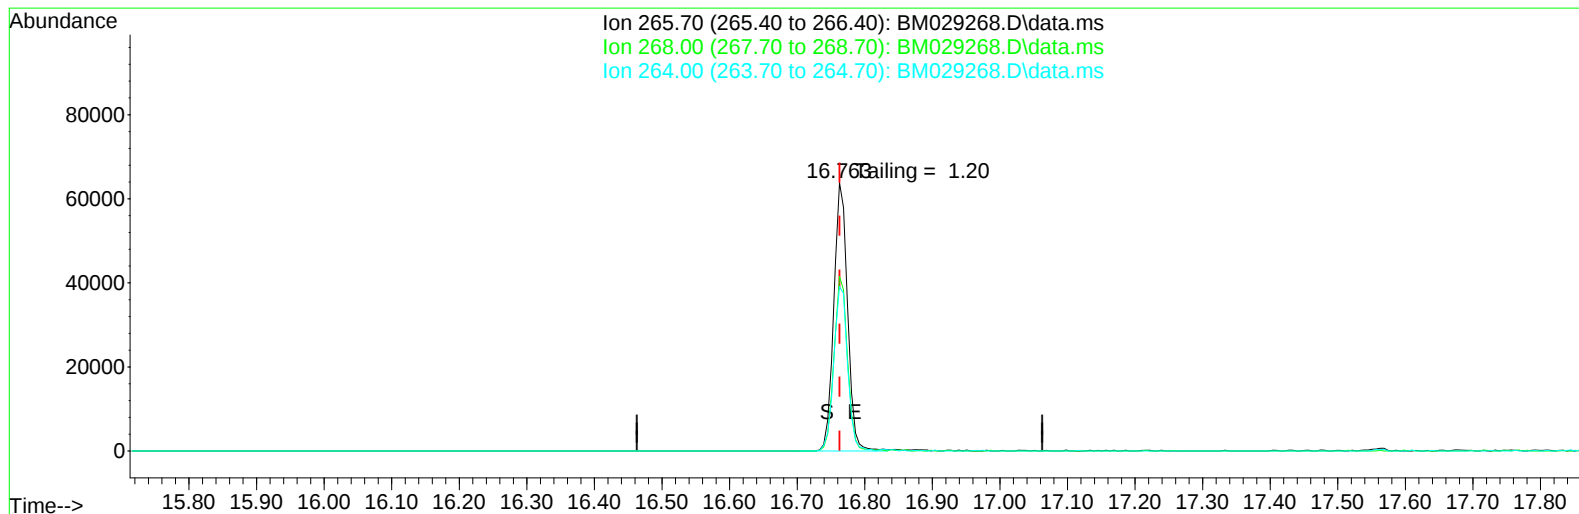

TIC: BM029268.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.000) 200460.39 ng

response 90570

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	65.06
264.00	63.60	61.33
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
3/30/2021	BNA_M	<u>BM029268.D</u>
Compound Name	Response	Retention Time
DDT	628588	20.58
DDD	4259	20.15
DDE	720	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4979	633567	0.79