
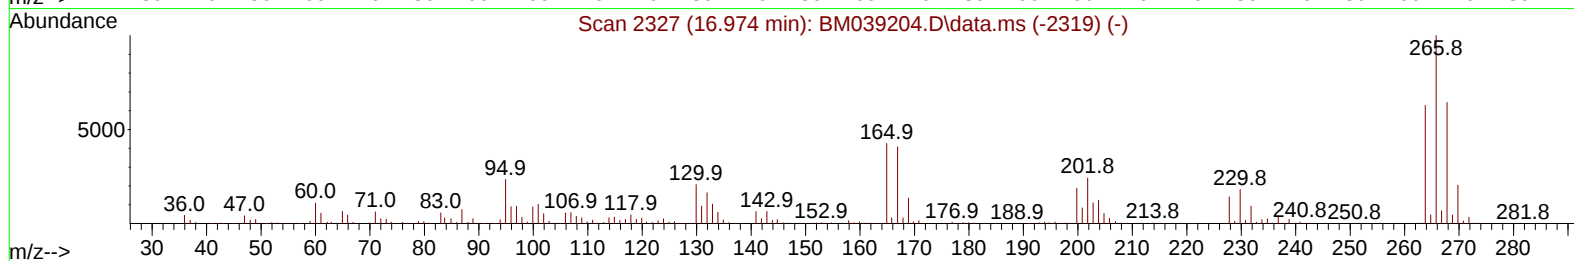
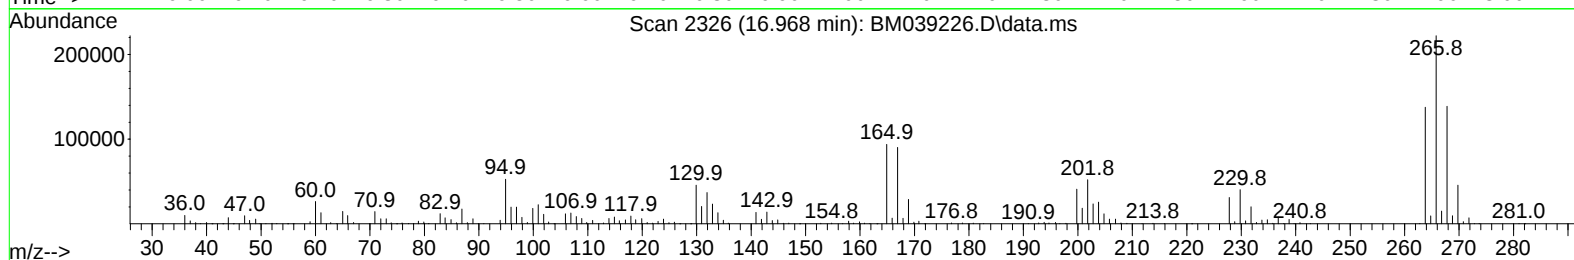


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
Data File : BM039226.D
Acq On : 30 Mar 2023 14:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 05:03:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 30 05:15:45 2023
Response via : Initial Calibration

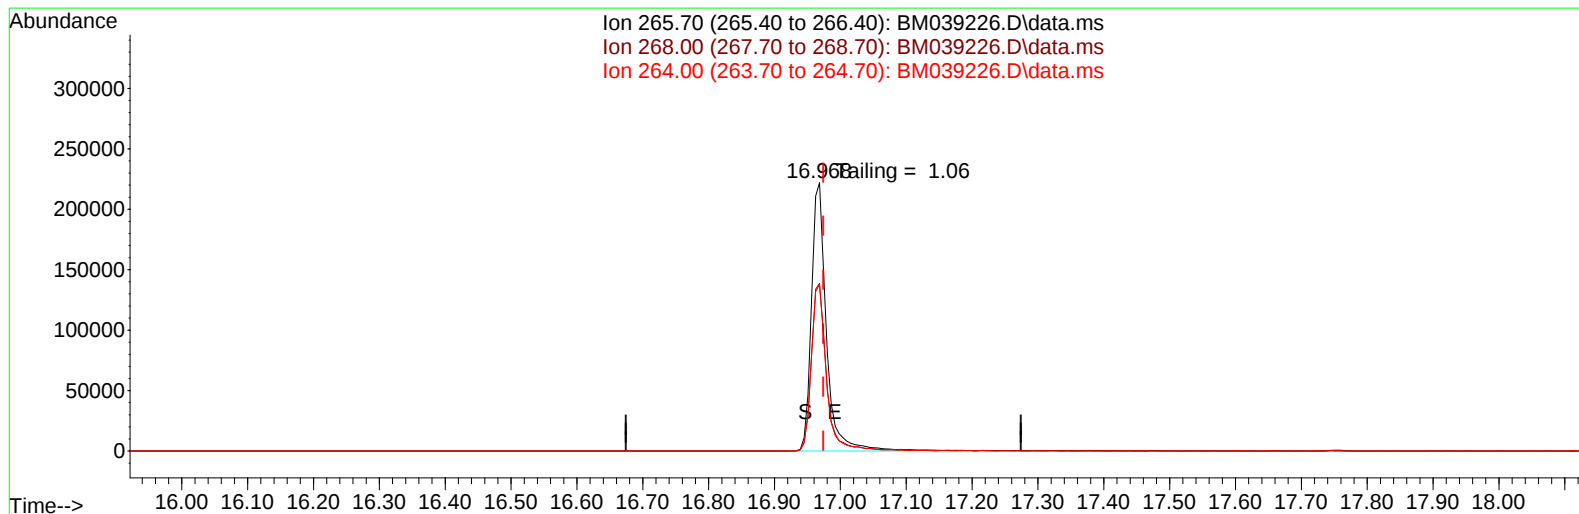

TIC: BM039226.D\data.ms

(70) Pentachlorophenol (C)




16.968min (-0.006) 0.00 ng

response 351312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	62.51
264.00	62.80	61.99
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\  
Data File : BM039226.D  
Acq On    : 30 Mar 2023  14:46  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 31 05:03:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 30 05:15:45 2023
Response via : Initial Calibration

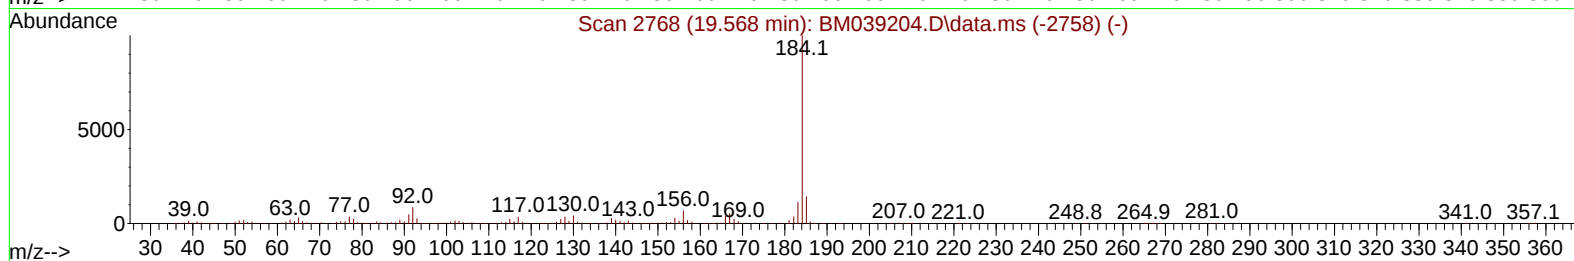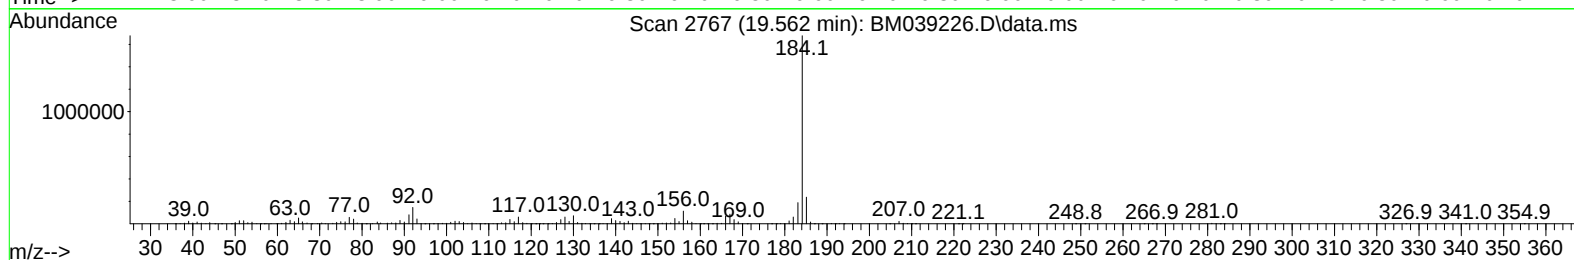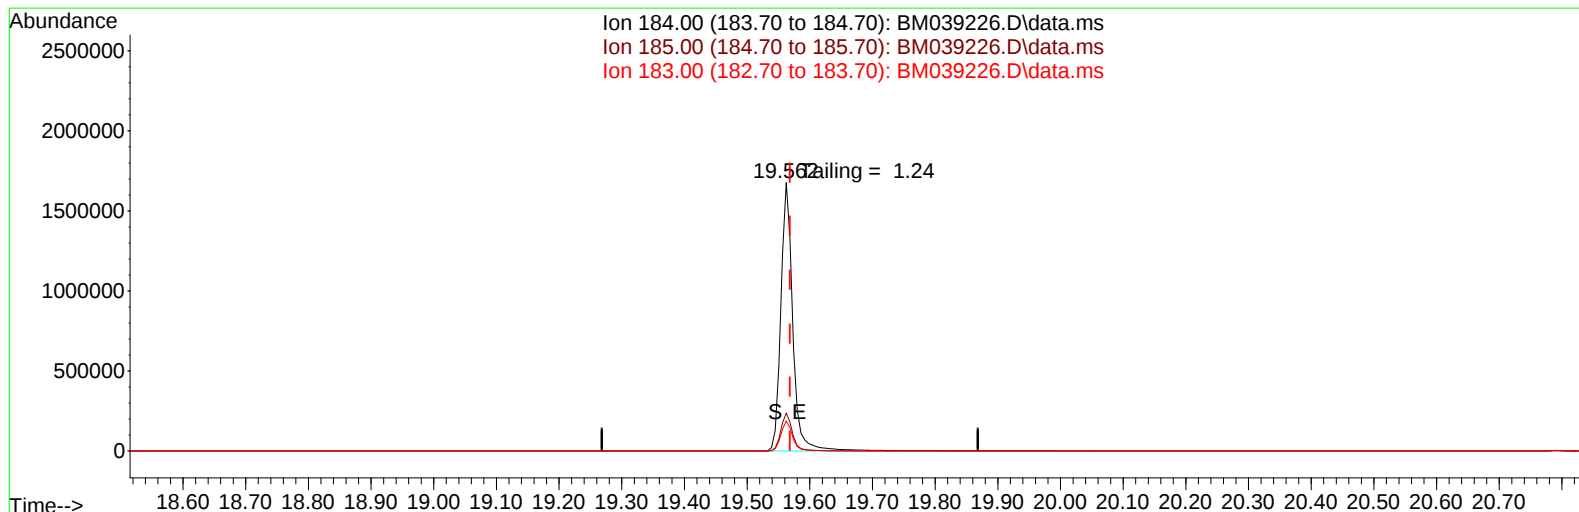

TIC: BM039226.D\data.ms

(77) Benzidine

19.562min (-0.006) 139149.98 ng

response **2235199**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.18
183.00	11.20	11.22
0.00	0.00	0.00