

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
 Data File : BM039220.D
 Acq On : 30 Mar 2023 09:58
 Operator : CG/JU
 Sample : PB151693BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB151693BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM039220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	288	294	302	rBV	2469933	3300462	26.35%	4.853%
2	5.481	367	373	393	rVB	5584837	8182252	65.33%	12.030%
3	7.093	638	647	664	rBV	5108312	7981076	63.72%	11.734%
4	7.922	781	788	798	rVB	989928	1542979	12.32%	2.269%
5	9.093	977	987	1004	rBV	3100234	5069748	40.48%	7.454%
6	10.734	1258	1266	1277	rBV	1199619	2005502	16.01%	2.949%
7	13.192	1677	1684	1699	rBV	7026048	10349300	82.63%	15.216%
8	14.569	1910	1918	1930	rBV	1618251	2371102	18.93%	3.486%
9	16.057	2164	2171	2200	rBV	4663381	6896662	55.07%	10.140%
10	17.316	2379	2385	2400	rBV	1820858	2568376	20.51%	3.776%
11	19.939	2825	2831	2845	rBV	10461303	12524429	100.00%	18.414%
12	21.498	3091	3096	3107	rBV	1925531	2597585	20.74%	3.819%
13	23.915	3501	3507	3516	rVB2	1294817	2625472	20.96%	3.860%




Sum of corrected areas: 68014945

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
Data File : BM039220.D
Acq On : 30 Mar 2023 09:58
Operator : CG/JU
Sample : PB151693BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151693BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

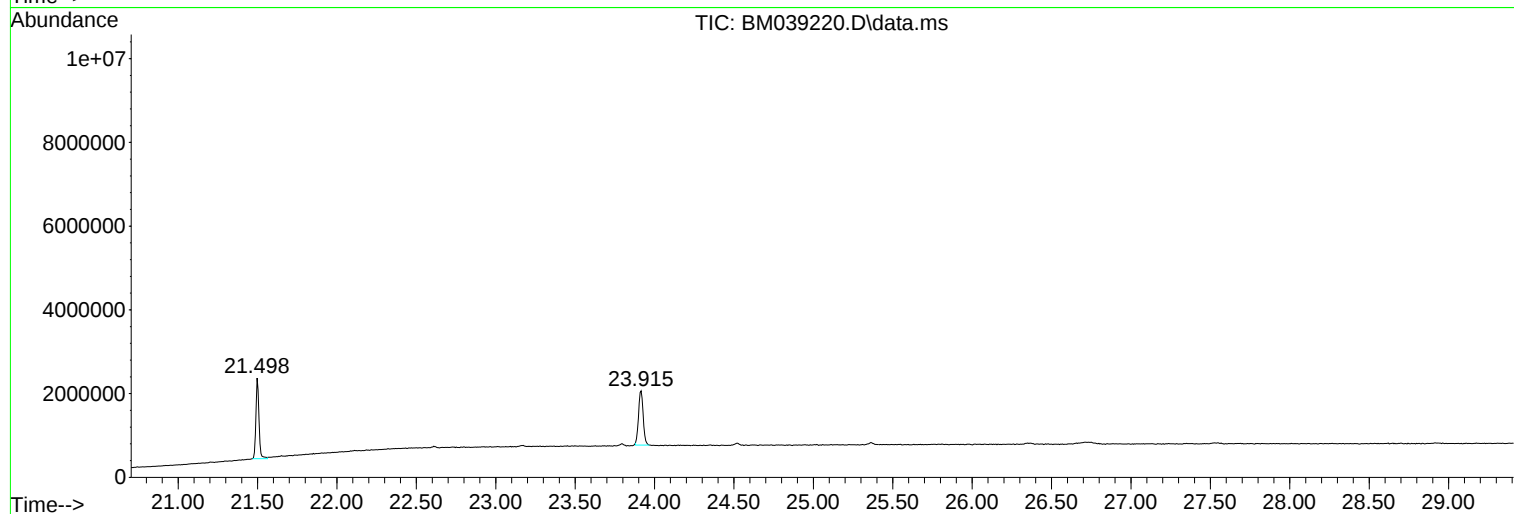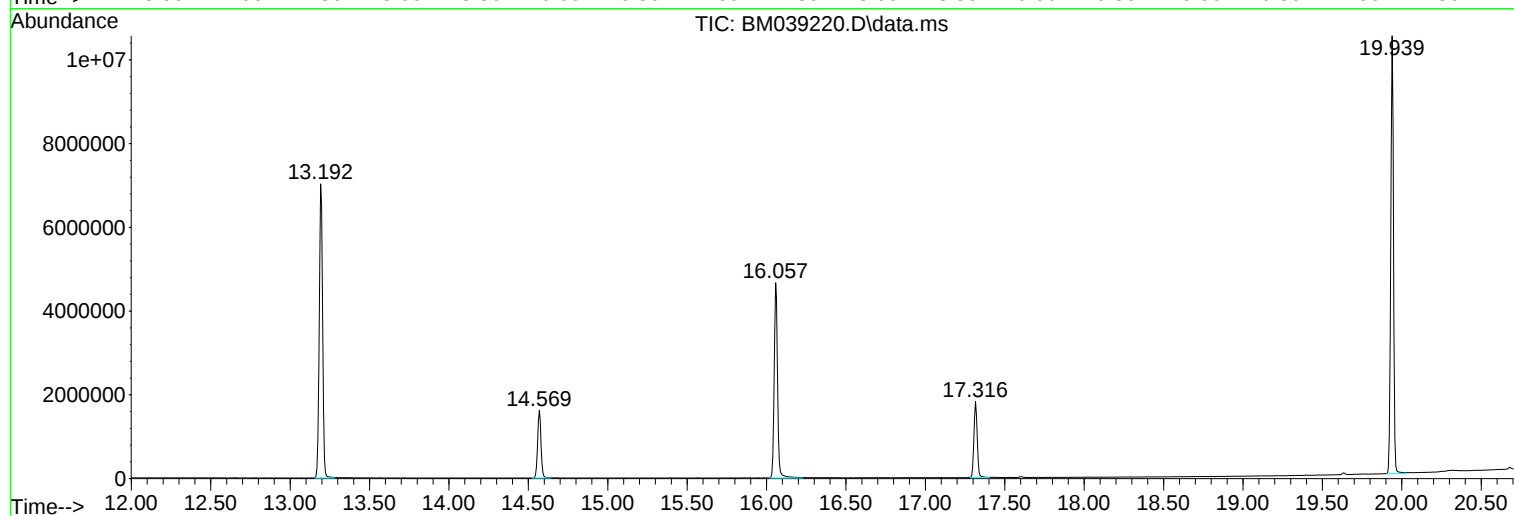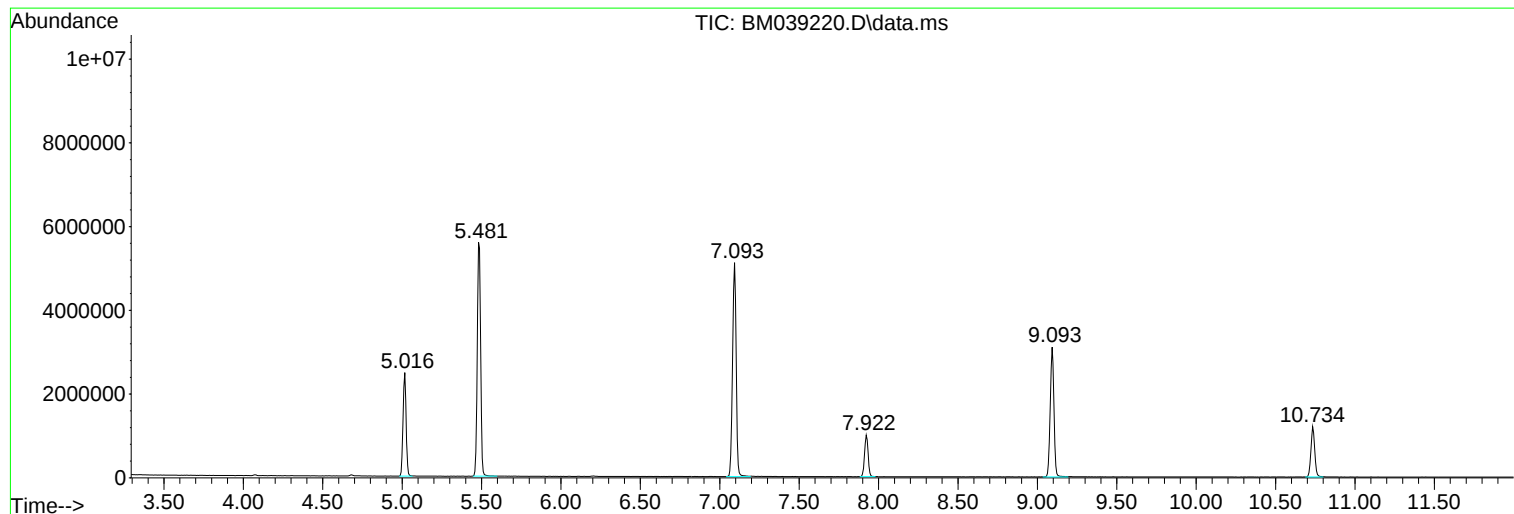

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
Data File : BM039220.D
Acq On : 30 Mar 2023 09:58
Operator : CG/JU
Sample : PB151693BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151693BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.016	42.78 ng	3300460	1,4-Dichlorobenzene-d4	7.922

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

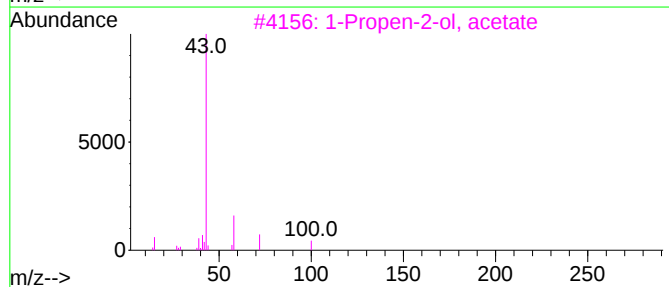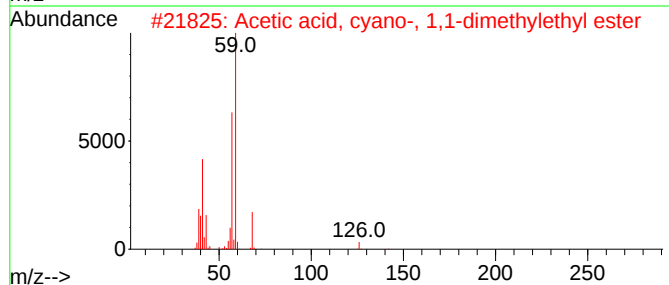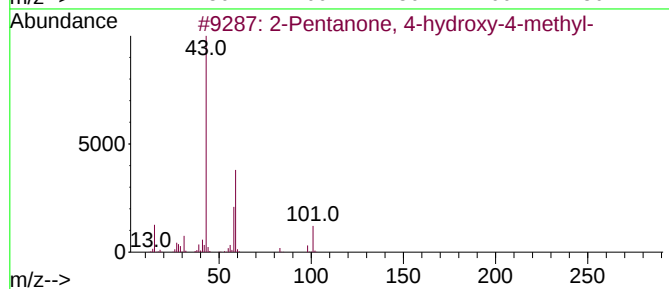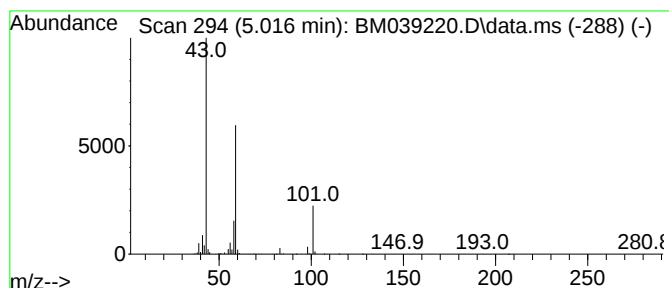

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
Data File : BM039220.D
Acq On : 30 Mar 2023 09:58
Operator : CG/JU
Sample : PB151693BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151693BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.016	42.8	ng	3300460	1	7.922	1542980	20.0