


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
Data File : BM039218.D
Acq On : 30 Mar 2023 08:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 30 05:15:45 2023

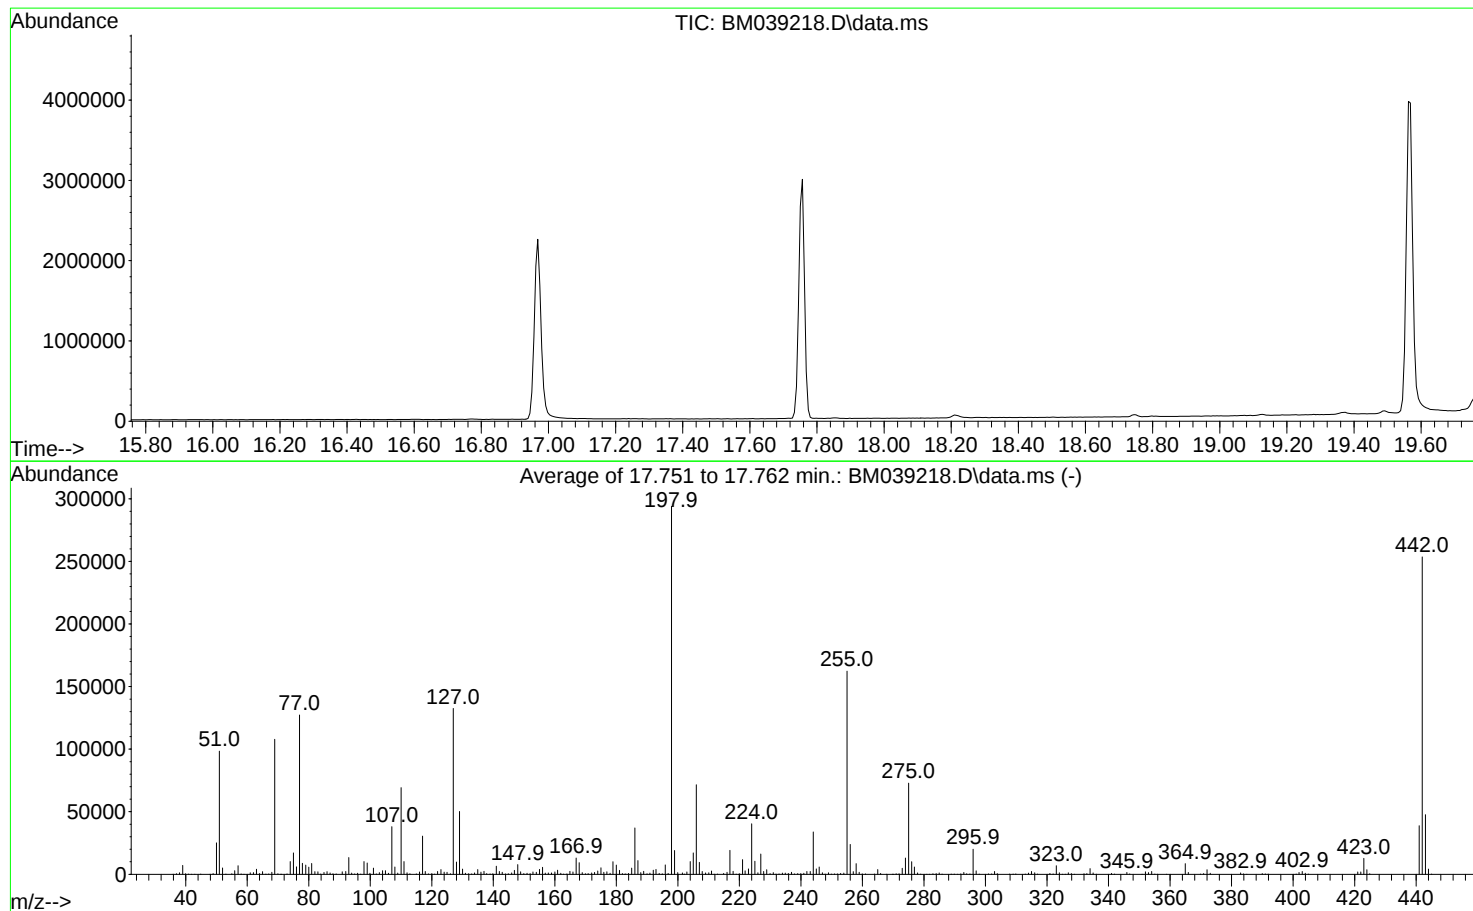




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	98434	PASS
68	69	0.00	2	1.5	1596	PASS
69	198	0.00	100	36.7	107849	PASS
70	69	0.00	2	0.4	450	PASS
127	198	10	80	45.1	132563	PASS
197	198	0.00	2	0.3	753	PASS
198	198	100	100	100.0	293952	PASS
199	198	5	9	6.4	18942	PASS
275	198	10	60	24.8	72872	PASS
365	198	1	100	2.9	8512	PASS
441	198	0.01	100	13.2	38832	PASS
442	442	50	100	100.0	253675	PASS
443	442	15	24	18.8	47584	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
Data File : BM039218.D
Acq On : 30 Mar 2023 08:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 31 05:05:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 30 05:15:45 2023
Response via : Initial Calibration

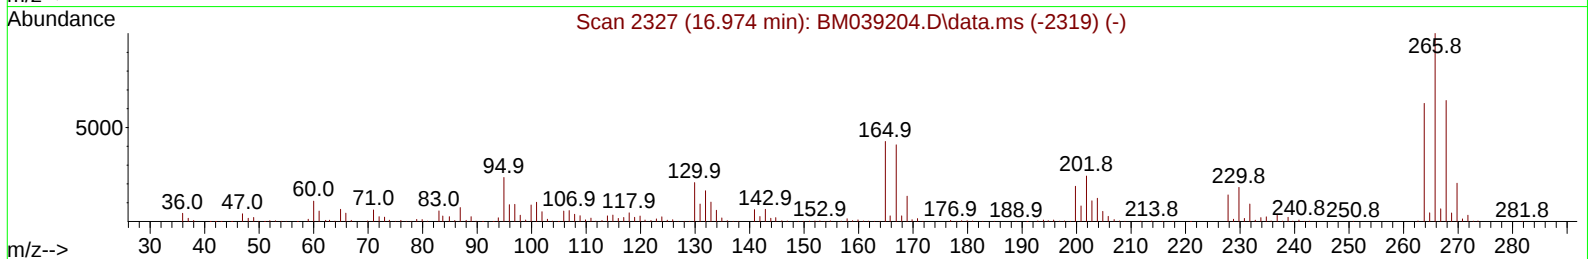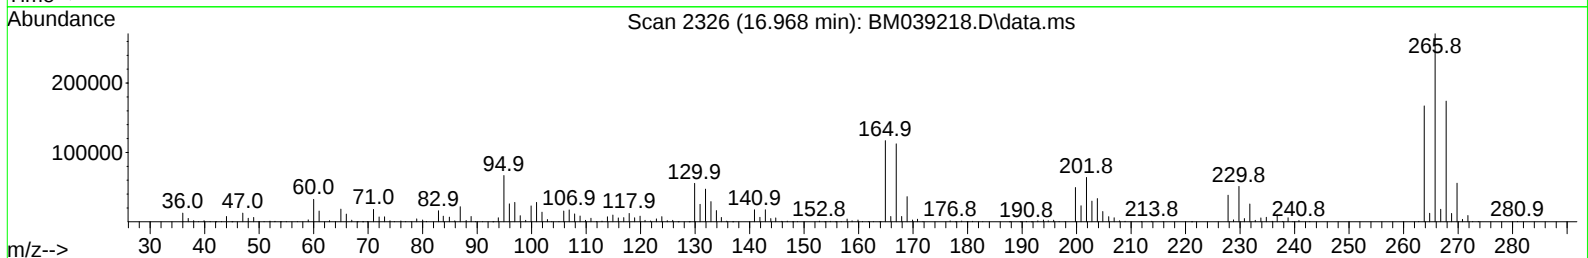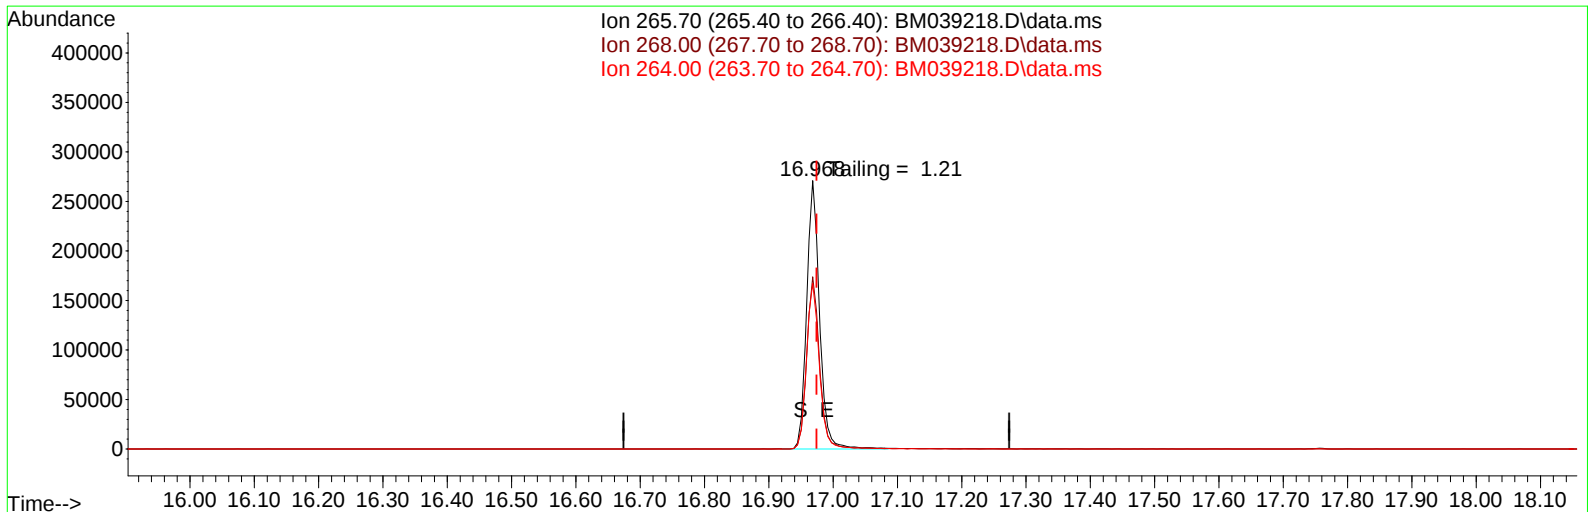

TIC: BM039218.D\data.ms

(70) Pentachlorophenol (C)

16.968min (-0.006) 64820.80 ng




response 380733

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.18
264.00	62.80	61.65
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\  
Data File : BM039218.D  
Acq On    : 30 Mar 2023  08:45  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 31 05:05:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 30 05:15:45 2023
Response via : Initial Calibration

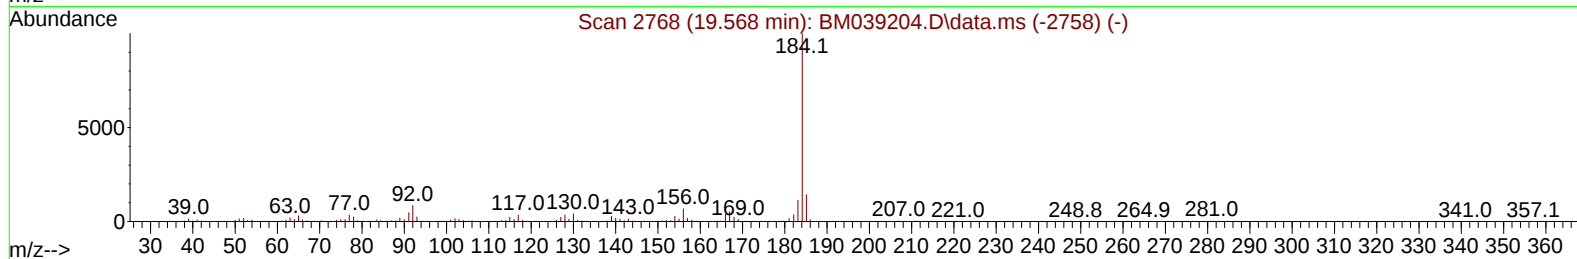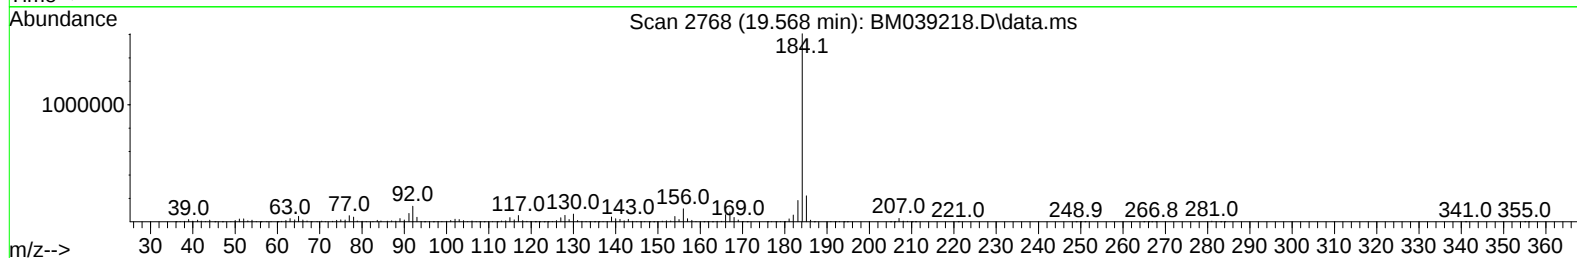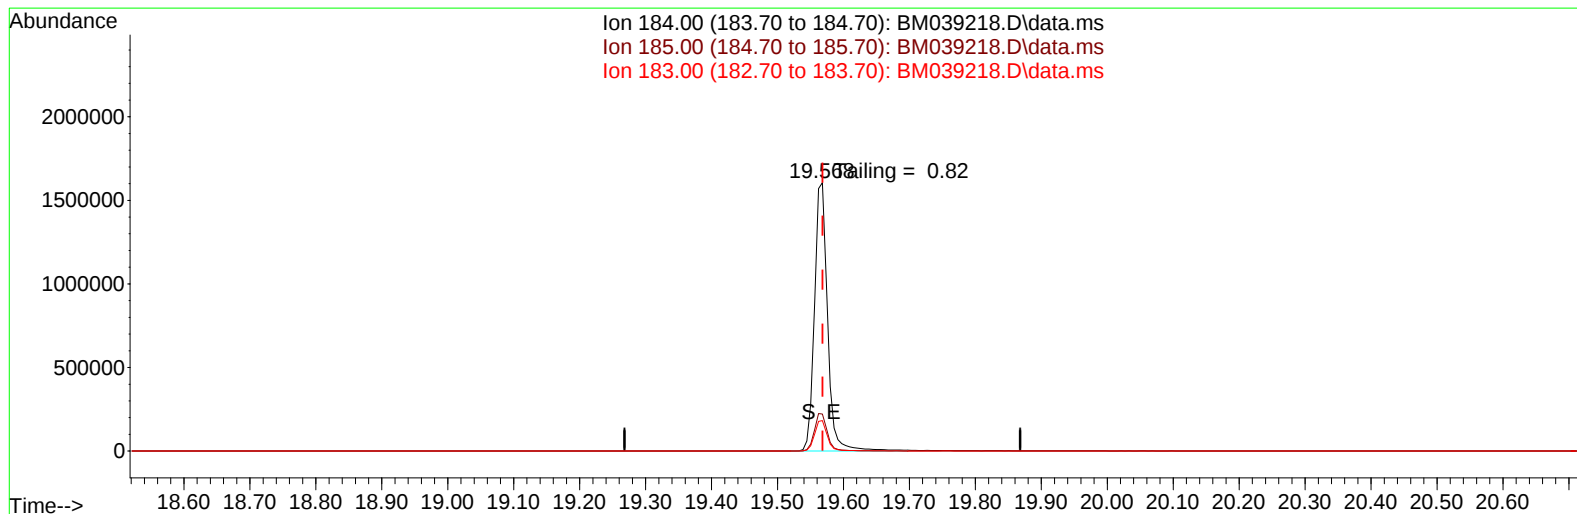

TIC: BM039218.D\data.ms

(77) Benzidine

19.568min (-0.000) 5440.98 ng

response **2214845**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.78
183.00	11.20	11.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/30/2023	BNA_M	<u>BM039218.D</u>
Compound Name	Response	Retention Time
DDT	1030291	20.797
DDD	13144	20.409
DDE	1018	19.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14162	1044453	1.36

Instrument :
BNA_M
ClientSampleId :
DFTPP