
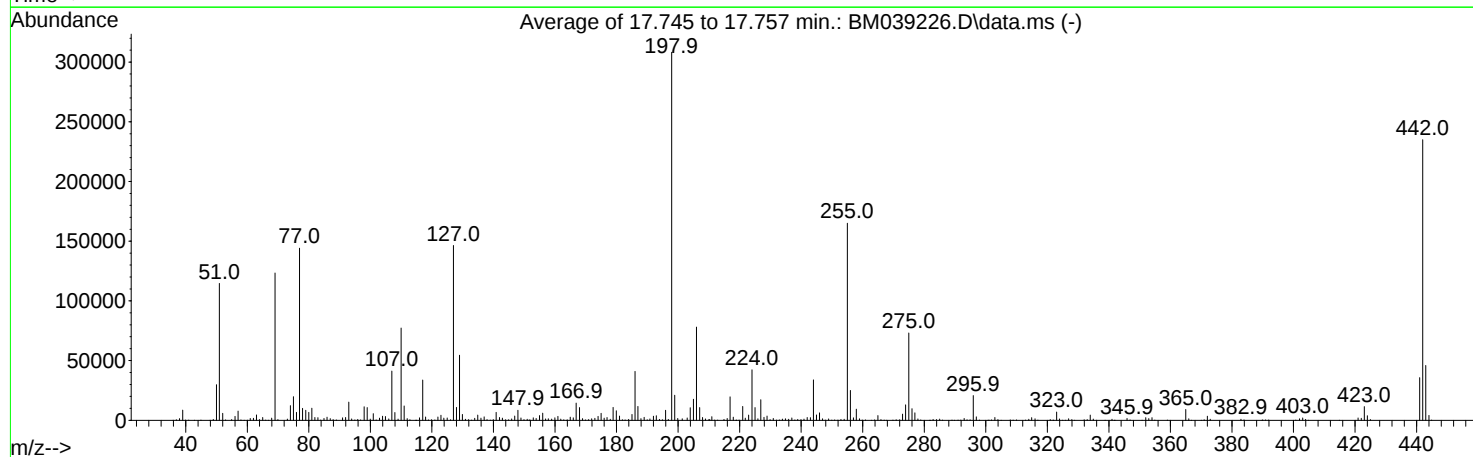


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
Data File : BM039226.D
Acq On : 30 Mar 2023 14:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 30 05:15:45 2023

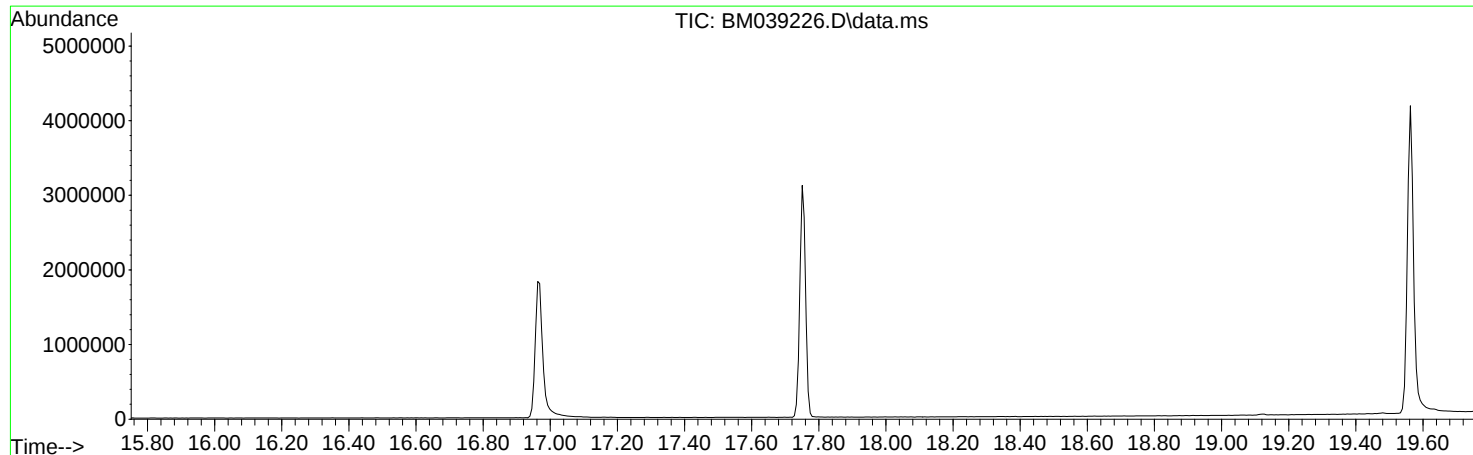




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	114626	PASS
68	69	0.00	2	1.5	1795	PASS
69	198	0.00	100	40.0	123362	PASS
70	69	0.00	2	0.5	600	PASS
127	198	10	80	47.5	146357	PASS
197	198	0.00	2	0.3	783	PASS
198	198	100	100	100.0	308096	PASS
199	198	5	9	6.8	21013	PASS
275	198	10	60	23.8	73179	PASS
365	198	1	100	2.9	9004	PASS
441	198	0.01	100	11.6	35715	PASS
442	442	50	100	100.0	235051	PASS
443	442	15	24	19.5	45880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
Data File : BM039226.D
Acq On : 30 Mar 2023 14:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 31 05:03:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 30 05:15:45 2023
Response via : Initial Calibration

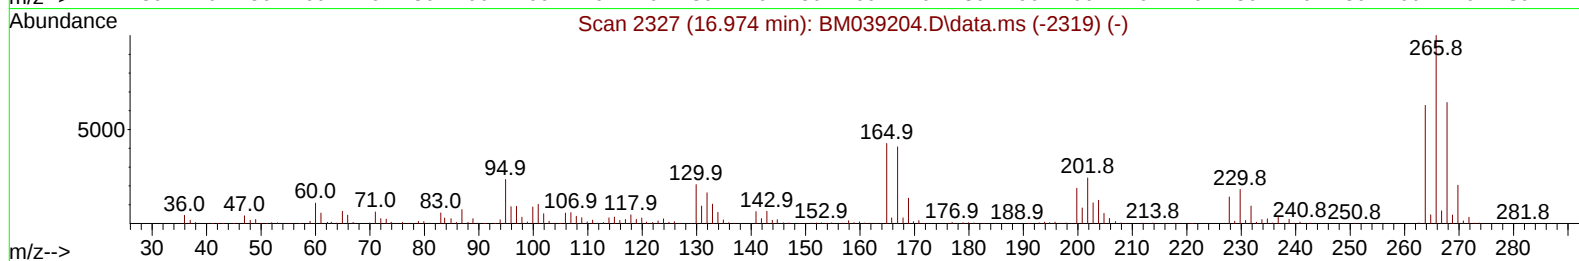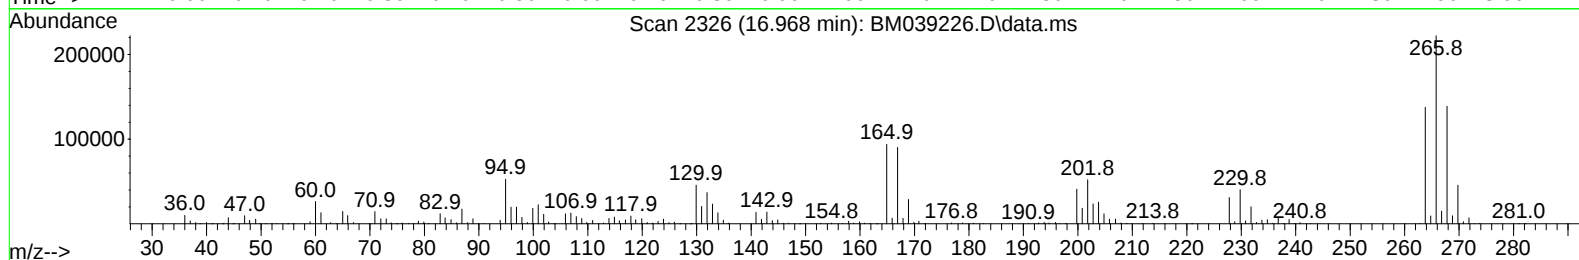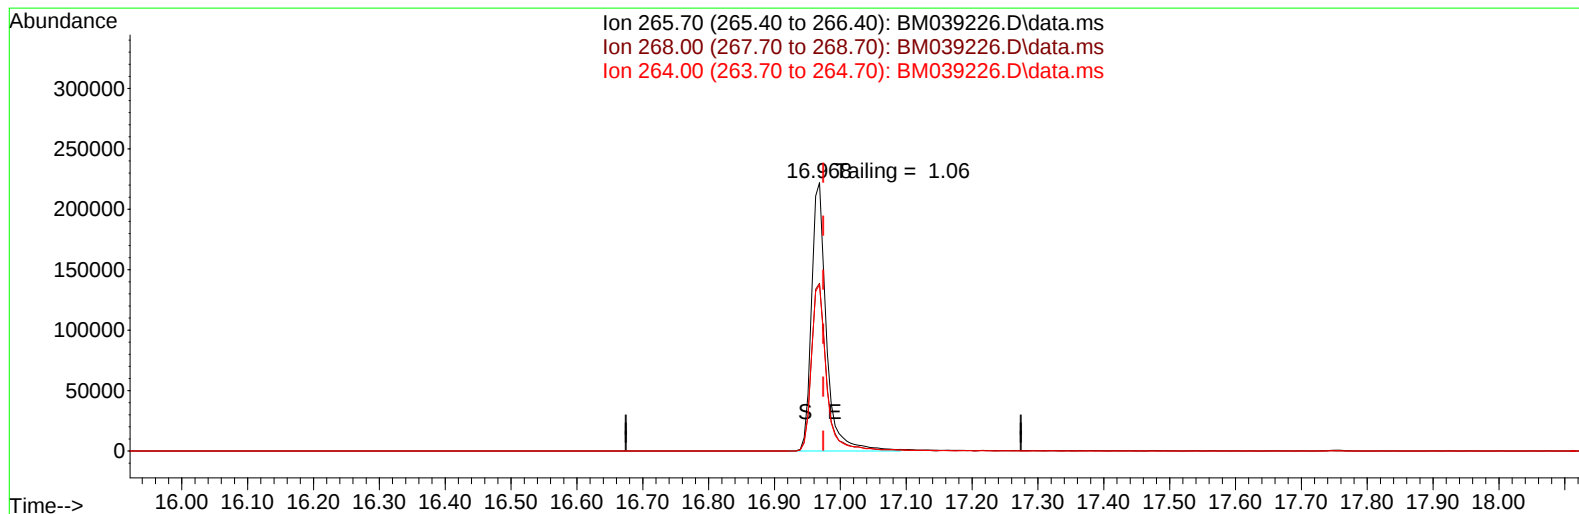

TIC: BM039226.D\data.ms

(70) Pentachlorophenol (C)

16.968min (-0.006) 0.00 ng




response 351312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	62.51
264.00	62.80	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033023\
 Data File : BM039226.D
 Acq On : 30 Mar 2023 14:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 31 05:03:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 30 05:15:45 2023
 Response via : Initial Calibration

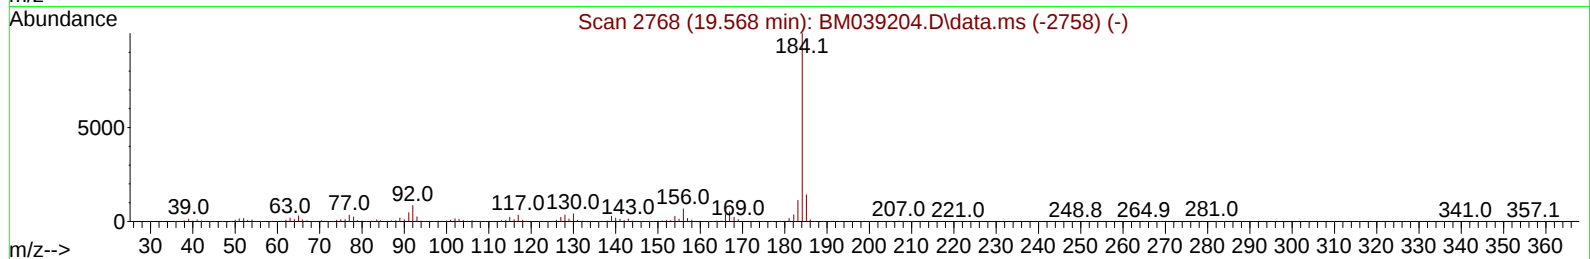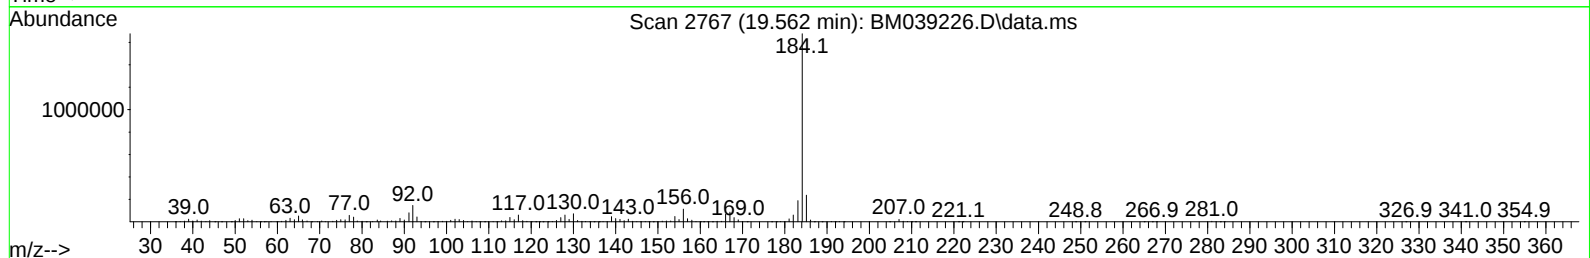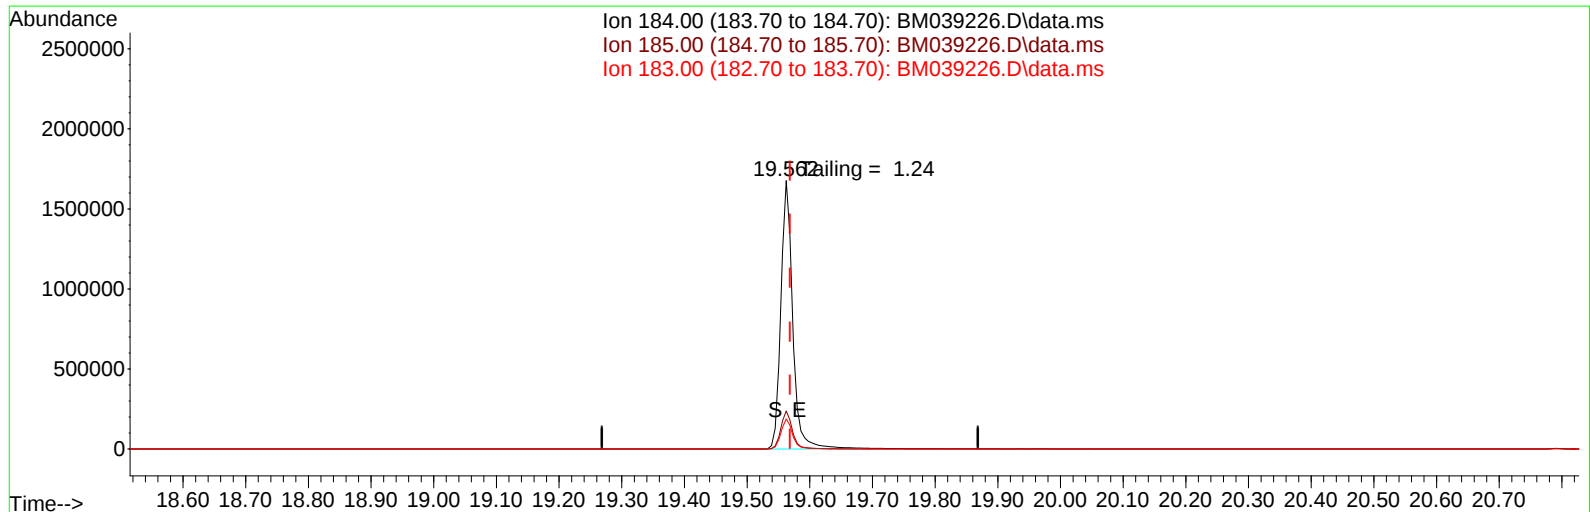

TIC: BM039226.D\data.ms

(77) Benzidine

19.562min (-0.006) 139149.98 ng

response 2235199

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.18
183.00	11.20	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/30/2023	BNA_M	<u>BM039226.D</u>
Compound Name	Response	Retention Time
DDT	1060474	20.792
DDD	11969	20.403
DDE	554	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12523	1072997	1.17

Instrument :
BNA_M
ClientSampleId :
DFTPP