


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM033115\
Data File : BM000776.D
Acq On : 01 Apr 2015 04:58
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM033115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 01 04:17:30 2015

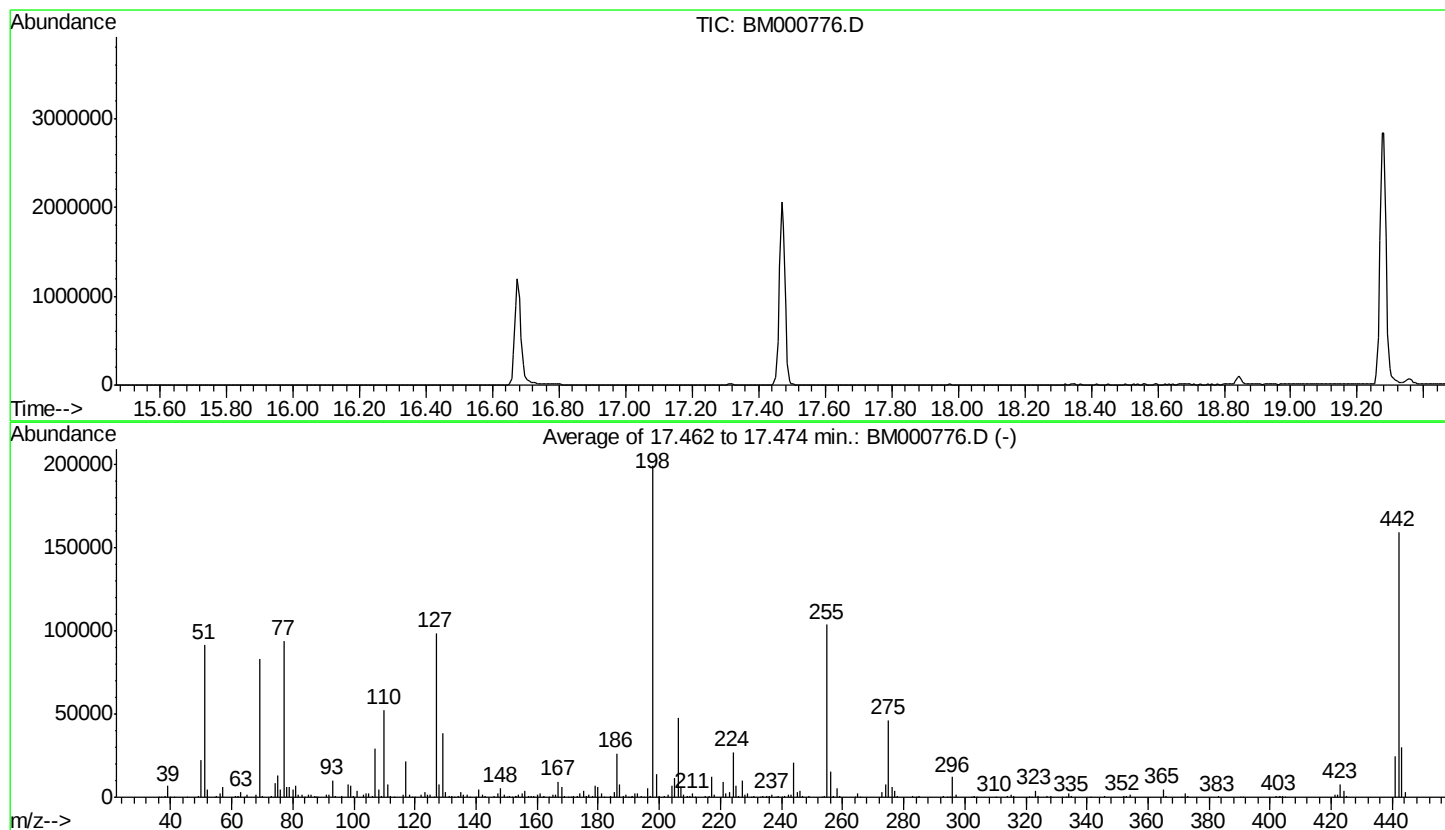

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	91469	PASS
68	69	0.00	2	1.5	1264	PASS
69	198	0.00	100	41.5	82648	PASS
70	69	0.00	2	0.6	459	PASS
127	198	10	80	49.6	98602	PASS
197	198	0.00	2	0.4	727	PASS
198	198	100	100	100.0	198954	PASS
199	198	5	9	6.8	13570	PASS
275	198	10	60	23.2	46253	PASS
365	198	1	100	2.4	4836	PASS
441	442	0.01	24	15.2	24283	PASS
442	198	50	100	80.1	159306	PASS
443	442	15	24	18.8	29968	PASS