


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM033115\
 Data File : BM000758.D
 Acq On : 31 Mar 2015 17:27
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM033115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 01 04:17:30 2015

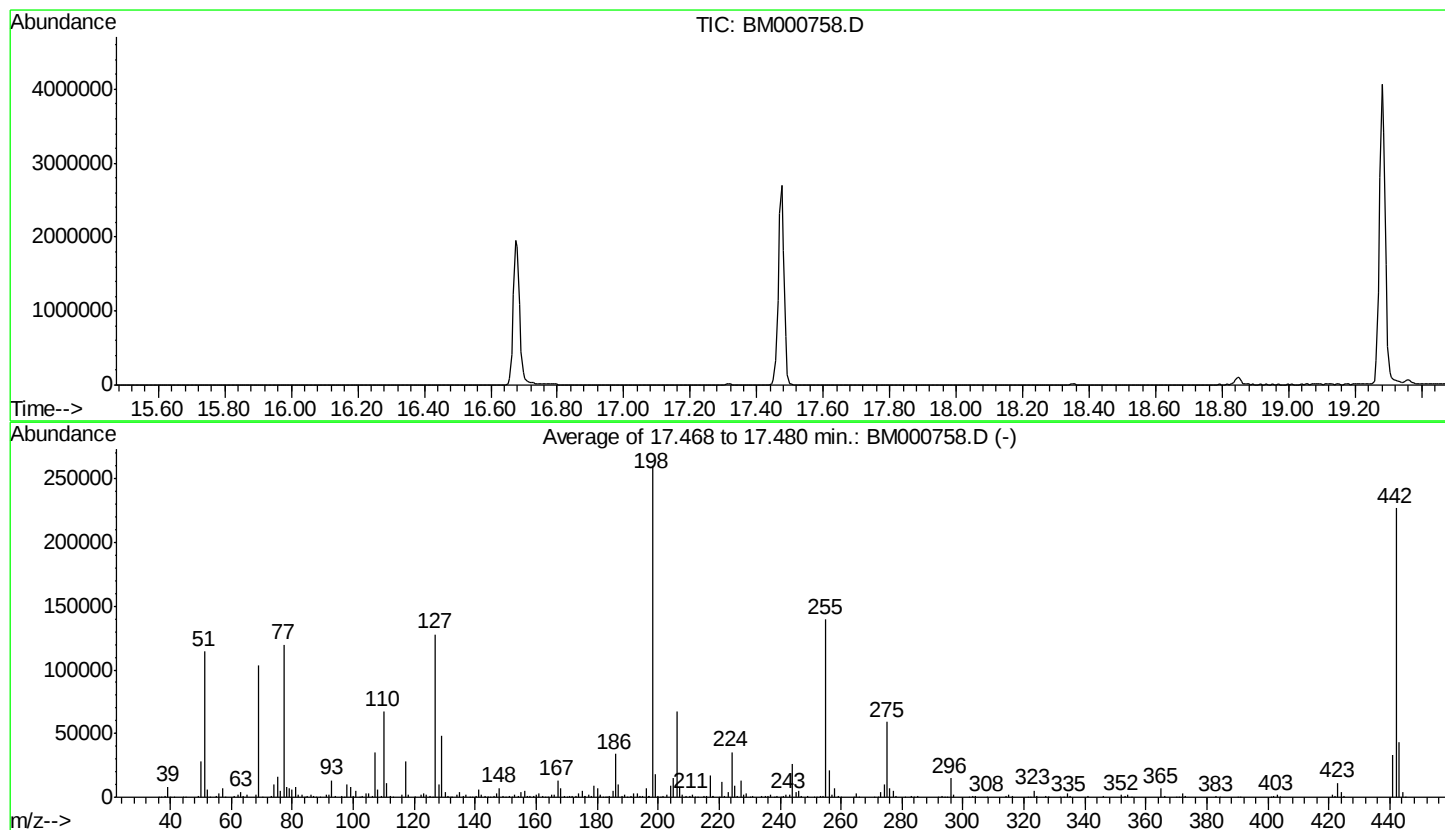

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	114258	PASS
68	69	0.00	2	1.6	1700	PASS
69	198	0.00	100	39.9	103818	PASS
70	69	0.00	2	0.4	433	PASS
127	198	10	80	49.0	127682	PASS
197	198	0.00	2	0.3	869	PASS
198	198	100	100	100.0	260416	PASS
199	198	5	9	6.8	17675	PASS
275	198	10	60	22.7	59128	PASS
365	198	1	100	2.7	6942	PASS
441	442	0.01	24	14.7	33464	PASS
442	198	50	100	87.1	226880	PASS
443	442	15	24	19.2	43536	PASS