
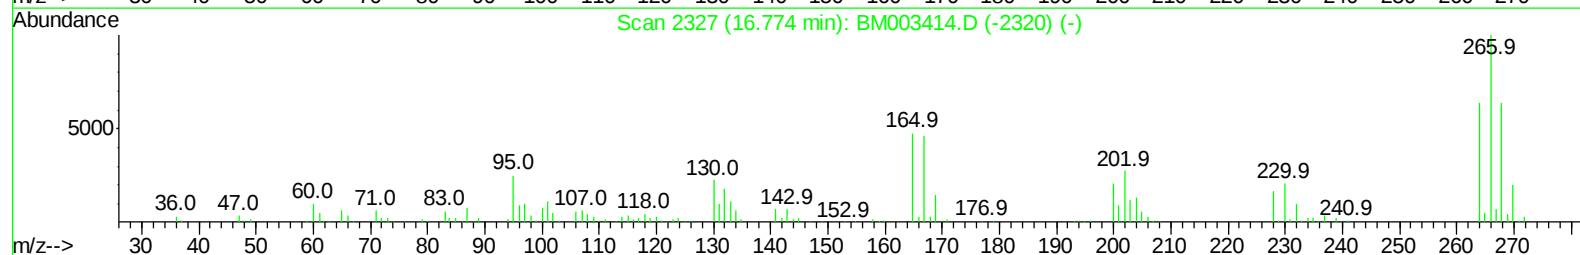
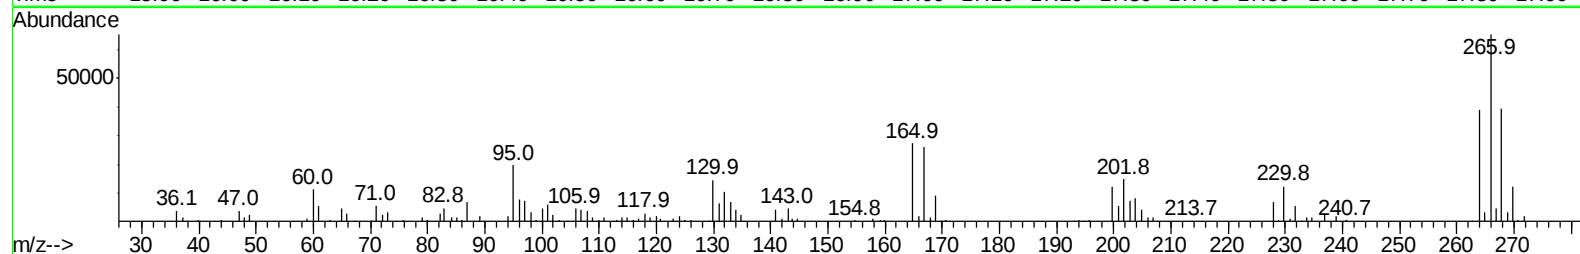


Data Path : Z:\HPCHEM1\BNA M\Data\BM033117\  
Data File : BM009486.D  
Acq On : 31 Mar 2017 22:33  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 04:54:48 2017  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 31 12:10:26 2017  
Response via : Initial Calibration

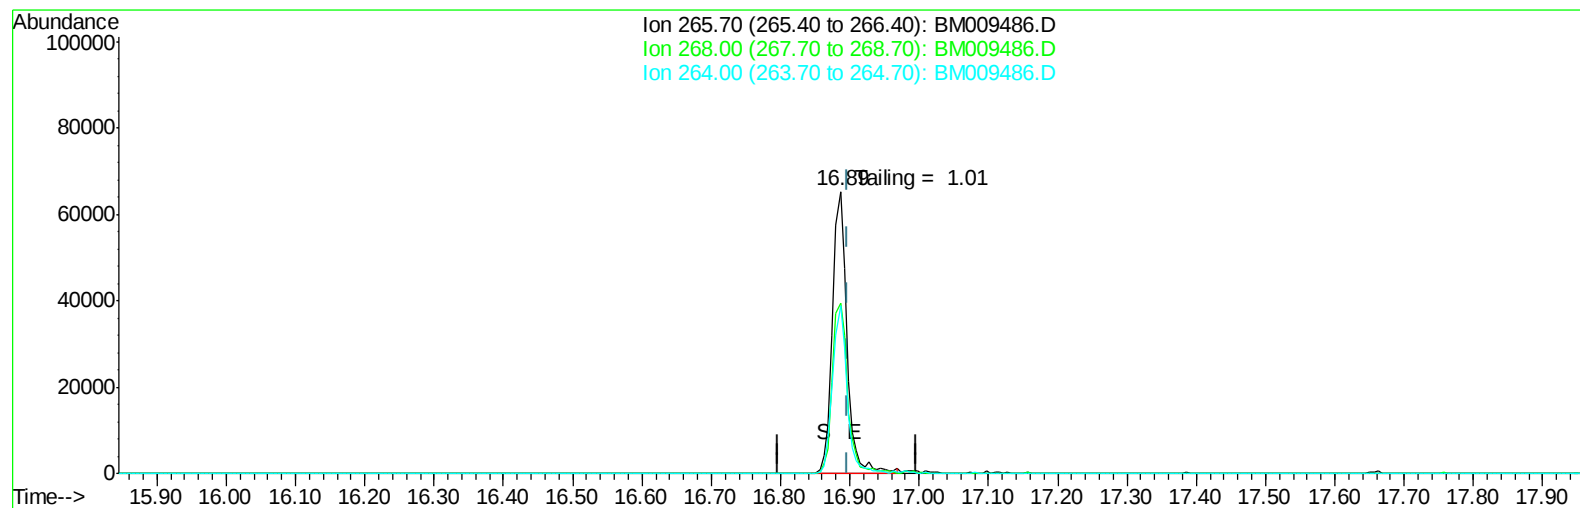

TIC: BM009486.D

(69) Pentachlorophenol (C)




16.886min (-0.012) 0.00ng

response 93778

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.00 | 60.47 |
| 264.00 | 61.20 | 59.62 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA M\Data\BM033117\  
Data File : BM009486.D  
Acq On : 31 Mar 2017 22:33  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 04:54:48 2017  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 31 12:10:26 2017  
Response via : Initial Calibration

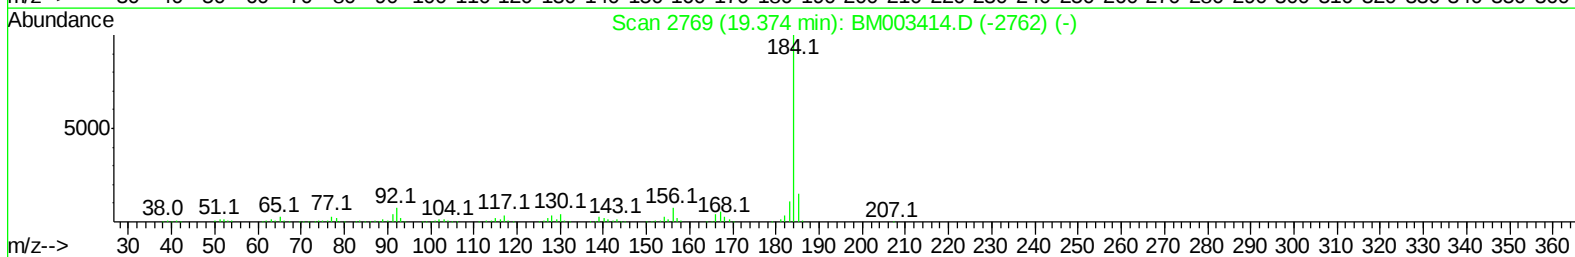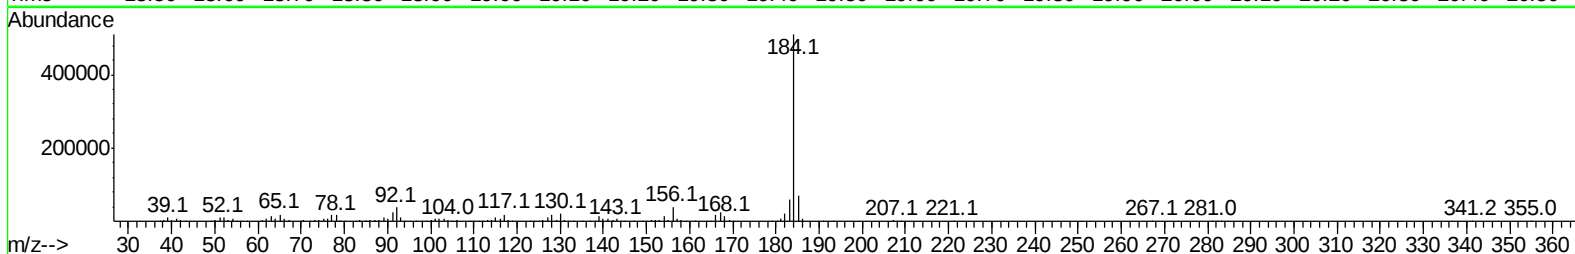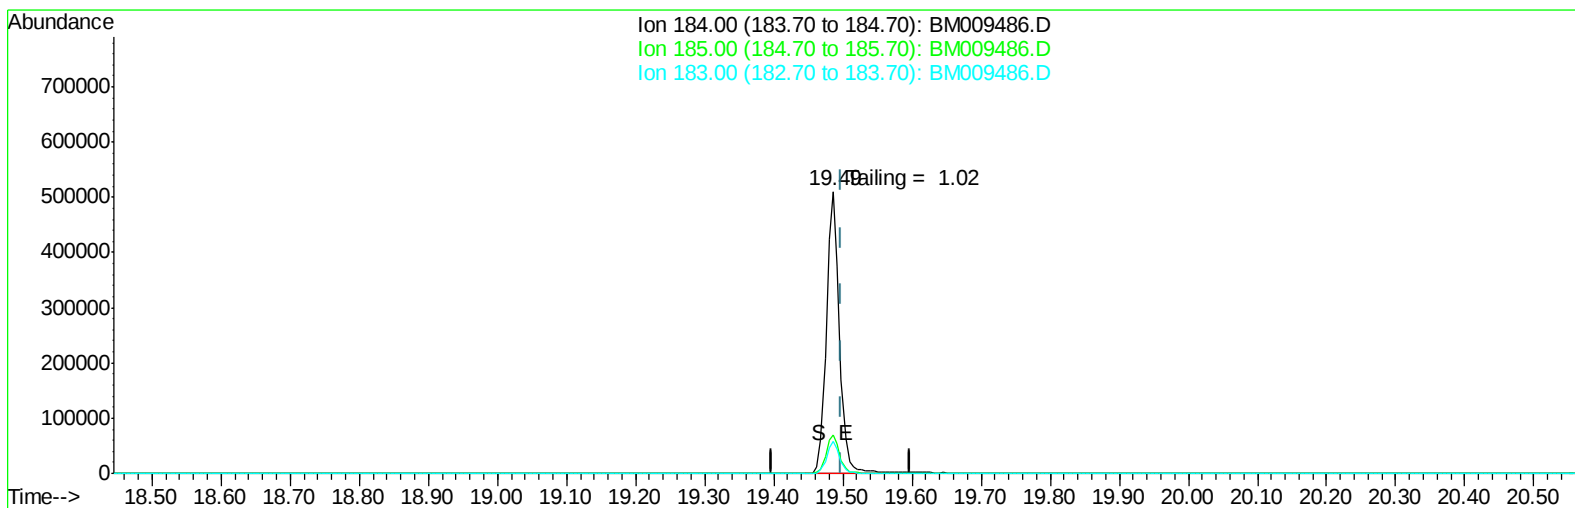

TIC: BM009486.D

(76) Benzidine

19.486min (-0.012) 23737.94ng

response 667851

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.10 | 13.60 |
| 183.00 | 11.10 | 11.44 |
| 0.00   | 0.00  | 0.00  |