

Data Path : Z:\HPCHEM1\BNA M\DATA\BM033117\
 Data File : BM009483.D
 Acq On : 31 Mar 2017 20:46
 Operator : SJ/MA
 Sample : I2462-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WELL-A

Quant Time: Mar 31 23:00:38 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 12:10:26 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	108697	20.00	ng	-0.02
21) Naphthalene-d8	10.65	136	405013	20.00	ng	-0.02
38) Acenaphthene-d10	14.49	164	234358	20.00	ng	-0.02
63) Phenanthrene-d10	17.24	188	544309	20.00	ng	-0.01
75) Chrysene-d12	21.42	240	752230	20.00	ng	-0.01
86) Perylene-d12	23.74	264	731633	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	410323	62.92	ng	-0.01
7) Phenol-d6	7.00	99	323675	36.40	ng	-0.02
23) Nitrobenzene-d5	9.01	82	1123274	103.99	ng	-0.02
41) 2,4,6-Tribromophenol	15.98	330	500952	172.06	ng	-0.02
44) 2-Fluorobiphenyl	13.10	172	2064615	106.15	ng	-0.02
78) Terphenyl-d14	19.86	244	2750029	76.39	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM033117\
Data File : BM009483.D
Acq On : 31 Mar 2017 20:46
Operator : SJ/MA
Sample : I2462-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WELL-A

Quant Time: Mar 31 23:00:38 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 12:10:26 2017
Response via : Initial Calibration

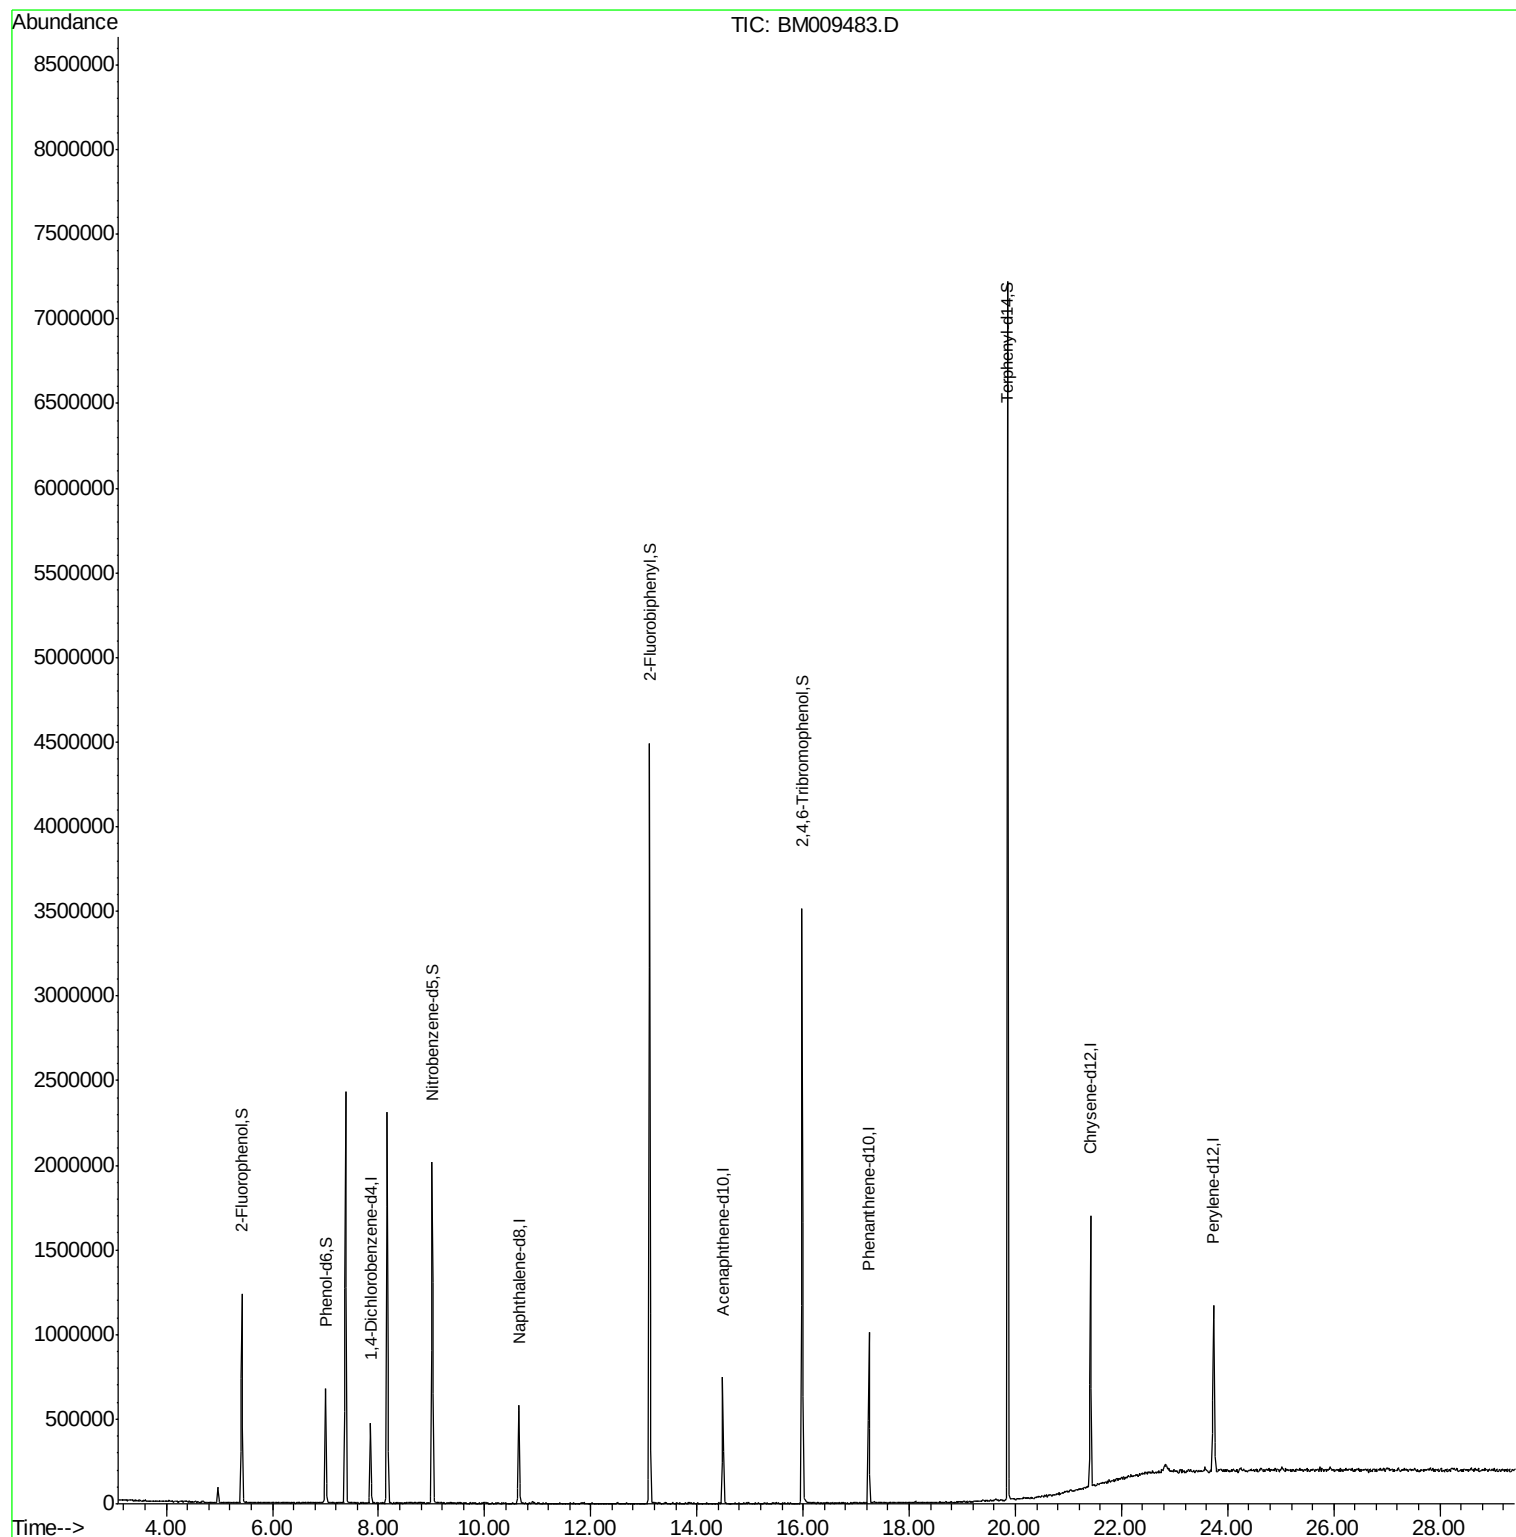

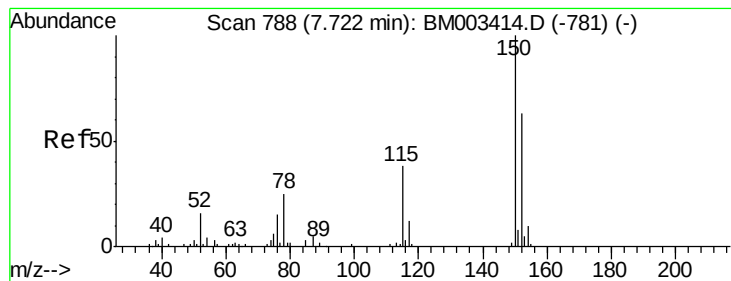


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.85 min Scan# 809
Delta R.T. -0.02 min
Lab File: BM009483.D
Acq: 31 Mar 2017 20:46

Instrument :
BNA_M
ClientSampleId :
WELL-A

Tot Ion	152	Resp	108697
Ion	Ratio	Lower	Upper
152	100		
150	153.6	119.5	179.3
115	63.0	43.0	64.4

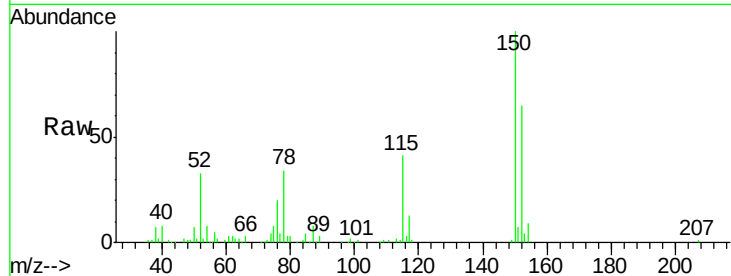


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

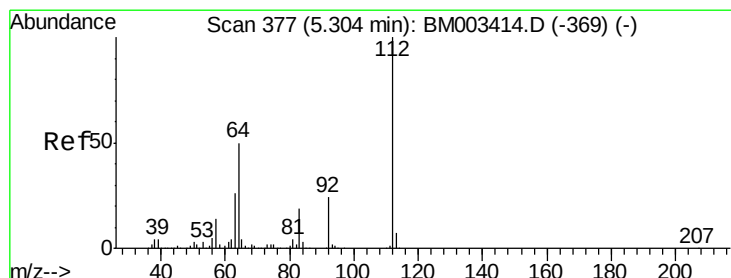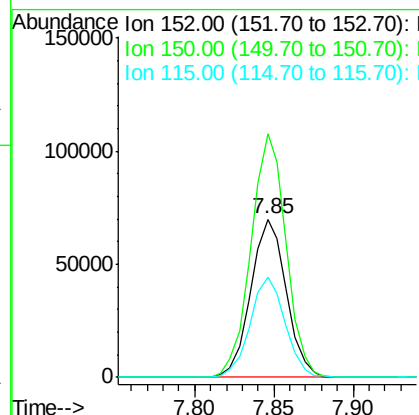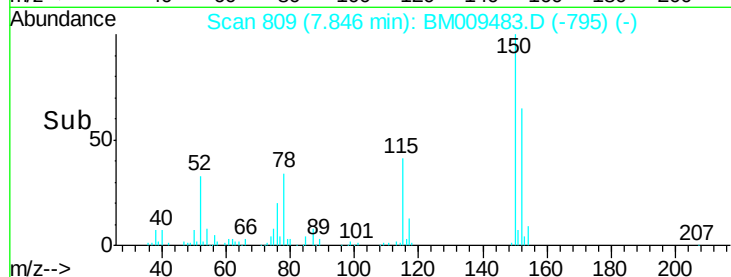



#5


2-Fluorophenol
Concen: 62.92 ng
RT: 5.42 min Scan# 397
Delta R.T. -0.01 min
Lab File: BM009483.D
Acq: 31 Mar 2017 20:46

Tgt Ion	112	Resp	410323
Ion	Ratio	Lower	Upper
112	100		
64	75.0	38.6	57.8#
63	40.4	19.3	28.9#

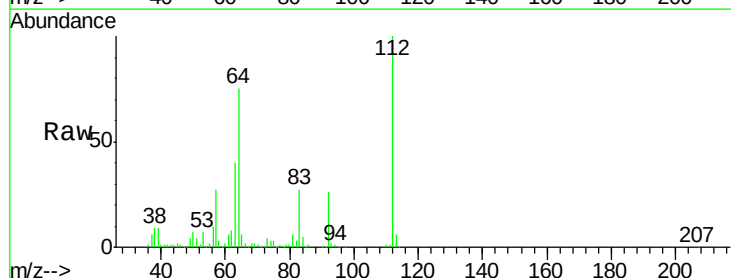

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

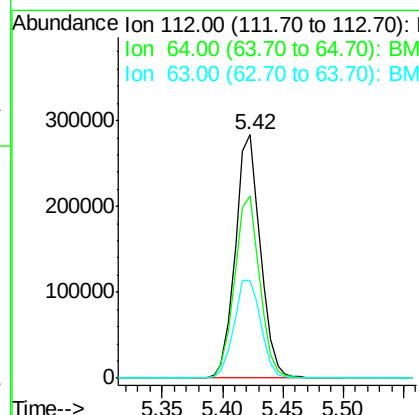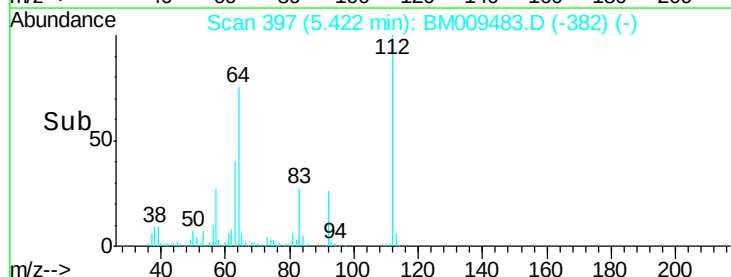

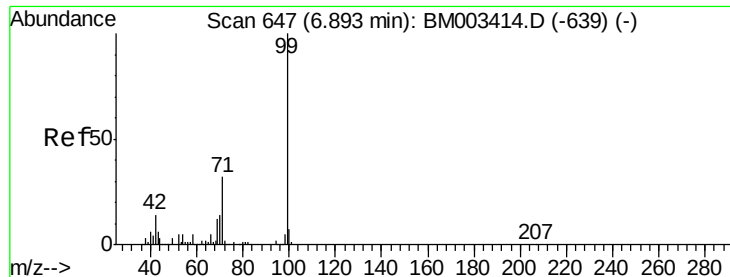

#7

Phenol-d6

Concen: 36.40 ng

RT: 7.00 min Scan# 666

Delta R.T. -0.02 min

Lab File: BM009483.D

Acq: 31 Mar 2017 20:46

Instrument :

BNA_M

ClientSampleId :

WELL-A


Tot Ion: 99 Resp: 323675

Ion Ratio Lower Upper

99 100

42 25.3 11.0 16.4#

71 41.2 23.4 35.2#



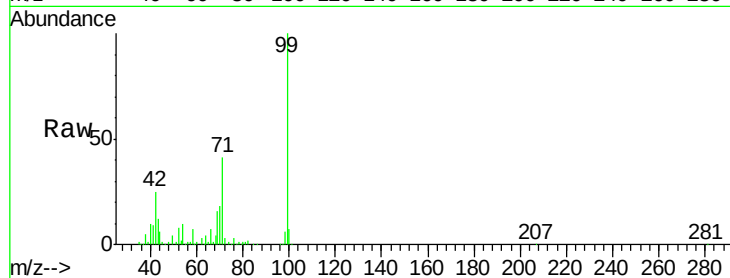


Abundance Ion 99.00 (98.70 to 99.70): BM003414.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM003414.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM003414.D (-639) (-)

Time-->

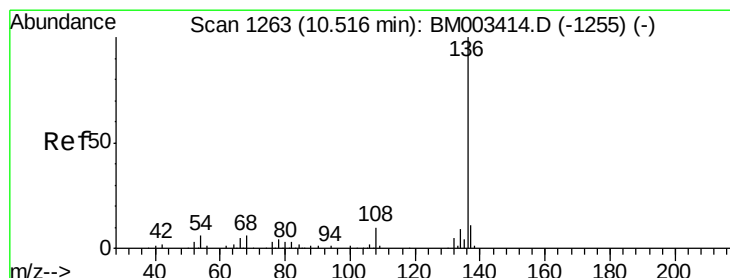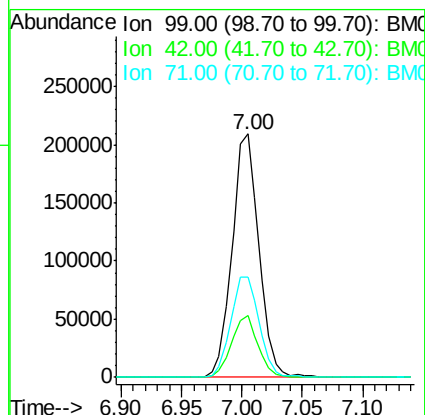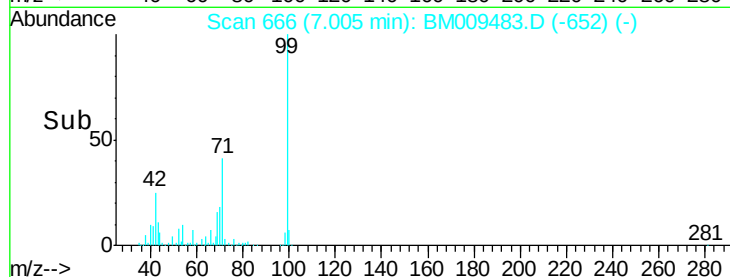

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.65 min Scan# 1285

Delta R.T. -0.02 min

Lab File: BM009483.D

Acq: 31 Mar 2017 20:46

Tgt Ion: 136 Resp: 405013


Ion Ratio Lower Upper

136 100

137 11.6 8.7 13.1

54 11.3 4.6 6.8#

68 7.4 3.7 5.5#

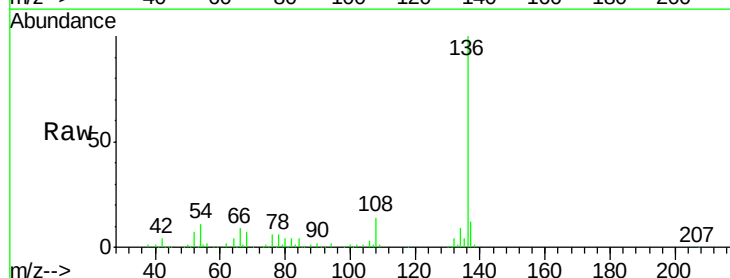



Abundance Ion 136.00 (135.70 to 136.70): BM003414.D (-1255) (-)


Ion 137.00 (136.70 to 137.70): BM003414.D (-1255) (-)

Ion 54.00 (53.70 to 54.70): BM003414.D (-1255) (-)

Ion 68.00 (67.70 to 68.70): BM003414.D (-1255) (-)

Time-->



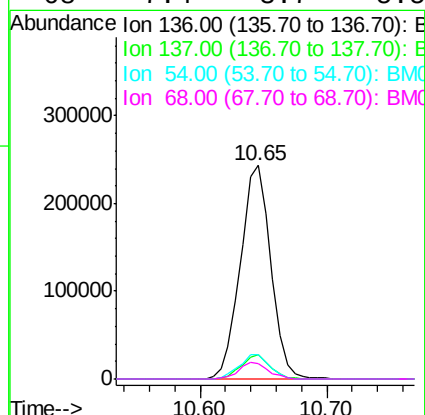
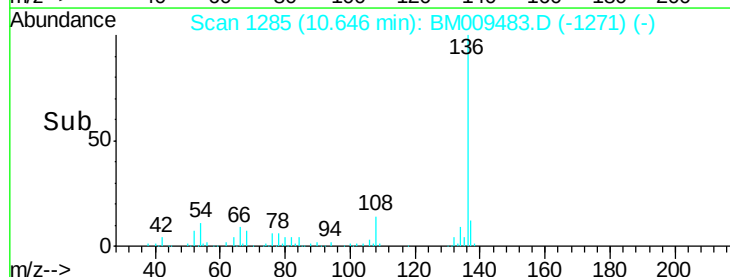


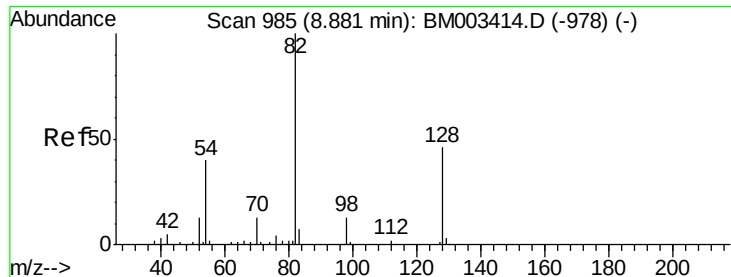

#23
Nitrobenzene-d5
Concen: 103.99 ng
RT: 9.01 min Scan# 1007
Delta R.T. -0.02 min
Lab File: BM009483.D
Acq: 31 Mar 2017 20:46




Instrument :
BNA_M
ClientSampleId :
WELL-A


Tot Ion: 82 Resp: 1123274
Ion Ratio Lower Upper
82 100
128 30.6 32.8 49.2#
54 53.6 40.6 60.8

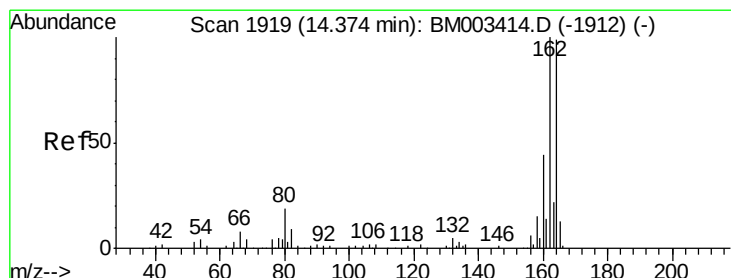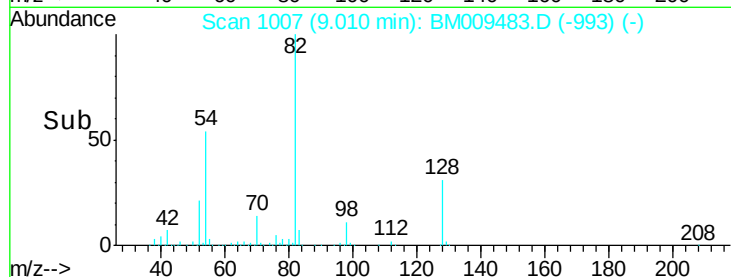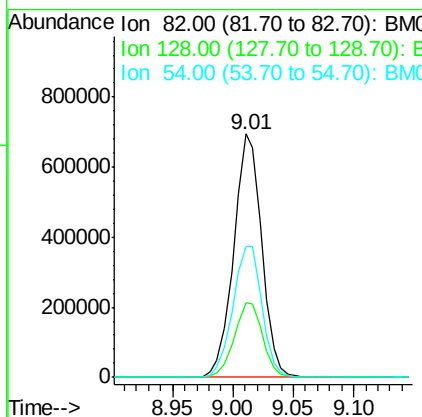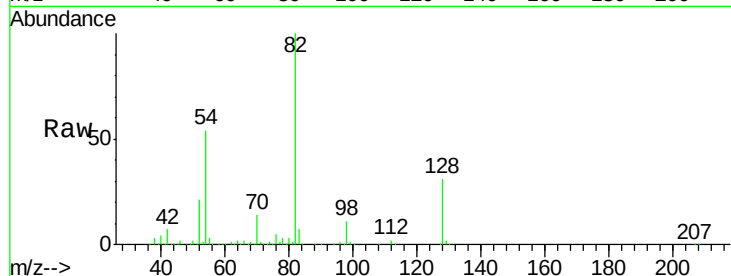

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.49 min Scan# 1938
Delta R.T. -0.02 min
Lab File: BM009483.D
Acq: 31 Mar 2017 20:46

Tgt Ion:164 Resp: 234358
Ion Ratio Lower Upper
164 100
162 97.7 82.4 123.6
160 43.7 35.8 53.6

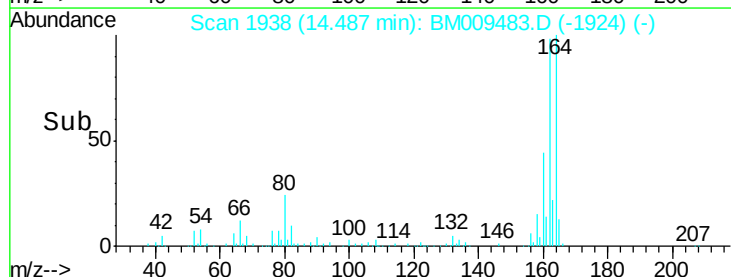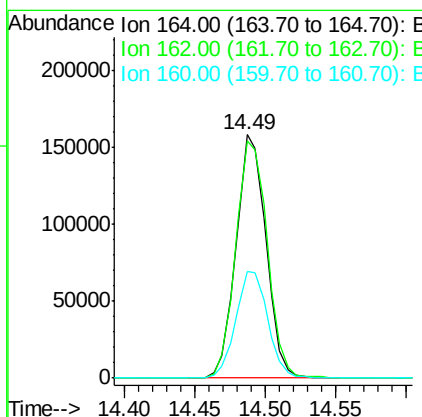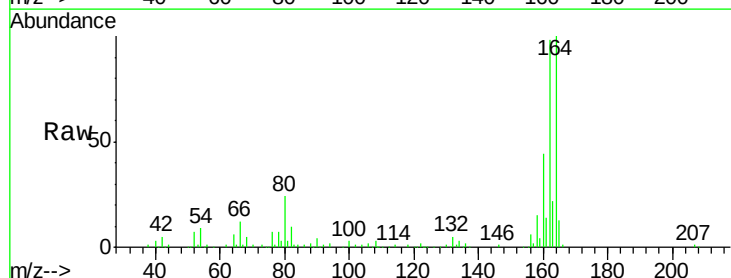


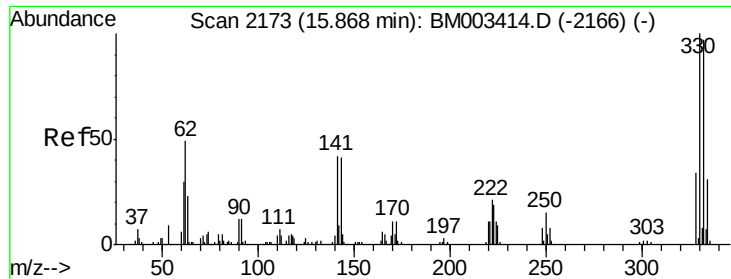




#41
 2,4,6-Tribromophenol
 Concen: 172.06 ng
 RT: 15.98 min Scan# 2192
 Delta R.T. -0.02 min
 Lab File: BM009483.D
 Acq: 31 Mar 2017 20:46

Instrument :
 BNA_M
 ClientSampleId :
 WELL-A

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.8	0.0	0.0#
141	40.7	0.0	0.0#

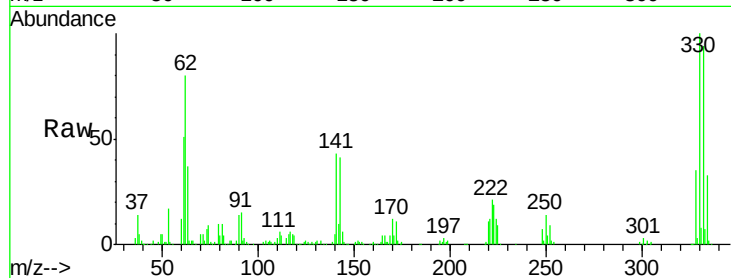


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

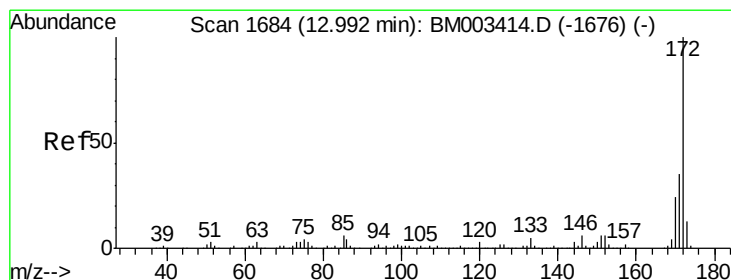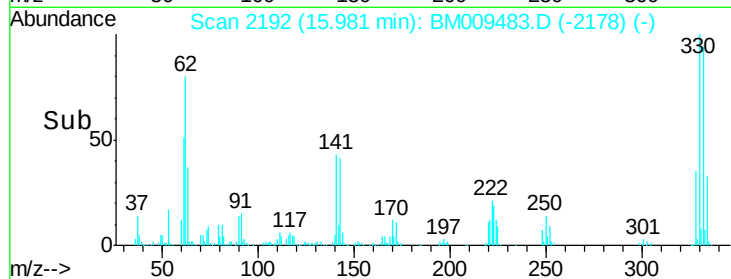
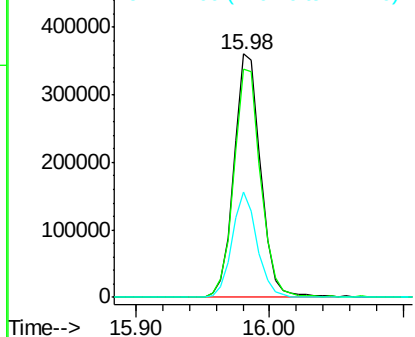



#44
 2-Fluorobiphenyl
 Concen: 106.15 ng
 RT: 13.10 min Scan# 1703
 Delta R.T. -0.02 min
 Lab File: BM009483.D
 Acq: 31 Mar 2017 20:46

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	28.5	42.7
170	22.6	18.8	28.2

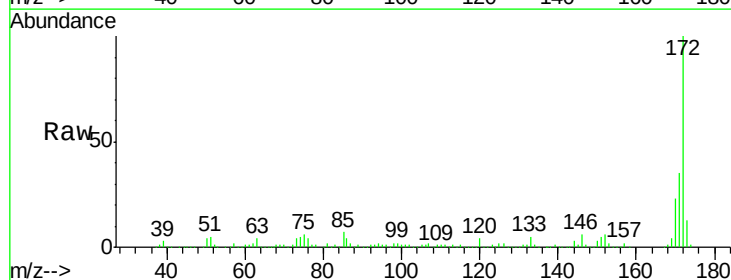

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



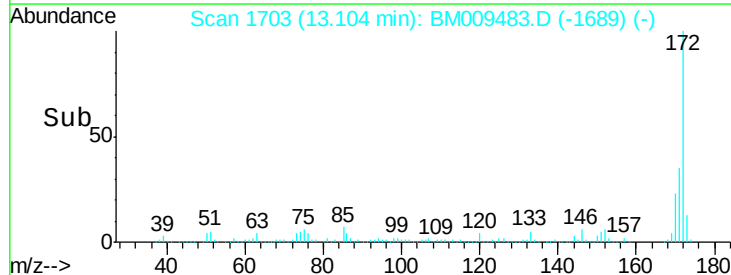
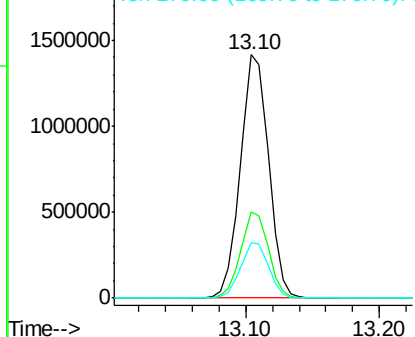


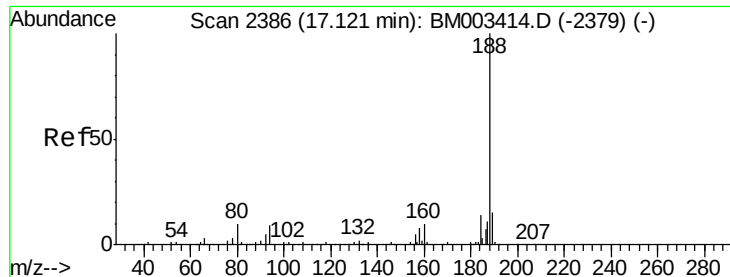

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.24 min Scan# 2406
Delta R.T. -0.01 min
Lab File: BM009483.D
Acq: 31 Mar 2017 20:46




Instrument :
BNA_M
ClientSampleId :
WELL-A


Tot Ion:188 Resp: 544309
Ion Ratio Lower Upper
188 100
94 7.9 8.7 13.1#
80 10.8 9.3 13.9

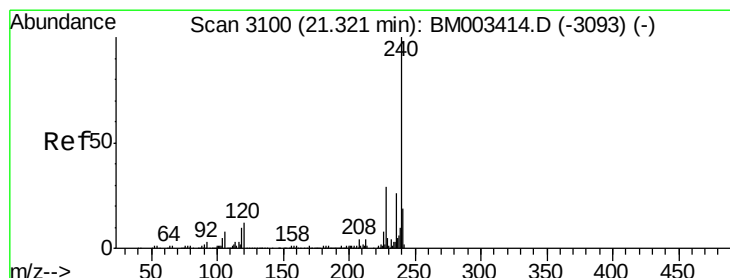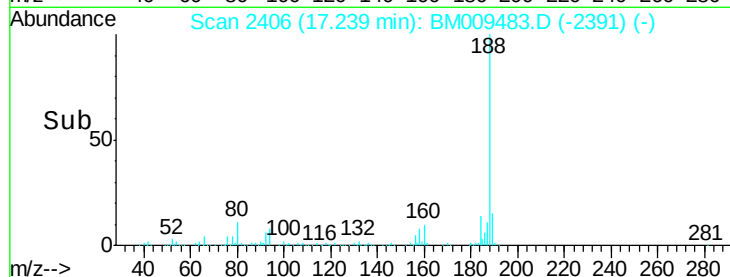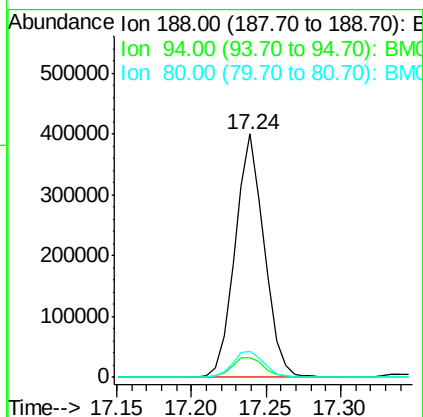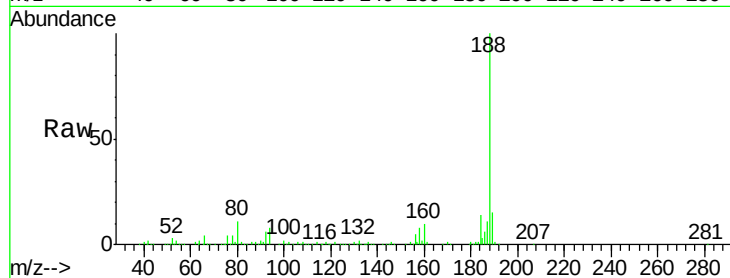

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.42 min Scan# 3116
Delta R.T. -0.01 min
Lab File: BM009483.D
Acq: 31 Mar 2017 20:46

Tgt Ion:240 Resp: 752230
Ion Ratio Lower Upper
240 100
120 9.0 8.2 12.2
236 23.7 20.0 30.0


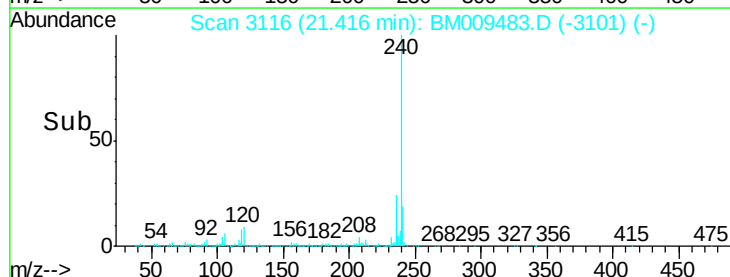
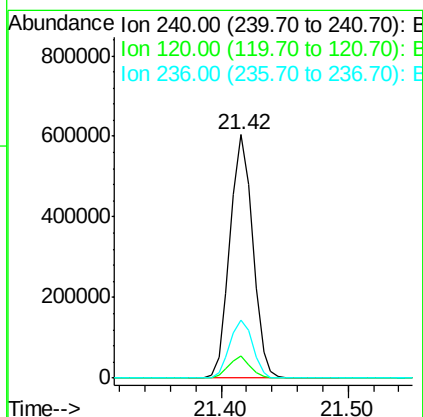
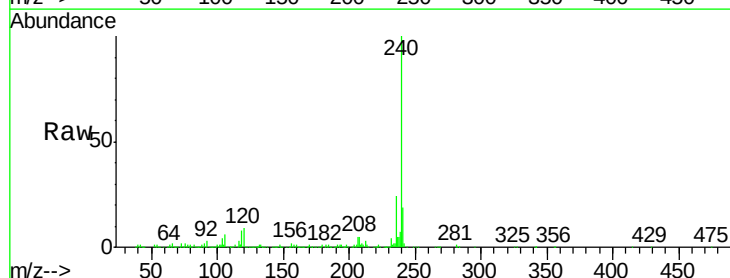


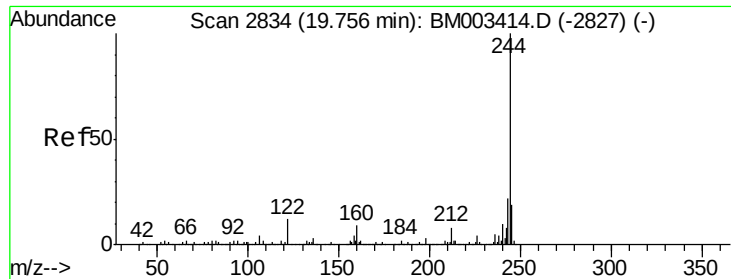

#78
 Terphenyl-d14
 Concen: 76.39 ng
 RT: 19.86 min Scan# 2851
 Delta R.T. -0.01 min
 Lab File: BM009483.D
 Acq: 31 Mar 2017 20:46

Instrument :
 BNA_M
 ClientSampleId :
 WELL-A

Tot Ion:244 Resp: 2750029
 Ion Ratio Lower Upper
 244 100
 212 7.5 4.9 7.3#
 122 9.0 6.2 9.4

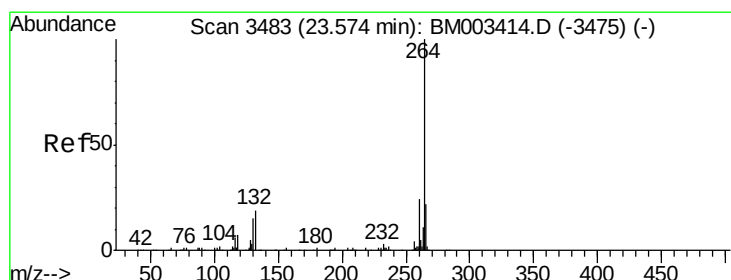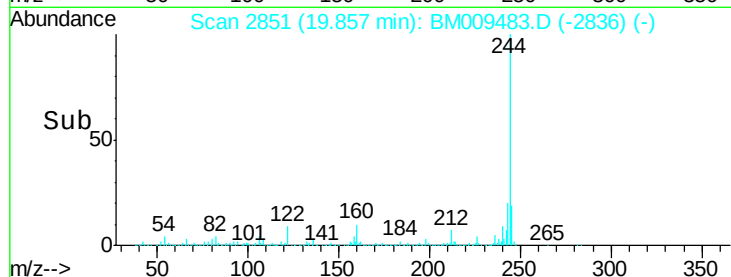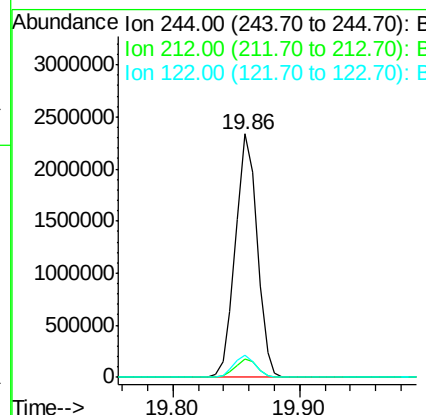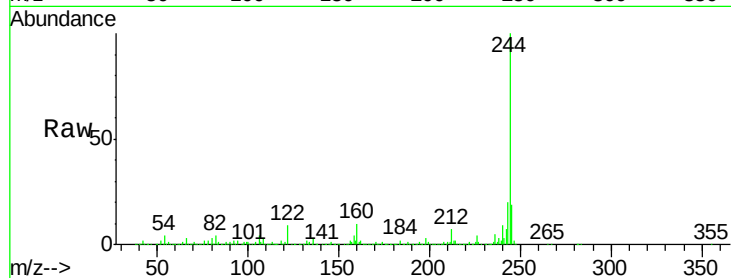

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 23.74 min Scan# 3511
 Delta R.T. -0.02 min
 Lab File: BM009483.D
 Acq: 31 Mar 2017 20:46

Tgt Ion:264 Resp: 731633
 Ion Ratio Lower Upper
 264 100
 260 21.5 18.6 27.8
 265 21.8 17.3 25.9

