

Data Path : Z:\HPCHEM1\BNA M\Data\BM033117\
 Data File : BM009490.D
 Acq On : 01 Apr 2017 00:56
 Operator : SJ/MA
 Sample : I2474-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 49B-9-11

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.969	316	320	329	rVB	100275	149466	2.08%	0.400%
2	5.422	391	397	407	rBV	1270933	1842686	25.59%	4.932%
3	7.004	659	666	673	rBV	774715	1186597	16.48%	3.176%
4	7.375	722	729	737	rBV	2059350	3196946	44.40%	8.556%
5	7.846	802	809	816	rBV	466311	753808	10.47%	2.017%
6	8.163	853	863	871	rBV	1958976	3116757	43.29%	8.341%
7	9.010	999	1007	1020	rBV	1732761	2832968	39.34%	7.582%
8	10.645	1276	1285	1290	rBV	573561	968198	13.45%	2.591%
9	10.692	1290	1293	1300	rVB2	62094	98972	1.37%	0.265%
10	13.104	1696	1703	1712	rBV	3765266	5480695	76.12%	14.668%
11	14.492	1931	1939	1945	rBV2	769649	1204401	16.73%	3.223%
12	14.551	1945	1949	1956	rVB2	63499	92700	1.29%	0.248%
13	15.980	2186	2192	2201	rBV	2592841	3530242	49.03%	9.448%
14	17.239	2398	2406	2411	rBV	1062927	1481201	20.57%	3.964%
15	19.857	2845	2851	2861	rBV	6021736	7200461	100.00%	19.271%
16	21.415	3111	3116	3124	rBV	1669417	2096755	29.12%	5.612%
17	22.262	3256	3260	3263	rBV4	83340	116589	1.62%	0.312%
18	23.739	3504	3511	3521	rVB2	1024153	2015407	27.99%	5.394%


Sum of corrected areas: 37364849

Data Path : Z:\HPCHEM1\BNA M\Data\BM033117\
Data File : BM009490.D
Acq On : 01 Apr 2017 00:56
Operator : SJ/MA
Sample : I2474-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
49B-9-11

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

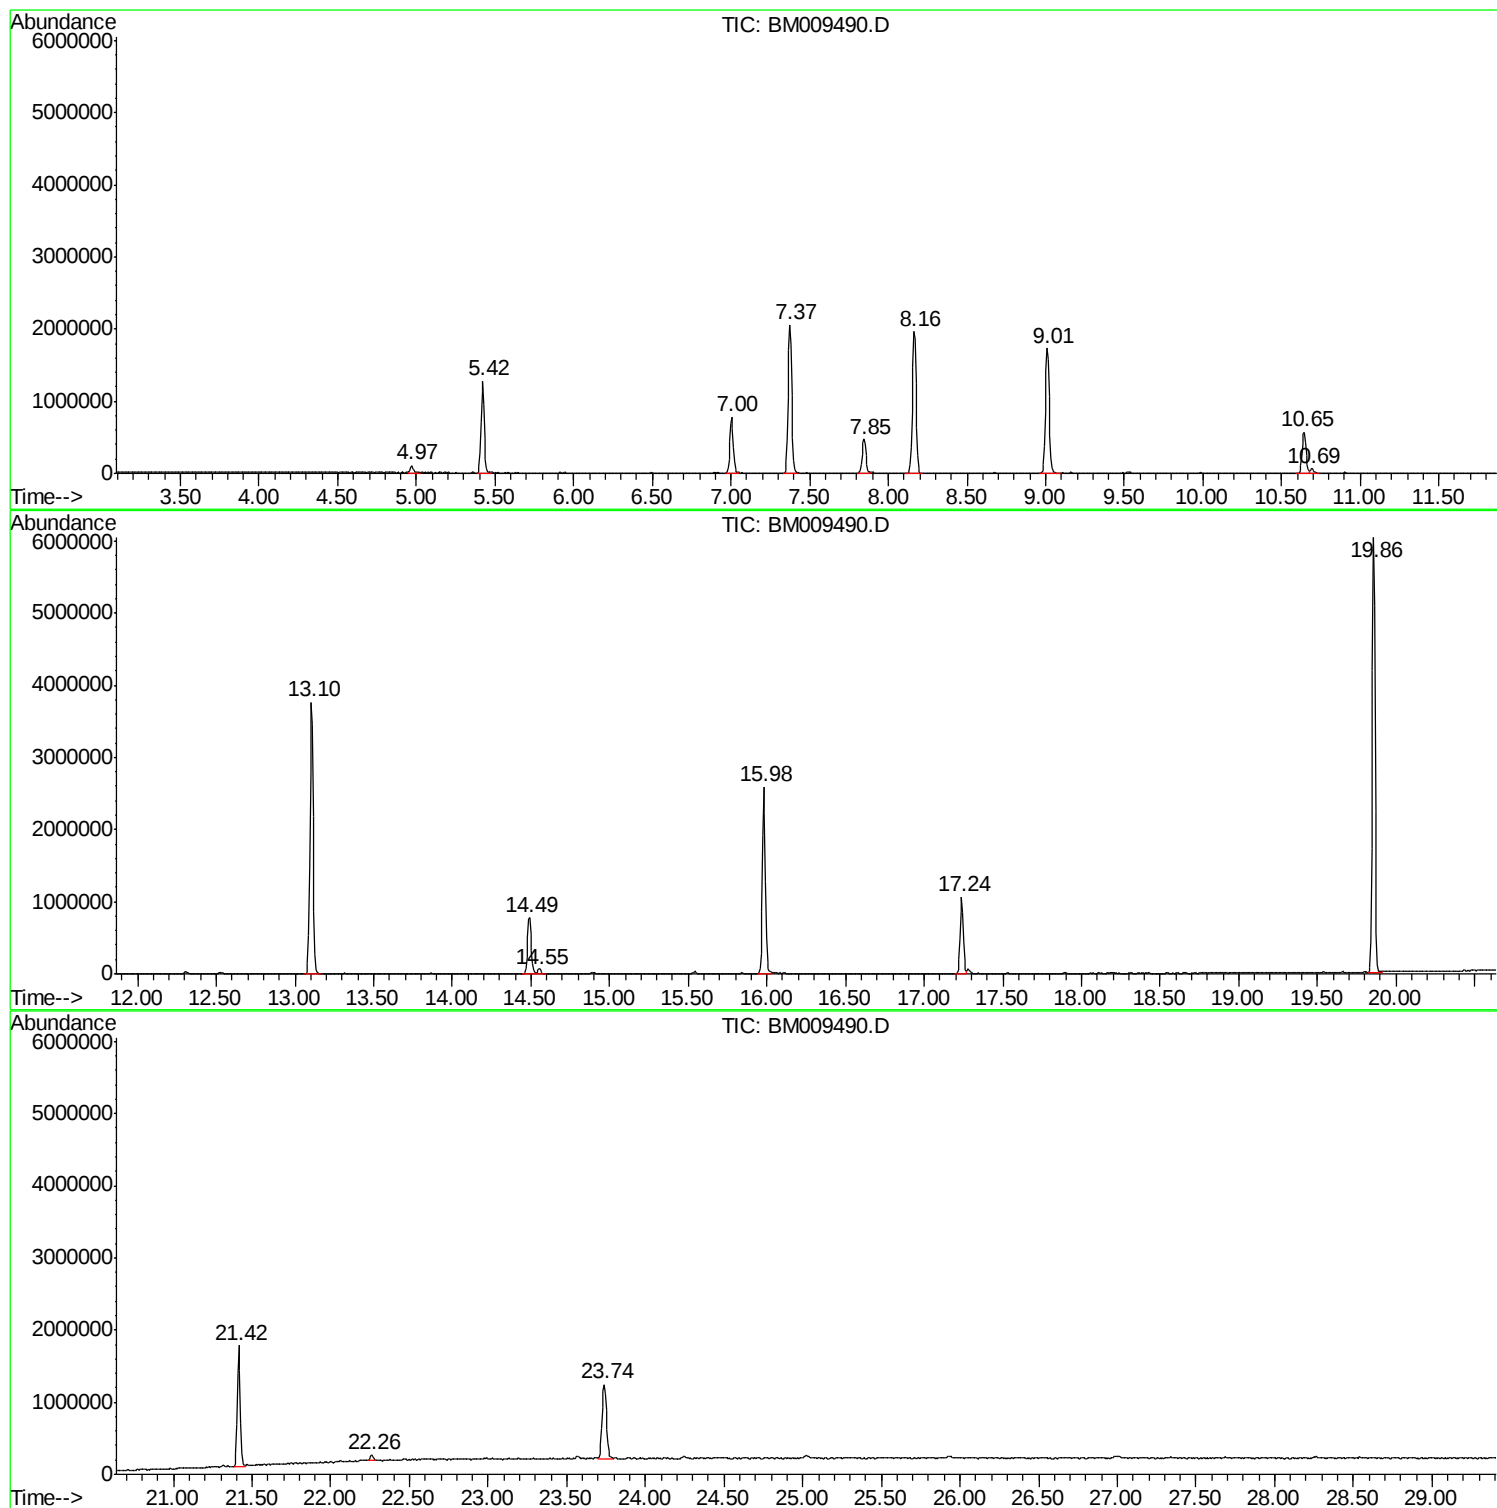

Data Path : Z:\HPCHEM1\BNA M\Data\BM033117\
Data File : BM009490.D
Acq On : 01 Apr 2017 00:56
Operator : SJ/MA
Sample : I2474-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
49B-9-11










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.97	3.97 ng	149466	1,4-Dichlorobenzene-d4	7.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			Hydrazine, 1,1-bis(1-methylethyl)-	116	C6H16N2	000921-14-2	40
3			Diacetamide	101	C4H7NO2	000625-77-4	38
4			Propane, 1-ethoxy-2-methyl-	102	C6H14O	000627-02-1	35
5			2-Nonanone, 9-hydroxy-	158	C9H18O2	025368-56-3	33

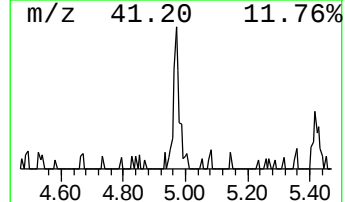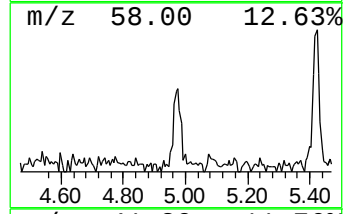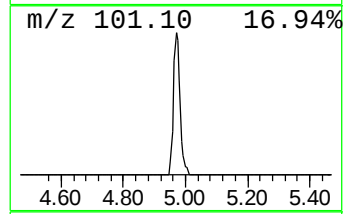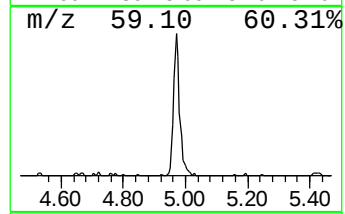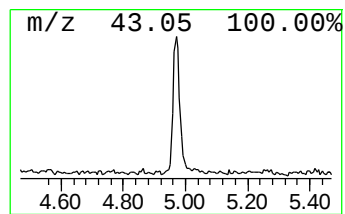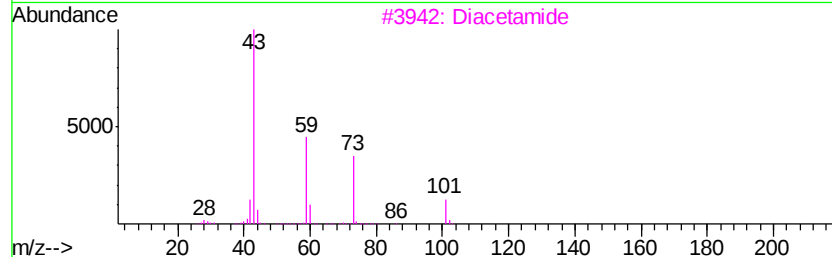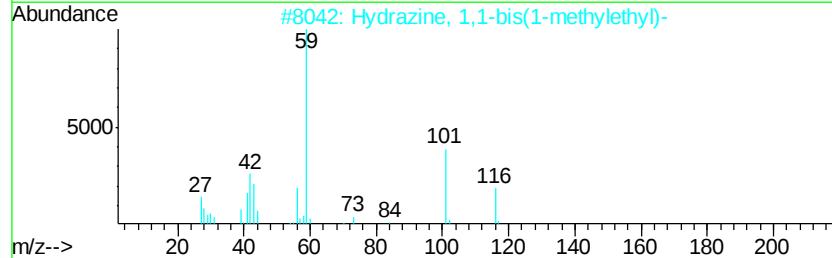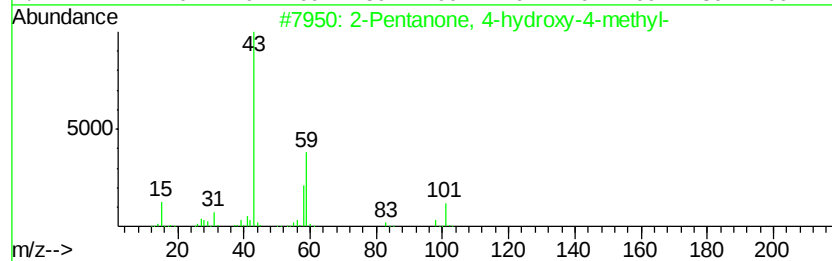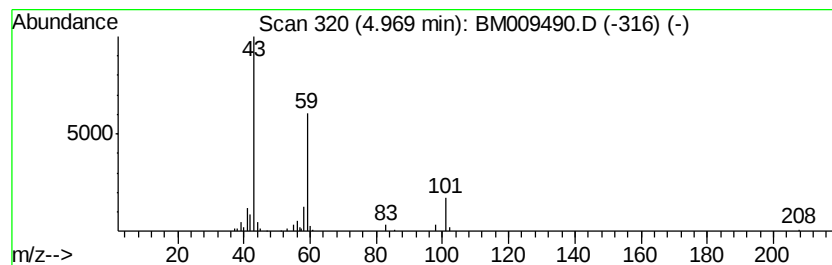

Data Path : Z:\HPCHEM1\BNA M\Data\BM033117\
Data File : BM009490.D
Acq On : 01 Apr 2017 00:56
Operator : SJ/MA
Sample : I2474-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
49B-9-11










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.37	84.82 ng	3196950	1,4-Dichlorobenzene-d4	7.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
2		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	14
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
5		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10

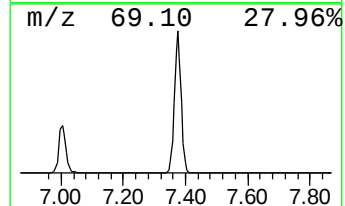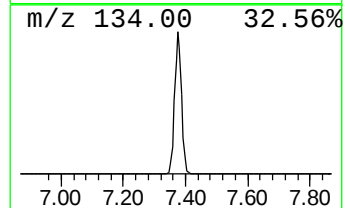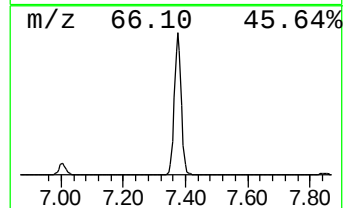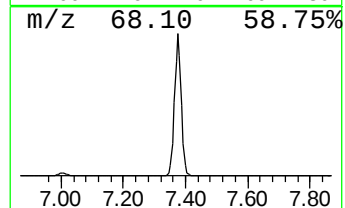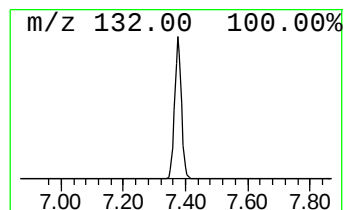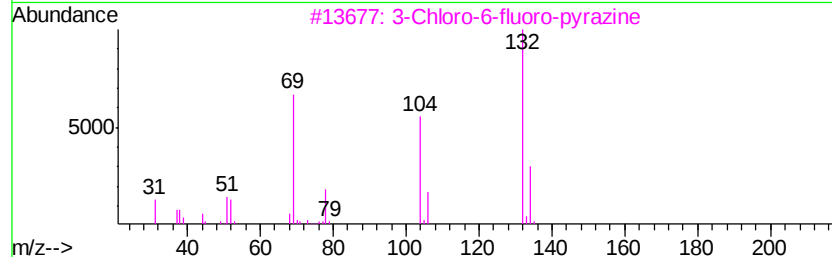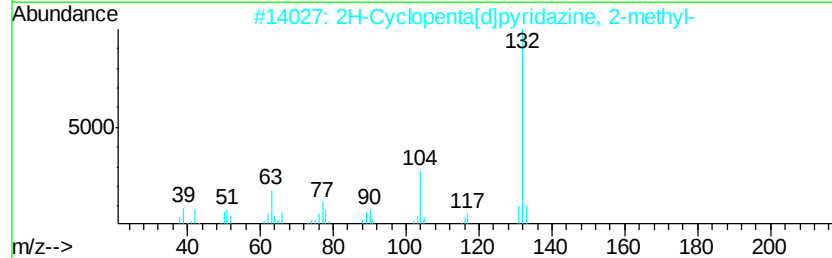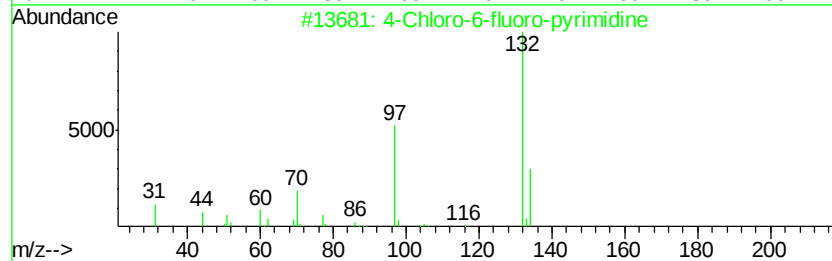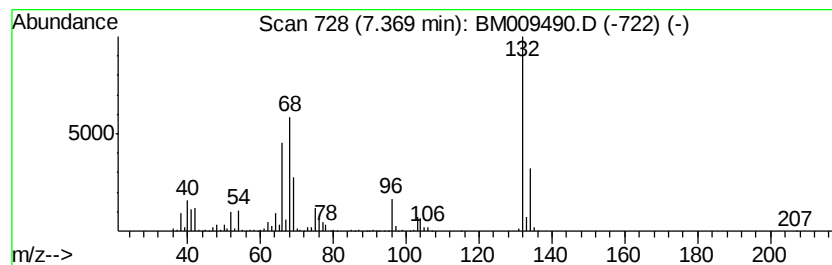

Data Path : Z:\HPCHEM1\BNA_M\Data\BM033117\
Data File : BM009490.D
Acq On : 01 Apr 2017 00:56
Operator : SJ/MA
Sample : I2474-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
49B-9-11

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.97	4.0	ng	149466	1	7.85	753808	20.0
unknown7.37	7.37	84.8	ng	3196950	1	7.85	753808	20.0