


Data Path : Z:\HPCHEM1\BNA M\Data\BM033117\
 Data File : BM009486.D
 Acq On : 31 Mar 2017 22:33
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 31 12:10:26 2017

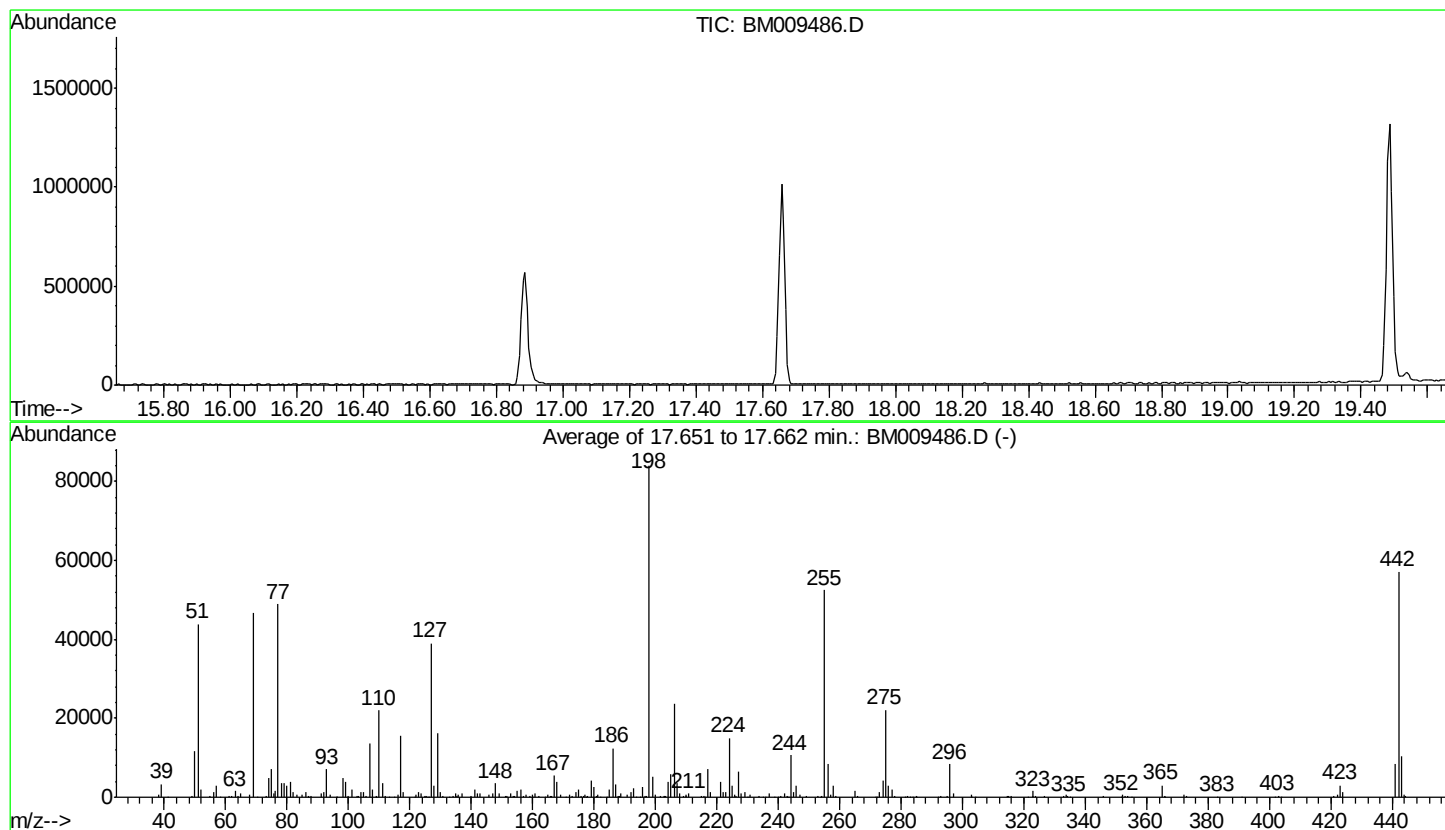

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	43946	PASS
68	69	0.00	2	1.7	779	PASS
69	198	0.00	100	55.7	46837	PASS
70	69	0.00	2	0.3	129	PASS
127	198	10	80	46.3	38936	PASS
197	198	0.00	2	0.5	404	PASS
198	198	100	100	100.0	84037	PASS
199	198	5	9	6.0	5064	PASS
275	198	10	60	26.4	22149	PASS
365	198	1	100	3.5	2934	PASS
441	442	0.01	24	14.7	8403	PASS
442	198	50	100	68.1	57266	PASS
443	442	15	24	18.0	10317	PASS