
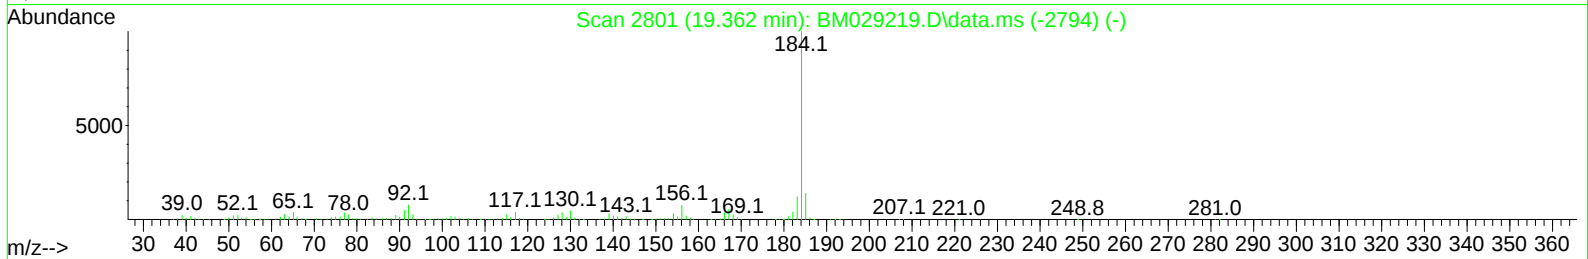
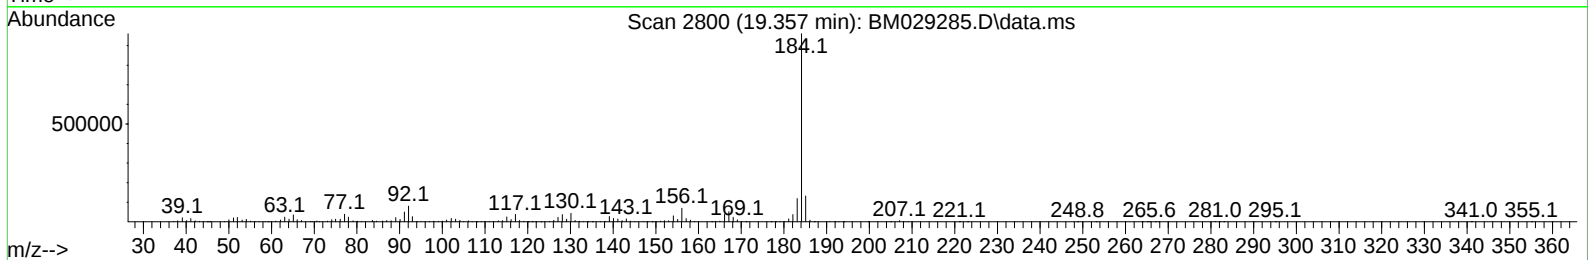


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033121\
 Data File : BM029285.D
 Acq On : 31 Mar 2021 09:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 11:06:23 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 29 11:14:33 2021
 Response via : Initial Calibration

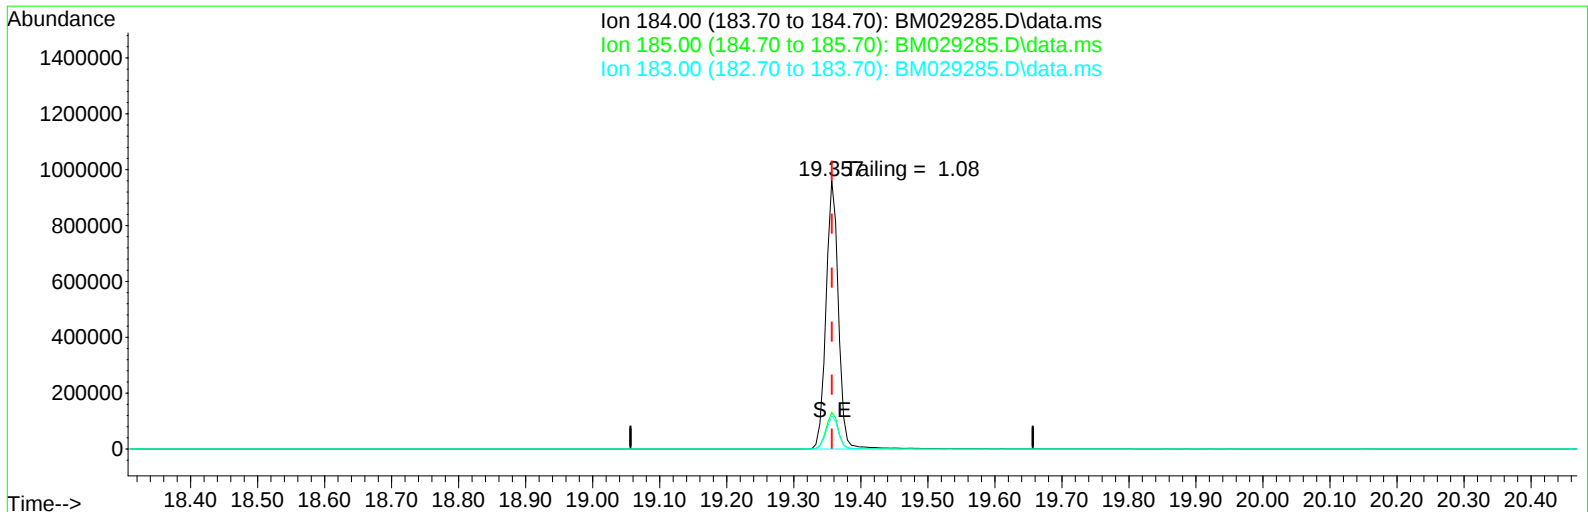

TIC: BM029285.D\data.ms

(77) Benzidine




19.357min (-0.000) 40139.92 ng

response 1236200

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.69
183.00	12.20	12.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033121\
Data File : BM029285.D
Acq On : 31 Mar 2021 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 11:06:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 29 11:14:33 2021
Response via : Initial Calibration

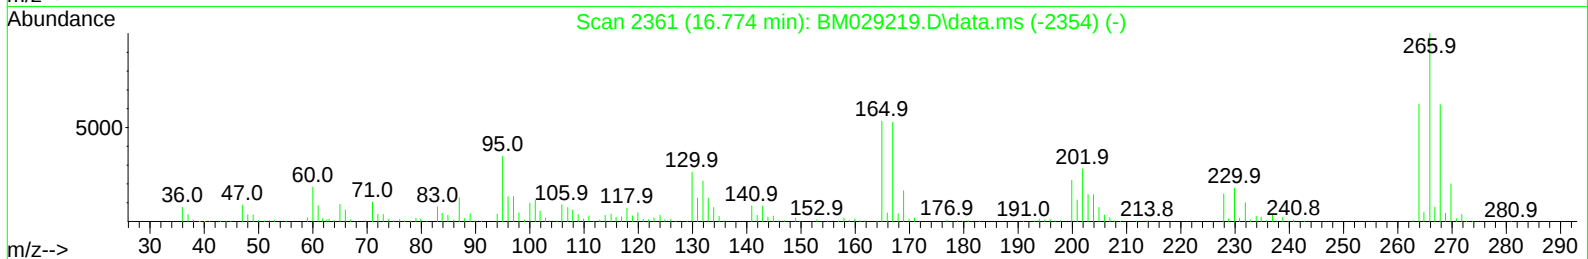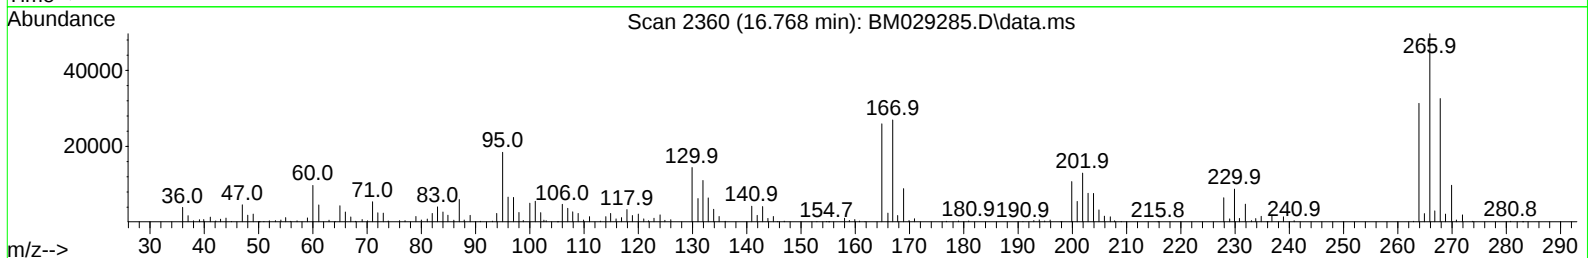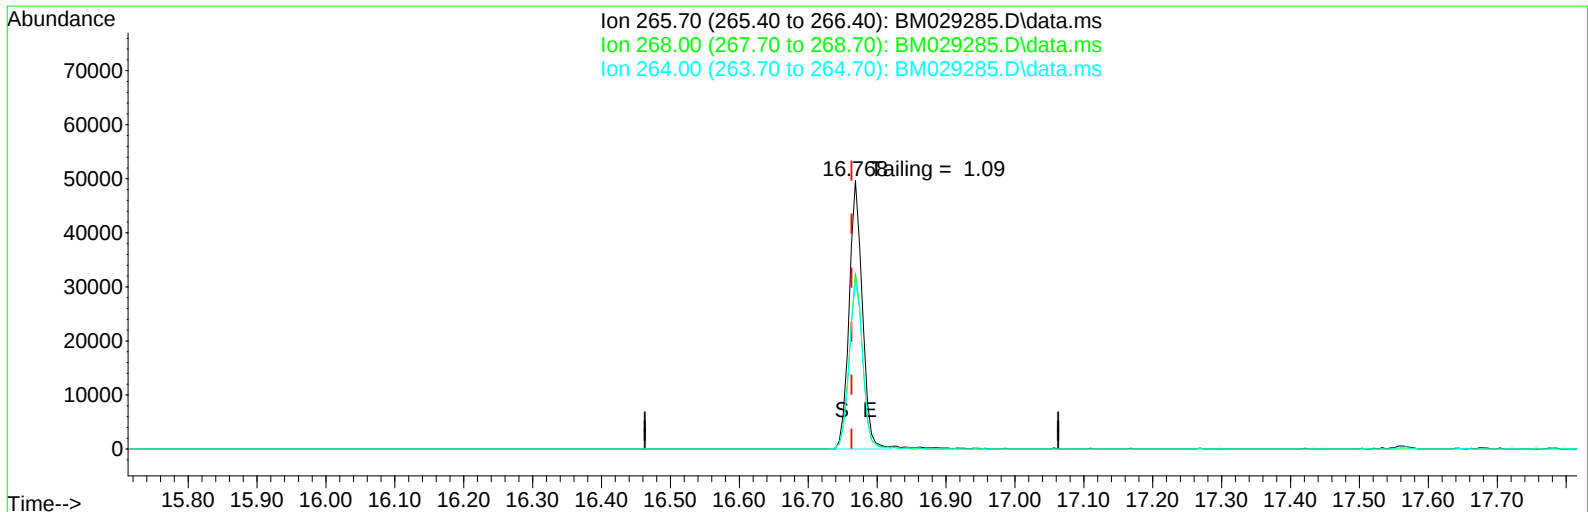

TIC: BM029285.D\data.ms

(70) Pentachlorophenol (C)

16.768min (+ 0.006) 177352.22 ng

response 65989

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	65.62
264.00	63.60	63.11
0.00	0.00	0.00