

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033121\
 Data File : BM029287.D
 Acq On : 31 Mar 2021 10:37
 Operator : CG/JU
 Sample : PB135441BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135441BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	24	27	32	rVB	74336	81402	1.12%	0.229%
2	5.351	412	419	429	rBV	2833028	4130480	56.90%	11.645%
3	6.922	678	686	700	rBV	2666837	4316307	59.46%	12.169%
4	7.745	819	826	834	rBV	524962	816178	11.24%	2.301%
5	8.898	1014	1022	1035	rBV	1717276	2802603	38.61%	7.901%
6	10.528	1291	1299	1310	rBV	637437	1085696	14.96%	3.061%
7	12.998	1712	1719	1729	rBV	4120331	5911014	81.43%	16.665%
8	14.374	1947	1953	1967	rVB	939373	1353194	18.64%	3.815%
9	15.862	2199	2206	2216	rBV	2484902	3491708	48.10%	9.844%
10	17.115	2412	2419	2428	rBV	1072100	1466308	20.20%	4.134%
11	19.739	2859	2865	2871	rBV	6053128	7258613	100.00%	20.464%
12	21.286	3123	3128	3134	rBV	1049415	1338416	18.44%	3.773%
13	23.521	3502	3508	3520	rVB2	730756	1417424	19.53%	3.996%




Sum of corrected areas: 35469343

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033121\
Data File : BM029287.D
Acq On : 31 Mar 2021 10:37
Operator : CG/JU
Sample : PB135441BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135441BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

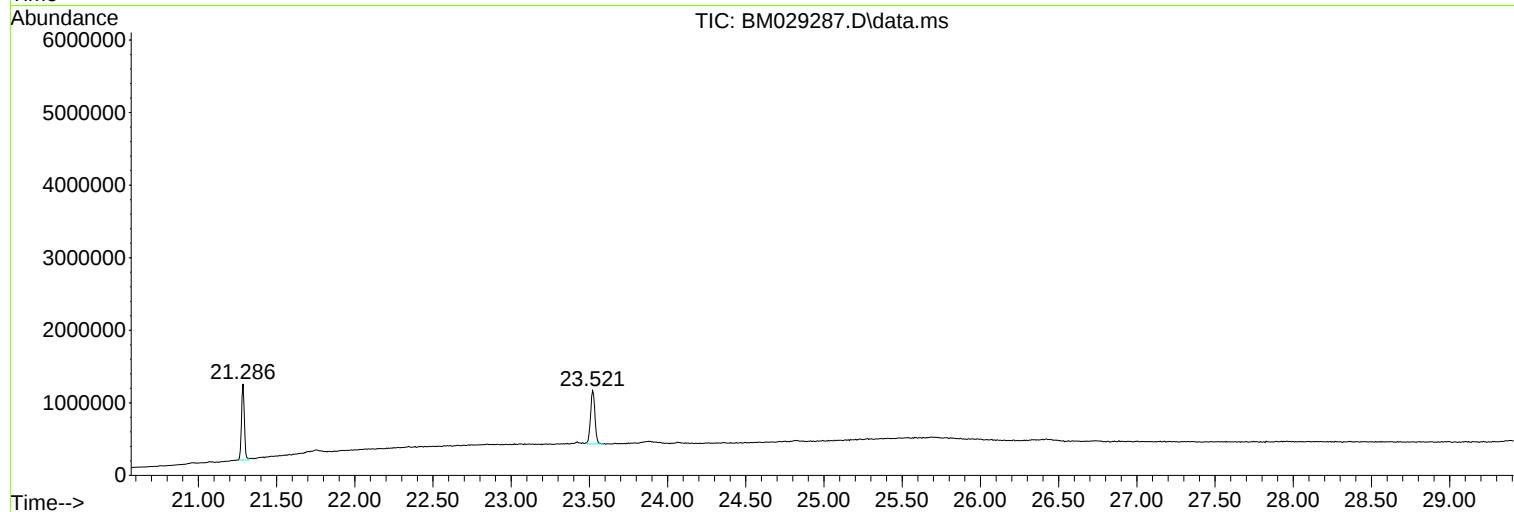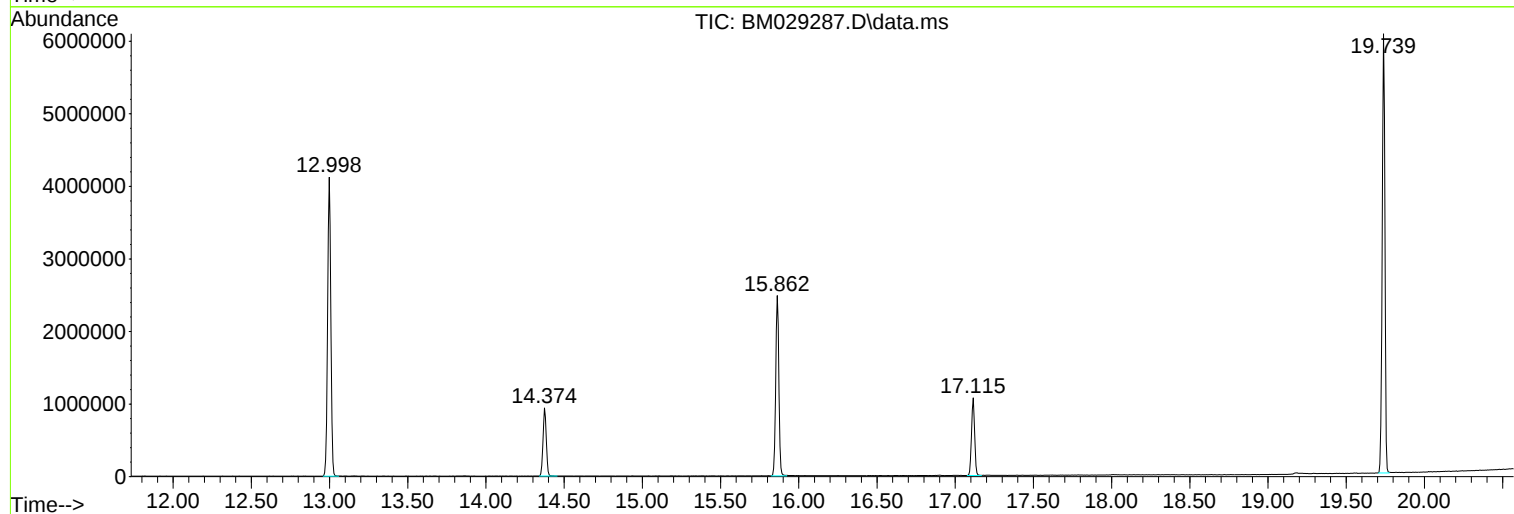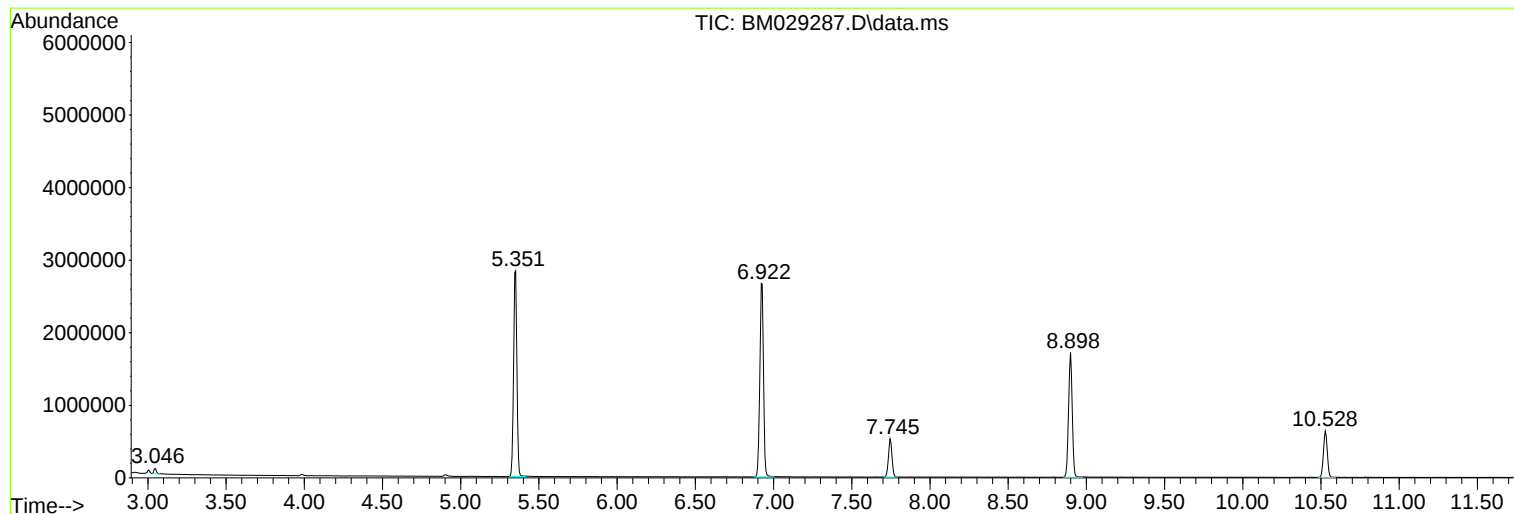

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033121\
Data File : BM029287.D
Acq On : 31 Mar 2021 10:37
Operator : CG/JU
Sample : PB135441BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135441BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033121\
Data File : BM029287.D
Acq On : 31 Mar 2021 10:37
Operator : CG/JU
Sample : PB135441BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135441BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------