


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033121\
 Data File : BM029285.D
 Acq On : 31 Mar 2021 09:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 29 11:14:33 2021

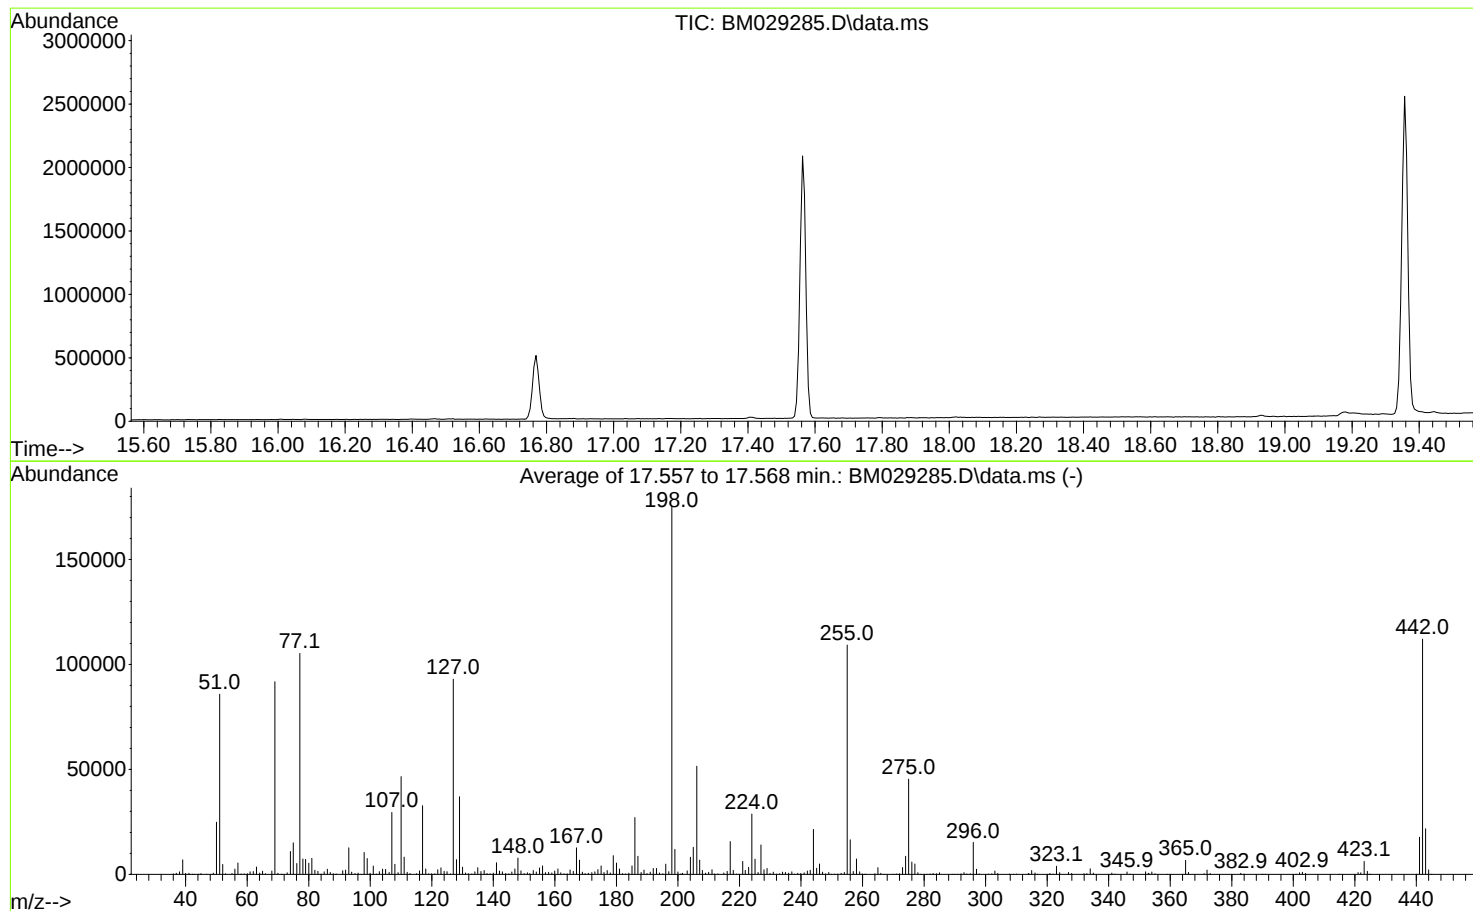

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	85828	PASS
68	69	0.00	2	1.8	1635	PASS
69	198	0.00	100	52.4	91775	PASS
70	69	0.00	2	0.6	559	PASS
127	198	10	80	53.1	92981	PASS
197	198	0.00	2	0.8	1317	PASS
198	198	100	100	100.0	175232	PASS
199	198	5	9	6.8	11883	PASS
275	198	10	60	25.9	45320	PASS
365	198	1	100	3.8	6699	PASS
441	198	0.01	100	10.1	17649	PASS
442	442	50	100	100.0	112051	PASS
443	442	15	24	19.4	21739	PASS

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2021	BNA_M	<u>BM029285.D</u>
Compound Name	Response	Retention Time
DDT	560480	20.59
DDD	33873	20.15
DDE	1067	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34940	595420	5.87

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033121\
Data File : BM029285.D
Acq On : 31 Mar 2021 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 31 11:06:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 29 11:14:33 2021
Response via : Initial Calibration

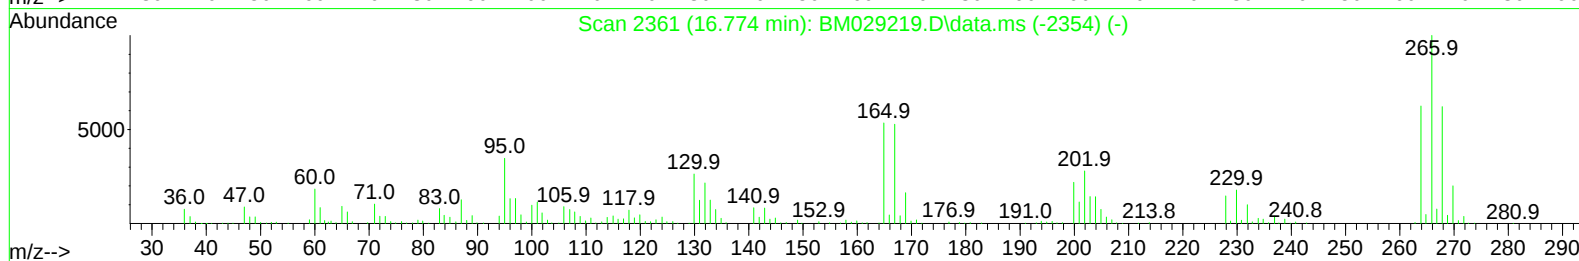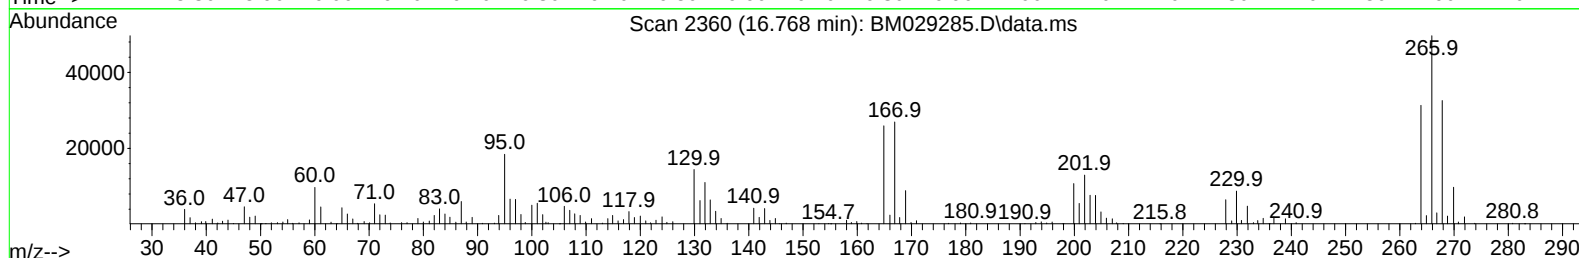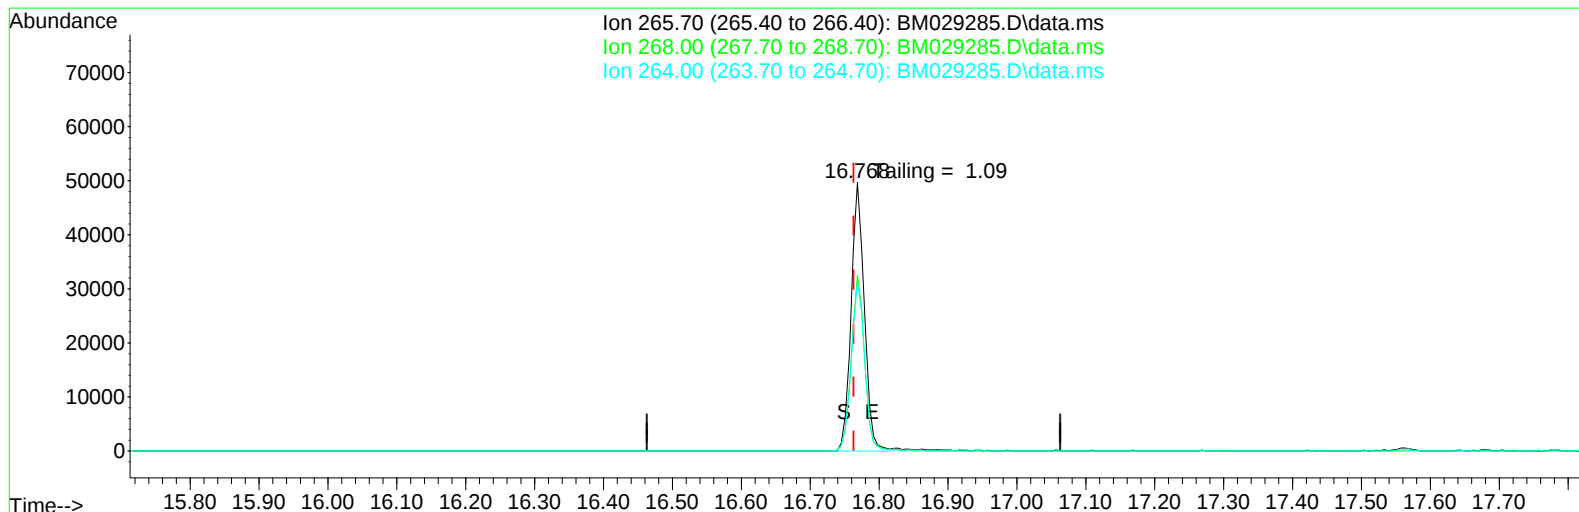

TIC: BM029285.D\data.ms

(70) Pentachlorophenol (C)

16.768min (+ 0.006) 177352.22 ng




response 65989

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	65.62
264.00	63.60	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033121\
Data File : BM029285.D
Acq On : 31 Mar 2021 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 31 11:06:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 29 11:14:33 2021
Response via : Initial Calibration

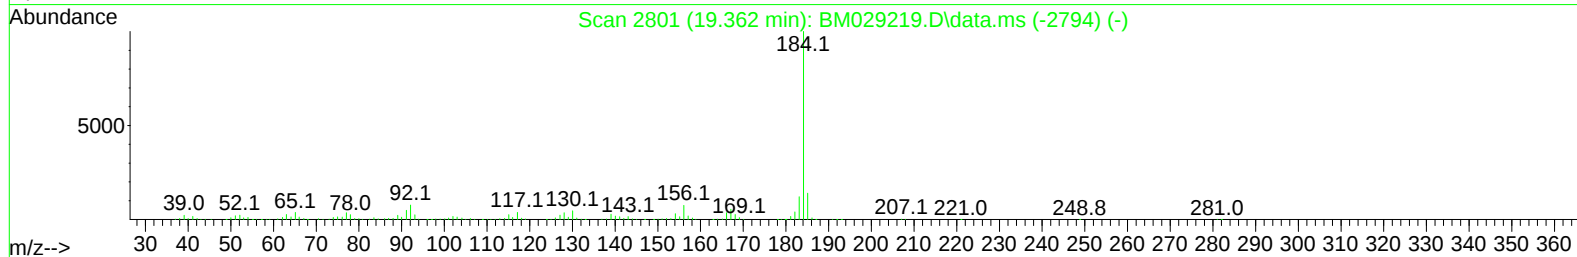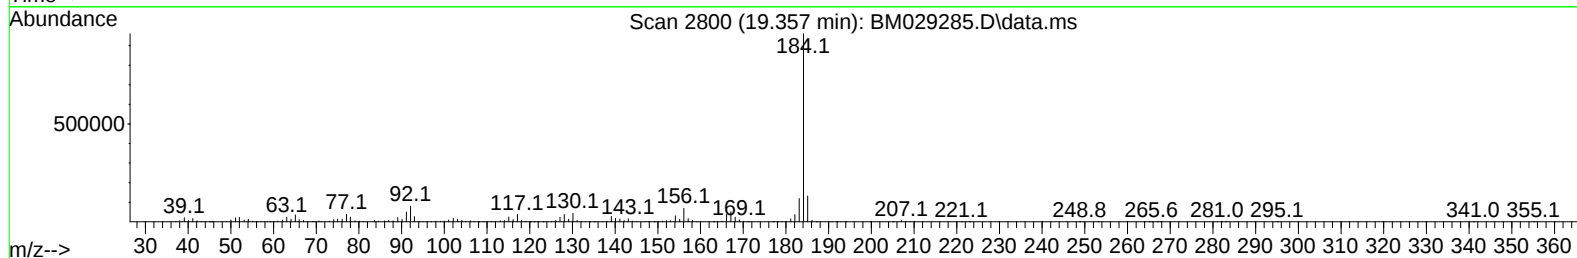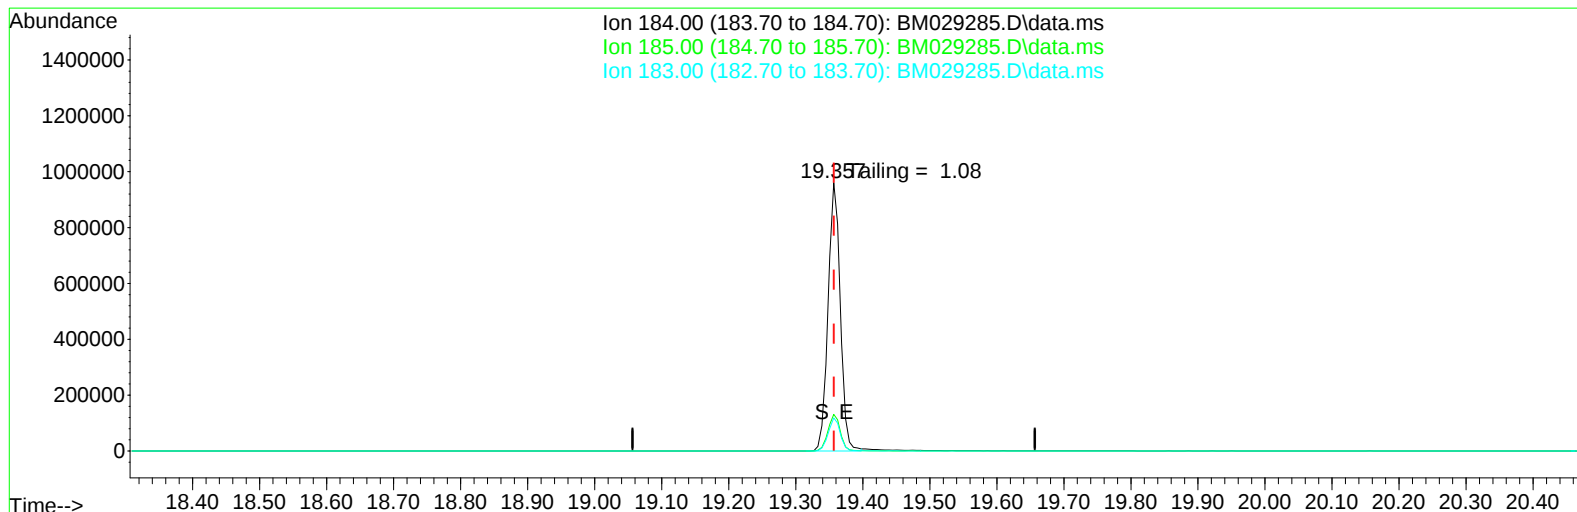

TIC: BM029285.D\data.ms

(77) Benzidine

19.357min (-0.000) 40139.92 ng

response 1236200

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.69
183.00	12.20	12.35
0.00	0.00	0.00