
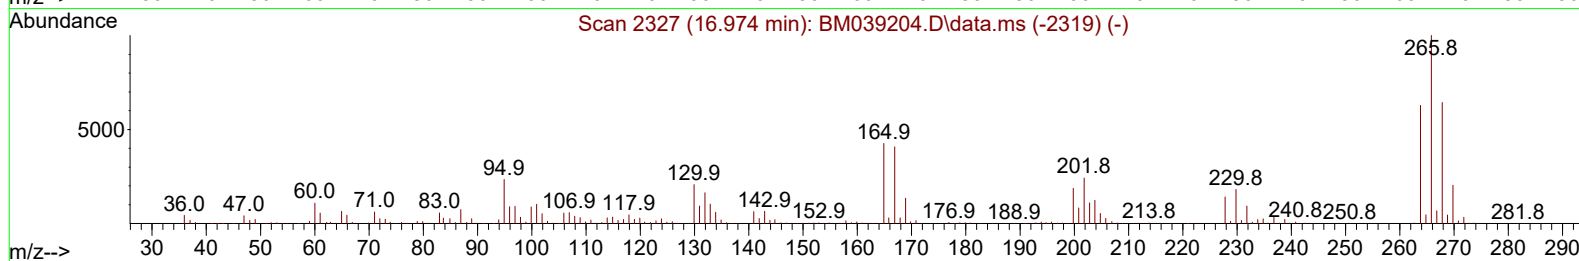
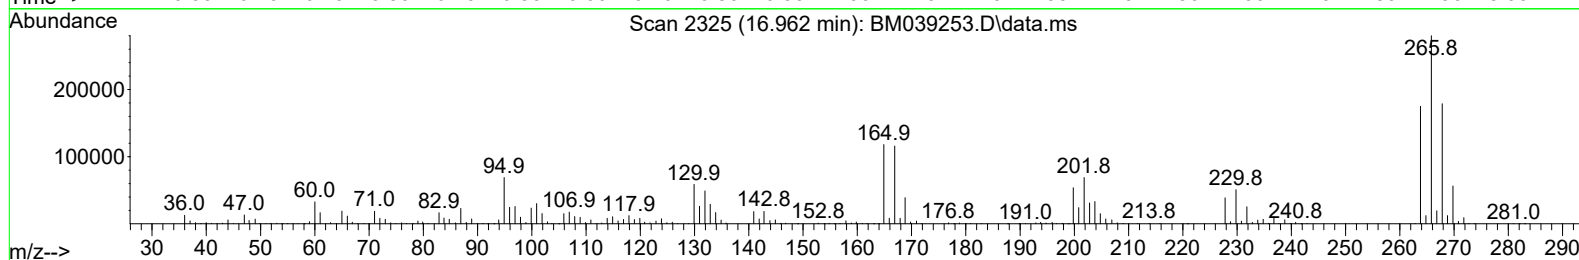


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039253.D
Acq On : 31 Mar 2023 15:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 05:09:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 17:03:41 2023
Response via : Initial Calibration

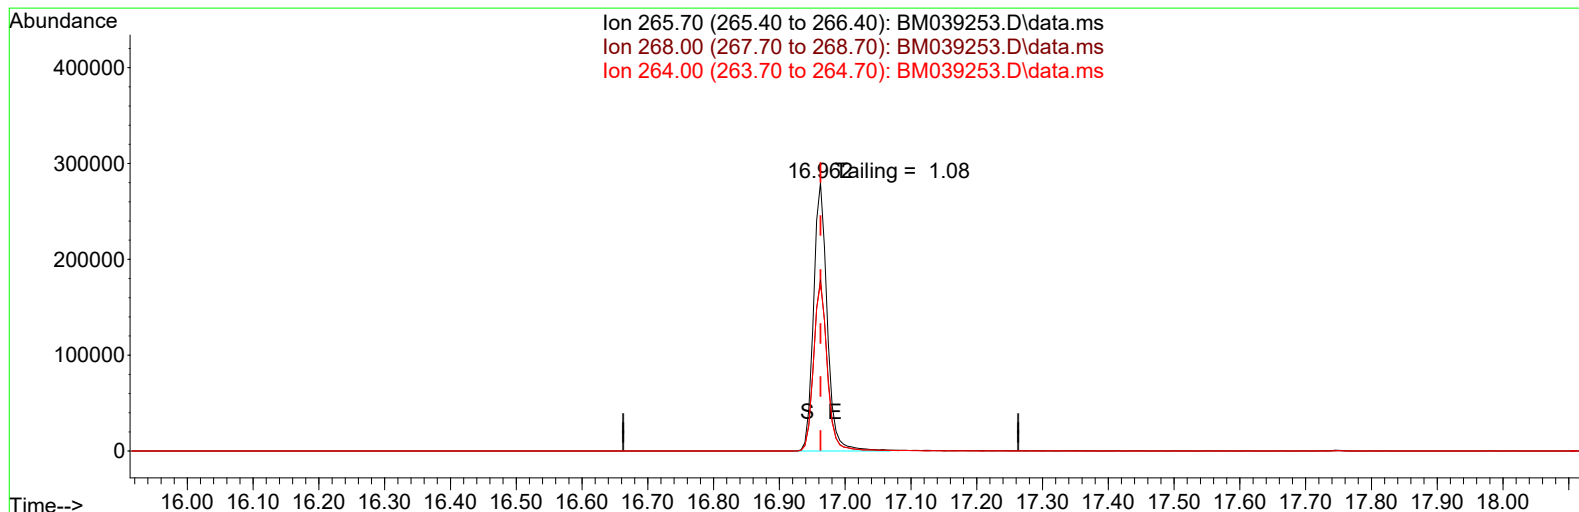

TIC: BM039253.D\data.ms

(70) Pentachlorophenol (C)




16.962min (-0.000) 374739.91 ng

response 404725

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.83
264.00	62.80	62.50
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\  
Data File : BM039253.D  
Acq On    : 31 Mar 2023  15:03  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 01 05:09:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 17:03:41 2023
Response via : Initial Calibration

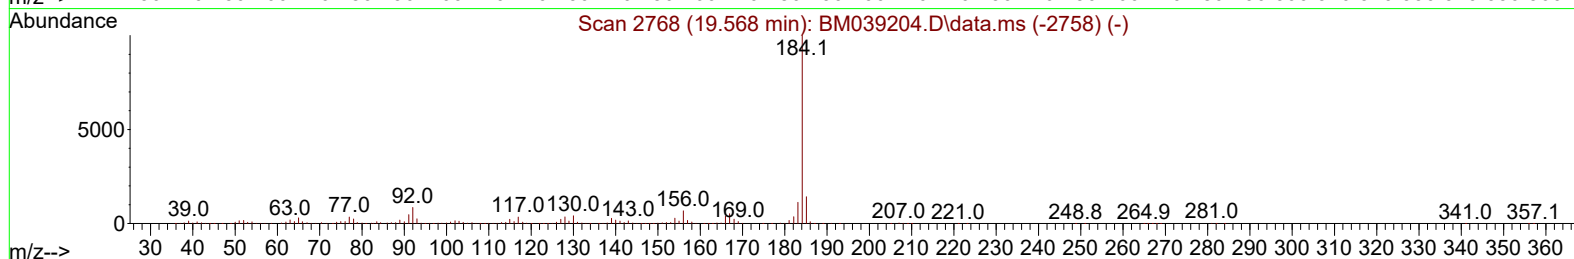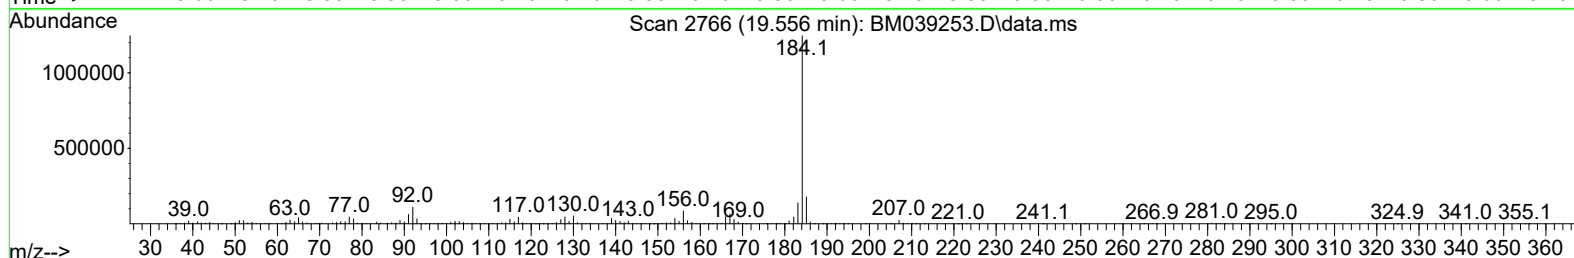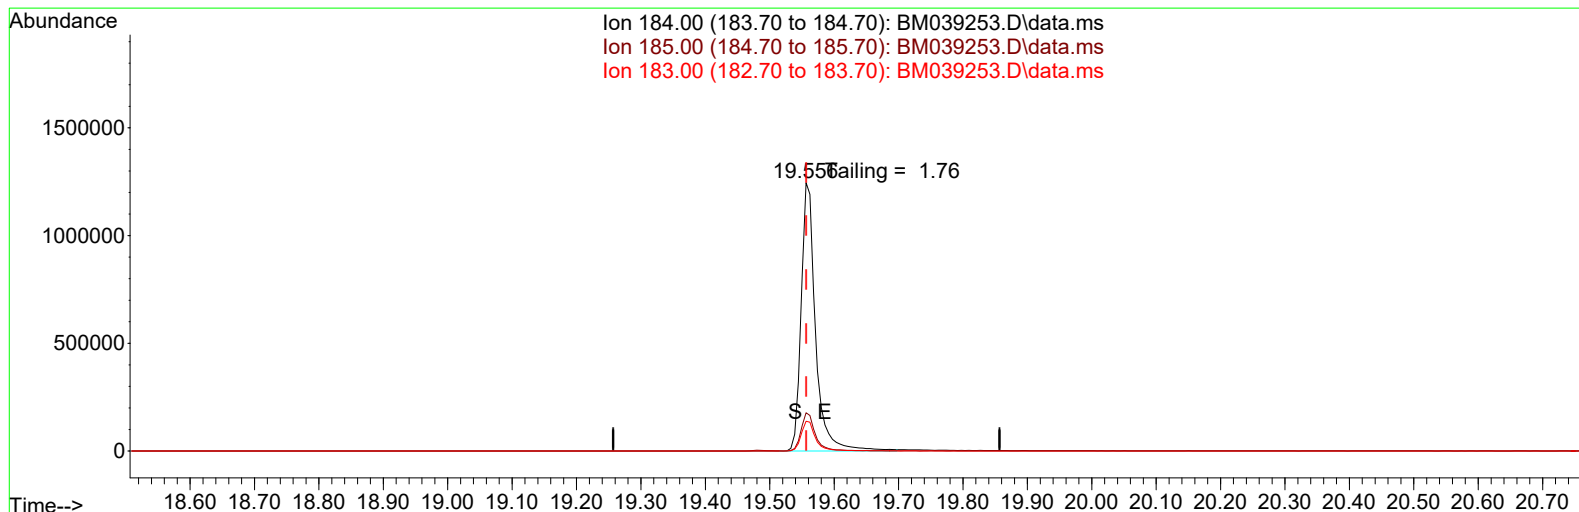

TIC: BM039253.D\data.ms

(77) Benzidine

19.556min (-0.000) 45058.87 ng

response **1956257**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.29
183.00	11.20	11.12
0.00	0.00	0.00