

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
 Data File : BM039247.D
 Acq On : 31 Mar 2023 11:08
 Operator : CG/JU
 Sample : PB151761BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB151761BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM039247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.010	287	293	304	rBV	1975431	2614532	24.19%	4.537%
2	5.481	366	373	387	rVB	4576762	6613753	61.19%	11.477%
3	7.087	638	646	665	rBV	4312596	6653828	61.56%	11.547%
4	7.916	781	787	796	rVB	814592	1255033	11.61%	2.178%
5	9.087	976	986	1001	rBV	2535784	4237796	39.21%	7.354%
6	10.728	1257	1265	1279	rBV	998456	1695612	15.69%	2.943%
7	13.186	1676	1683	1700	rBV	5941959	8793936	81.36%	15.261%
8	14.563	1911	1917	1927	rBV	1411769	2046411	18.93%	3.551%
9	16.051	2164	2170	2192	rBV	4074356	6048941	55.97%	10.497%
10	17.310	2378	2384	2397	rBV	1602375	2277172	21.07%	3.952%
11	18.204	2532	2536	2546	rBV4	53144	109471	1.01%	0.190%
12	19.933	2825	2830	2843	rBV	8754097	10808084	100.00%	18.756%
13	21.492	3090	3095	3105	rBV	1698764	2238819	20.71%	3.885%
14	23.903	3499	3505	3515	rVB2	1109806	2230300	20.64%	3.870%




Sum of corrected areas: 57623688

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039247.D
Acq On : 31 Mar 2023 11:08
Operator : CG/JU
Sample : PB151761BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151761BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

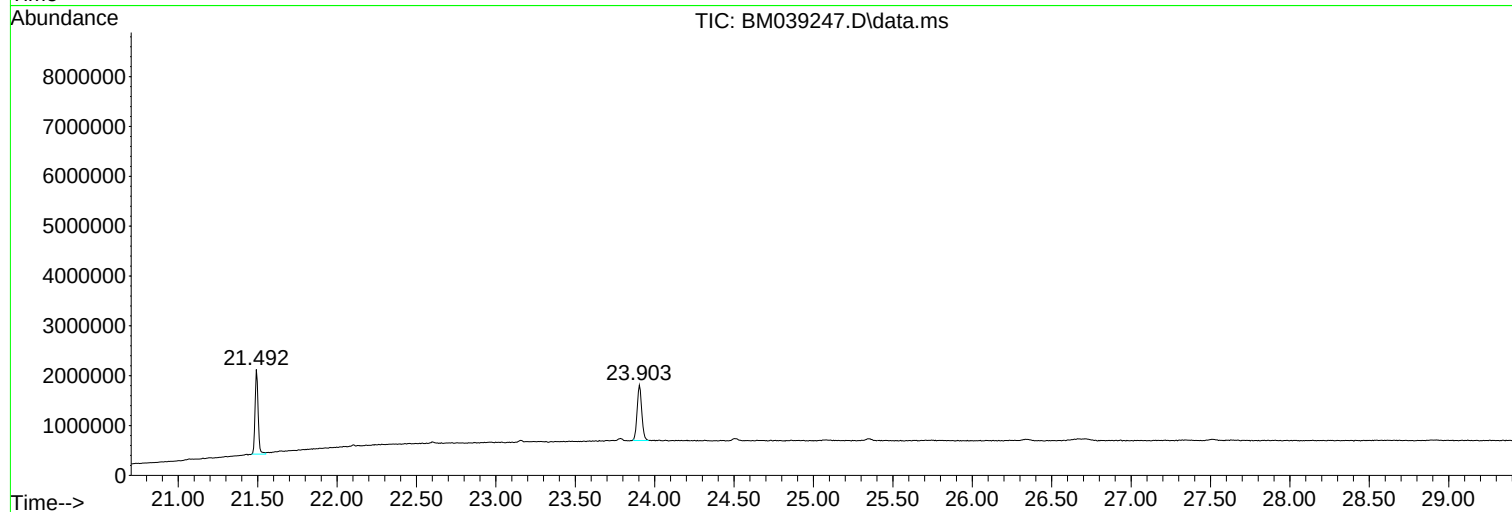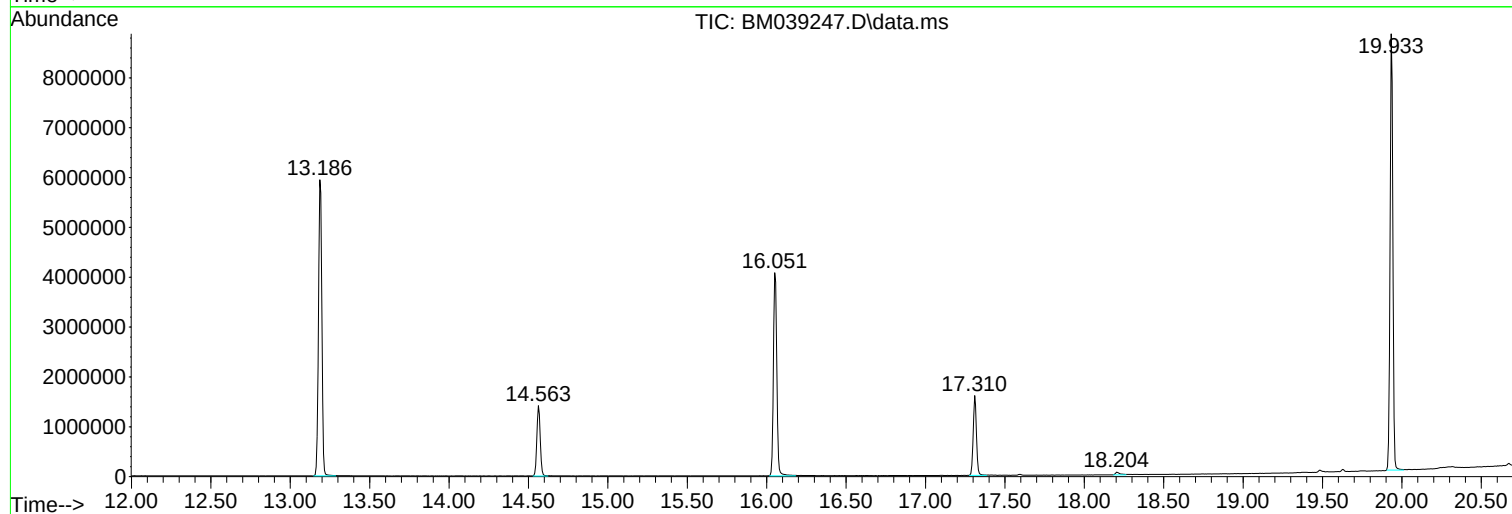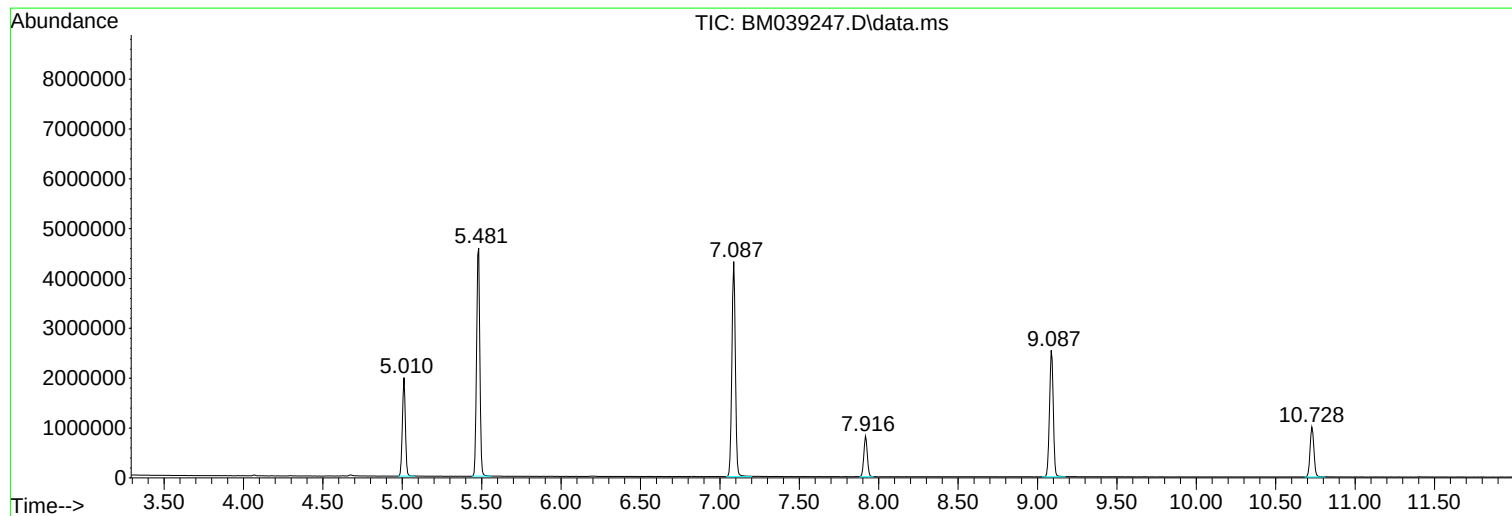

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039247.D
Acq On : 31 Mar 2023 11:08
Operator : CG/JU
Sample : PB151761BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB151761BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.010	41.66 ng	2614530	1,4-Dichlorobenzene-d4	7.916	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9

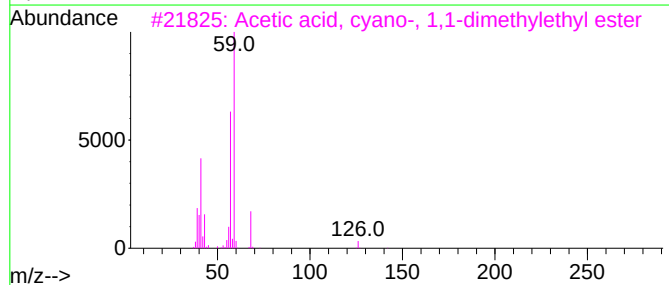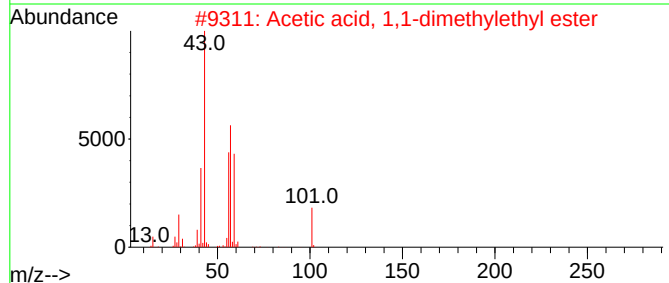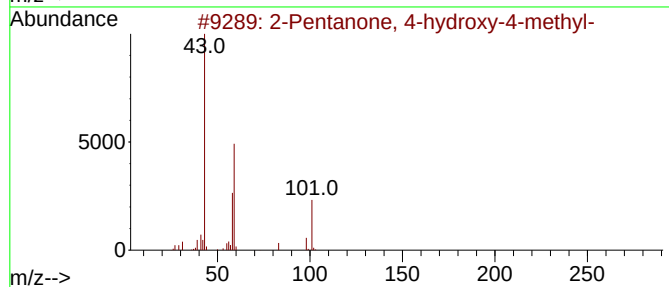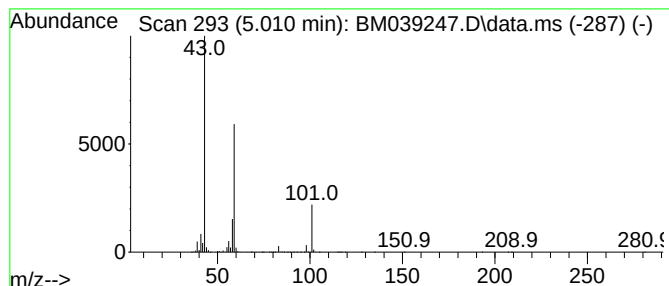

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039247.D
Acq On : 31 Mar 2023 11:08
Operator : CG/JU
Sample : PB151761BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151761BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.010	41.7	ng	2614530	1	7.916	1255030	20.0