

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
 Data File : BM039255.D
 Acq On : 31 Mar 2023 16:17
 Operator : CG/JU
 Sample : PB151822BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB151822BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM039255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	287	294	304	rBV	2858103	3985039	28.50%	4.836%
2	5.481	366	373	389	rBV	6981854	9972915	71.33%	12.103%
3	7.093	639	647	667	rBV	6399934	9956830	71.22%	12.083%
4	7.916	781	787	795	rBV	1194802	1893533	13.54%	2.298%
5	9.092	974	987	1002	rBV	3929521	6473147	46.30%	7.855%
6	10.728	1256	1265	1282	rBV	1530145	2565458	18.35%	3.113%
7	13.192	1676	1684	1697	rBV	8806506	13328863	95.34%	16.175%
8	14.563	1910	1917	1926	rBV	2169291	3071993	21.97%	3.728%
9	16.051	2164	2170	2189	rBV	6005214	8919407	63.80%	10.824%
10	17.310	2378	2384	2397	rBV	2295295	3241290	23.18%	3.933%
11	18.204	2532	2536	2545	rBV	128815	245015	1.75%	0.297%
12	19.933	2825	2830	2842	rBV	11056283	13980561	100.00%	16.966%
13	21.492	3091	3095	3102	rBV	1889993	2474690	17.70%	3.003%
14	23.903	3499	3505	3518	rVB2	1133154	2294258	16.41%	2.784%




Sum of corrected areas: 82402999

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039255.D
Acq On : 31 Mar 2023 16:17
Operator : CG/JU
Sample : PB151822BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151822BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

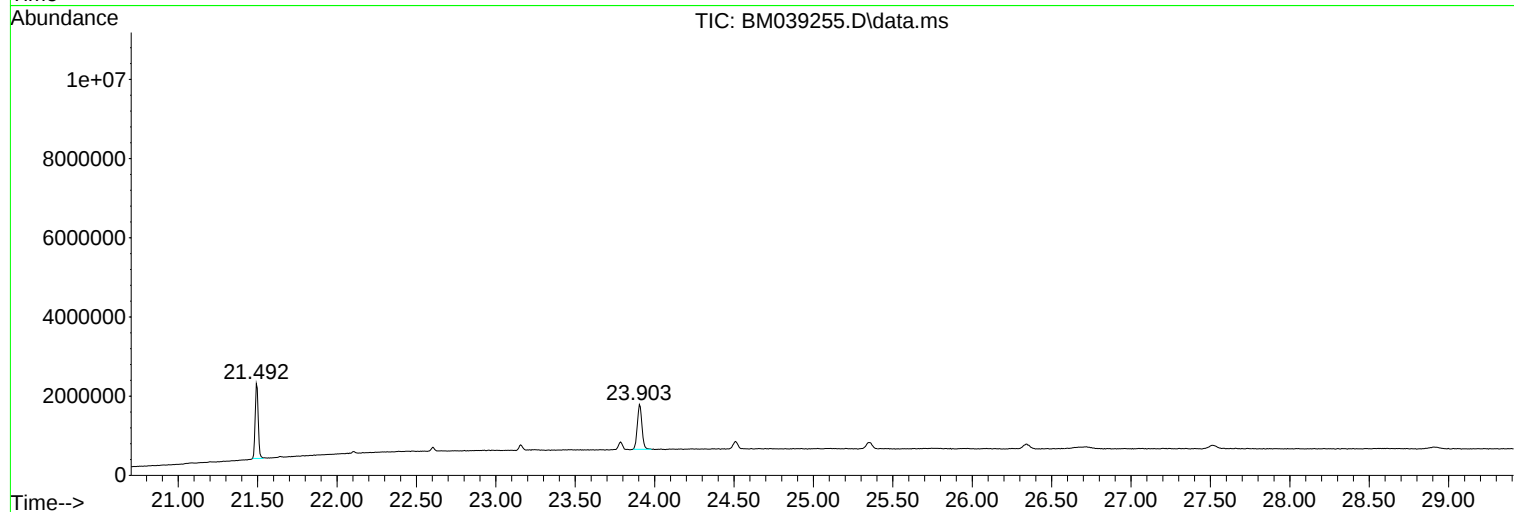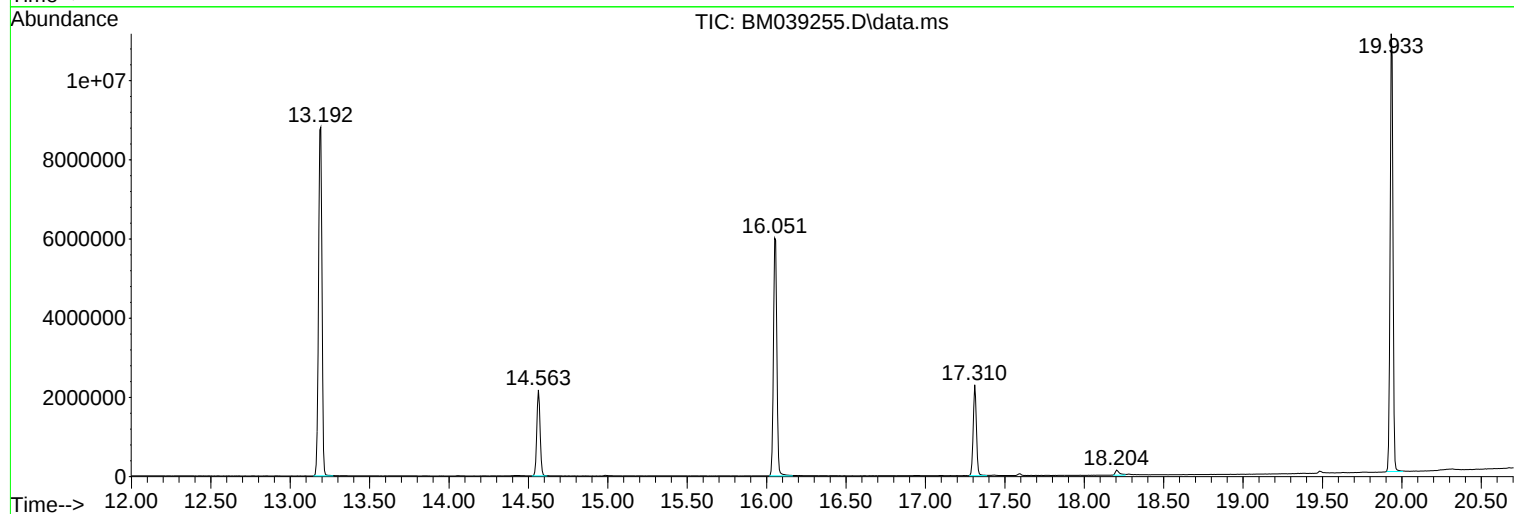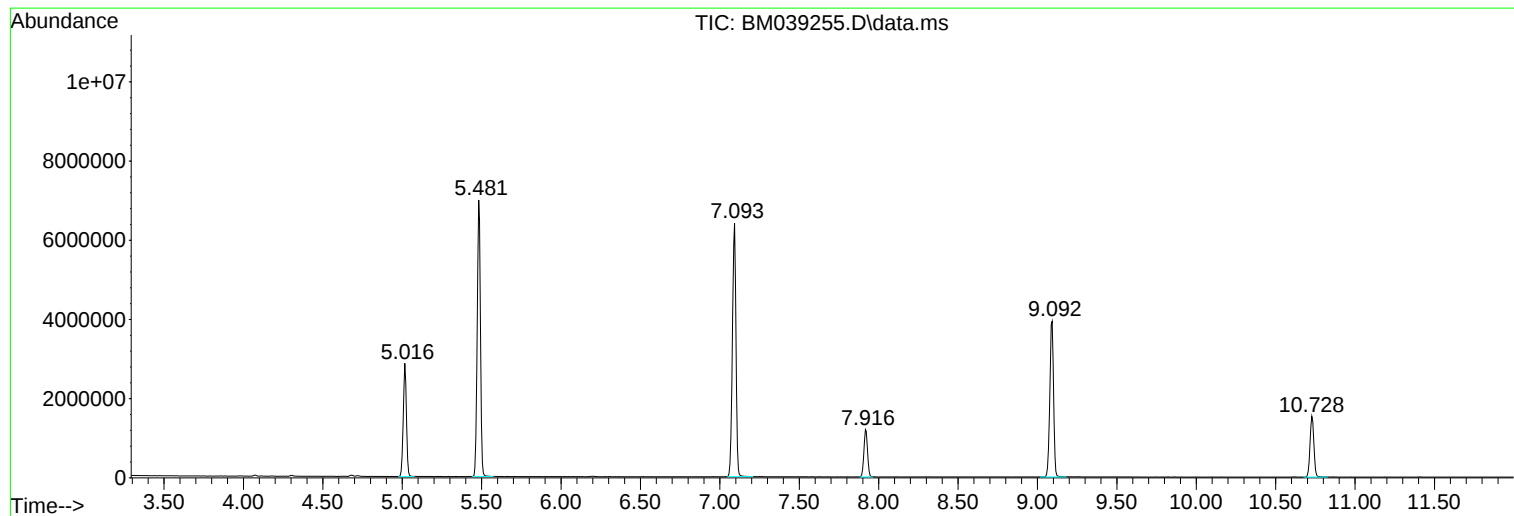

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039255.D
Acq On : 31 Mar 2023 16:17
Operator : CG/JU
Sample : PB151822BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151822BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.016	42.09 ng	3985040	1,4-Dichlorobenzene-d4	7.916

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

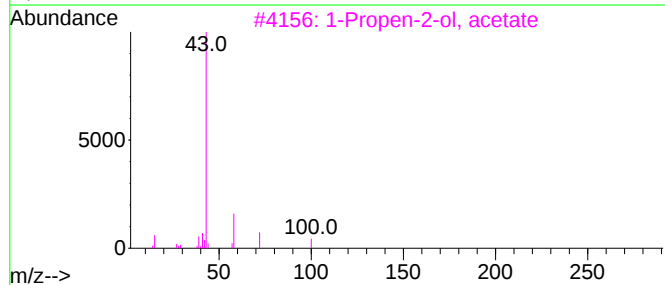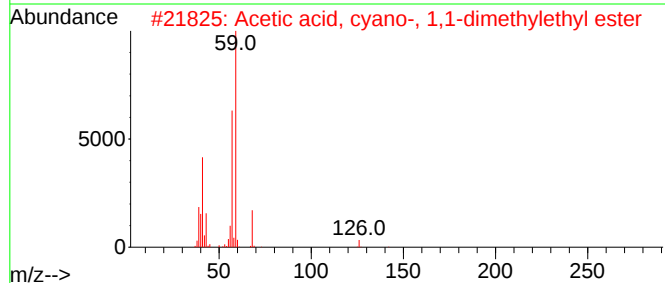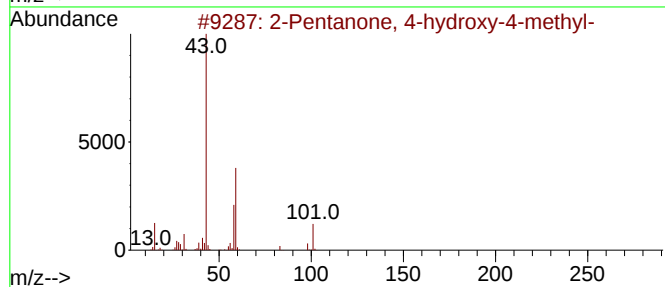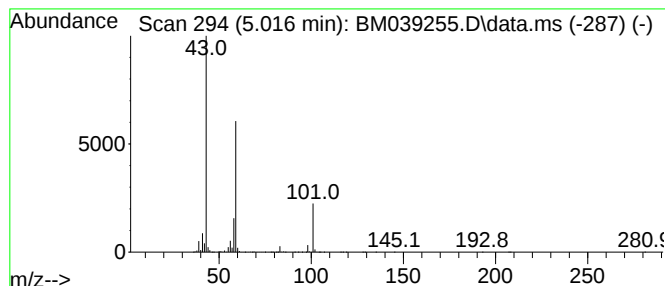

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039255.D
Acq On : 31 Mar 2023 16:17
Operator : CG/JU
Sample : PB151822BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151822BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.016	42.1	ng	3985040	1	7.916	1893530	20.0