


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
 Data File : BM039245.D
 Acq On : 31 Mar 2023 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 31 17:03:41 2023

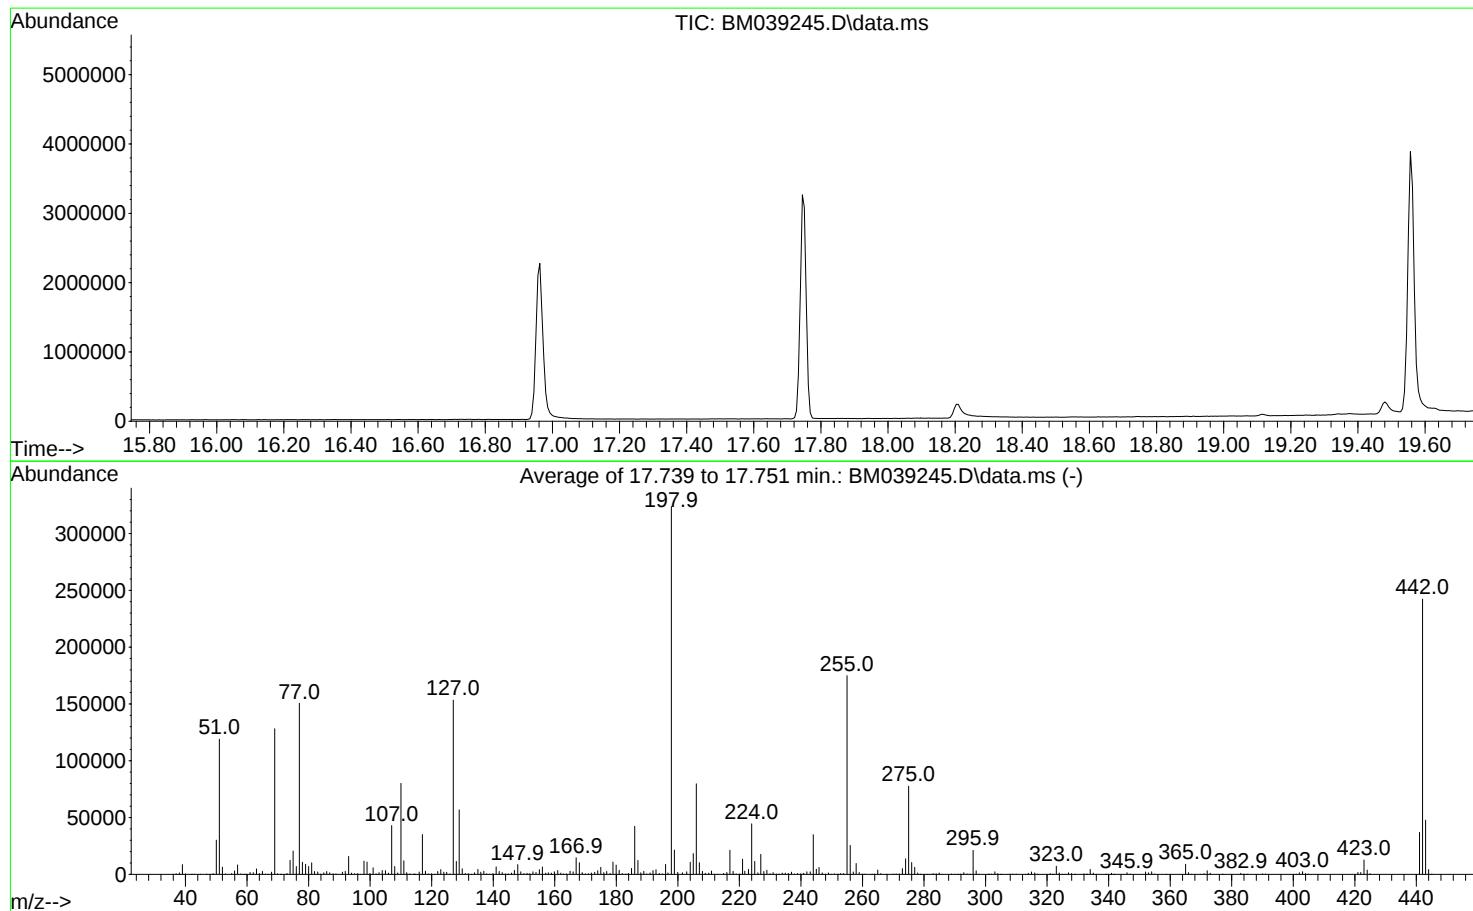




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	119043	PASS
68	69	0.00	2	1.5	1980	PASS
69	198	0.00	100	39.6	128120	PASS
70	69	0.00	2	0.4	524	PASS
127	198	10	80	47.4	153416	PASS
197	198	0.00	2	0.4	1282	PASS
198	198	100	100	100.0	323819	PASS
199	198	5	9	6.6	21443	PASS
275	198	10	60	24.0	77563	PASS
365	198	1	100	2.7	8861	PASS
441	198	0.01	100	11.4	36965	PASS
442	442	50	100	100.0	242221	PASS
443	442	15	24	19.7	47707	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039245.D
Acq On : 31 Mar 2023 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 01 05:03:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 17:03:41 2023
Response via : Initial Calibration

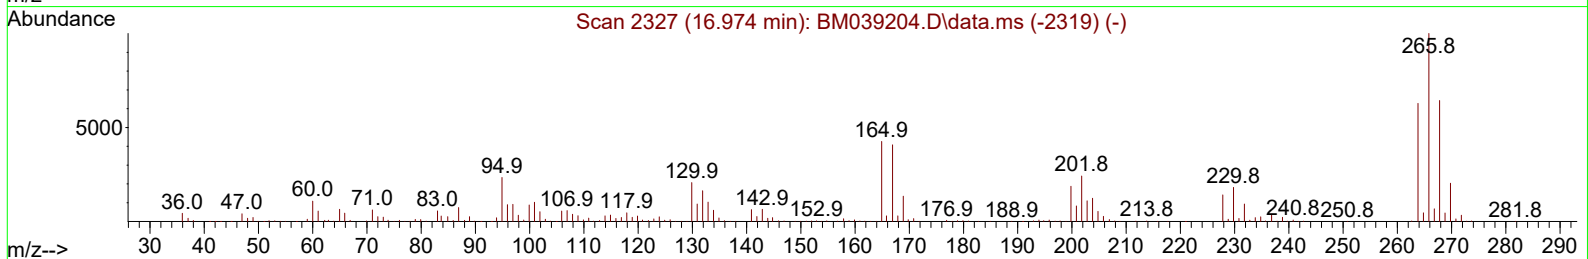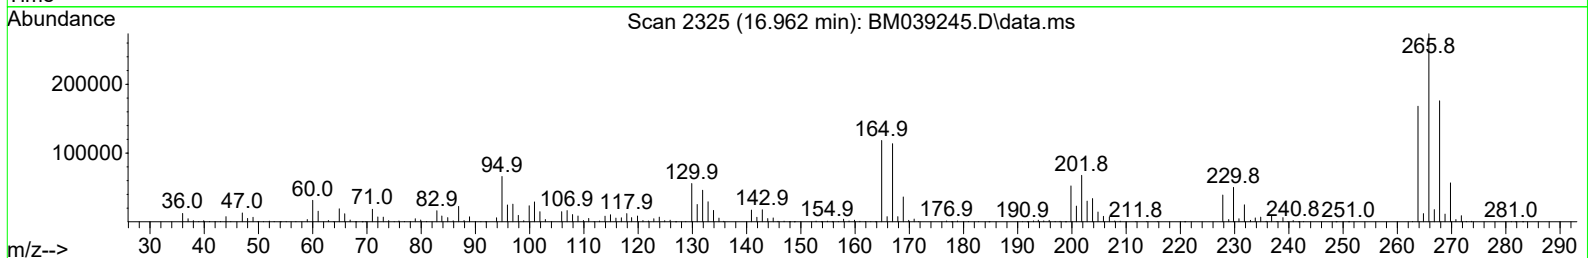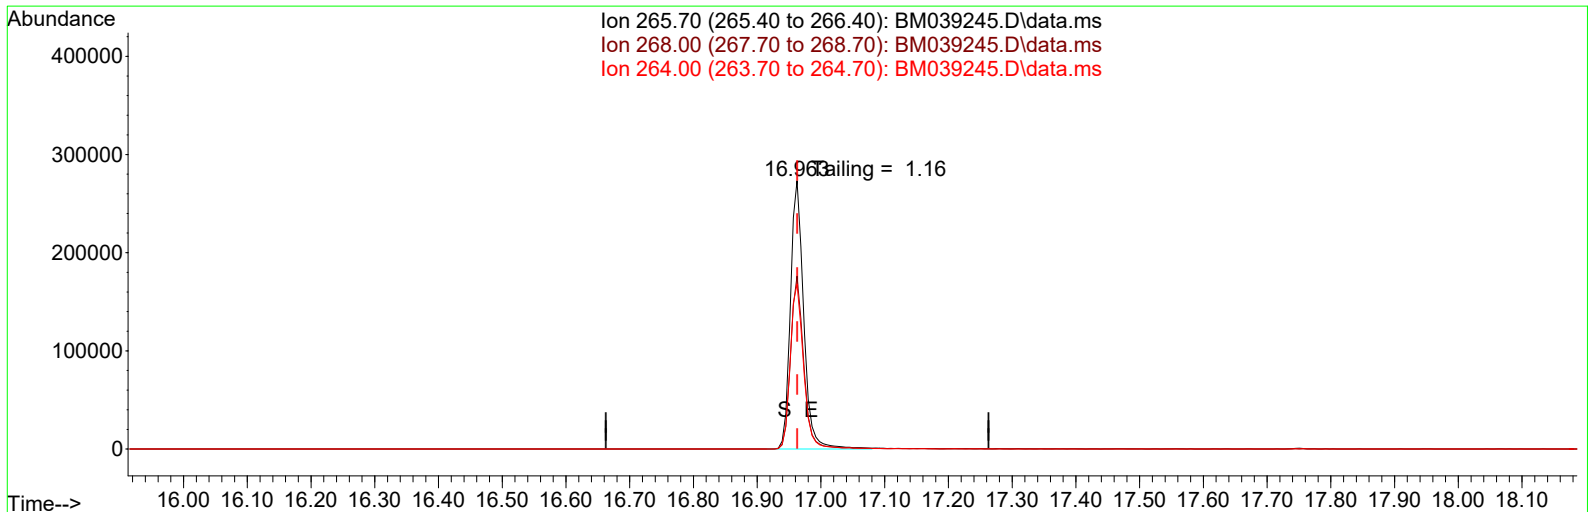

TIC: BM039245.D\data.ms

(70) Pentachlorophenol (C)

16.962min (-0.000) 169164.37 ng




response 400535

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.40
264.00	62.80	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
 Data File : BM039245.D
 Acq On : 31 Mar 2023 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 05:03:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 17:03:41 2023
 Response via : Initial Calibration

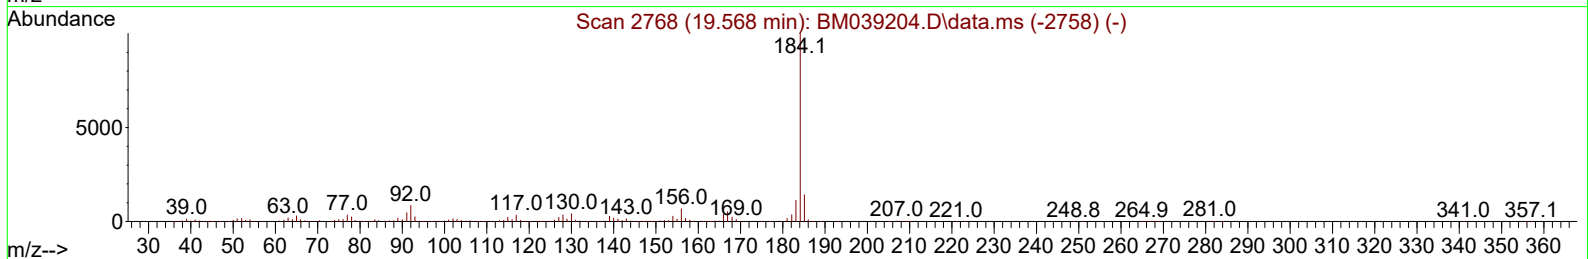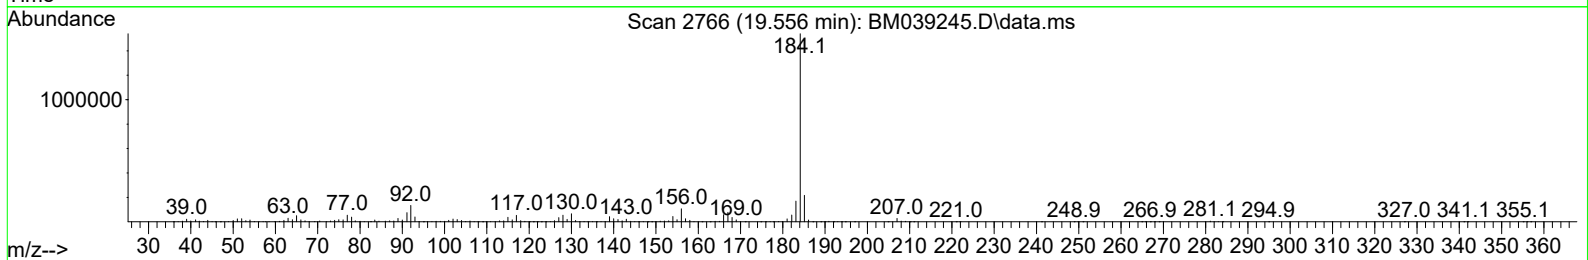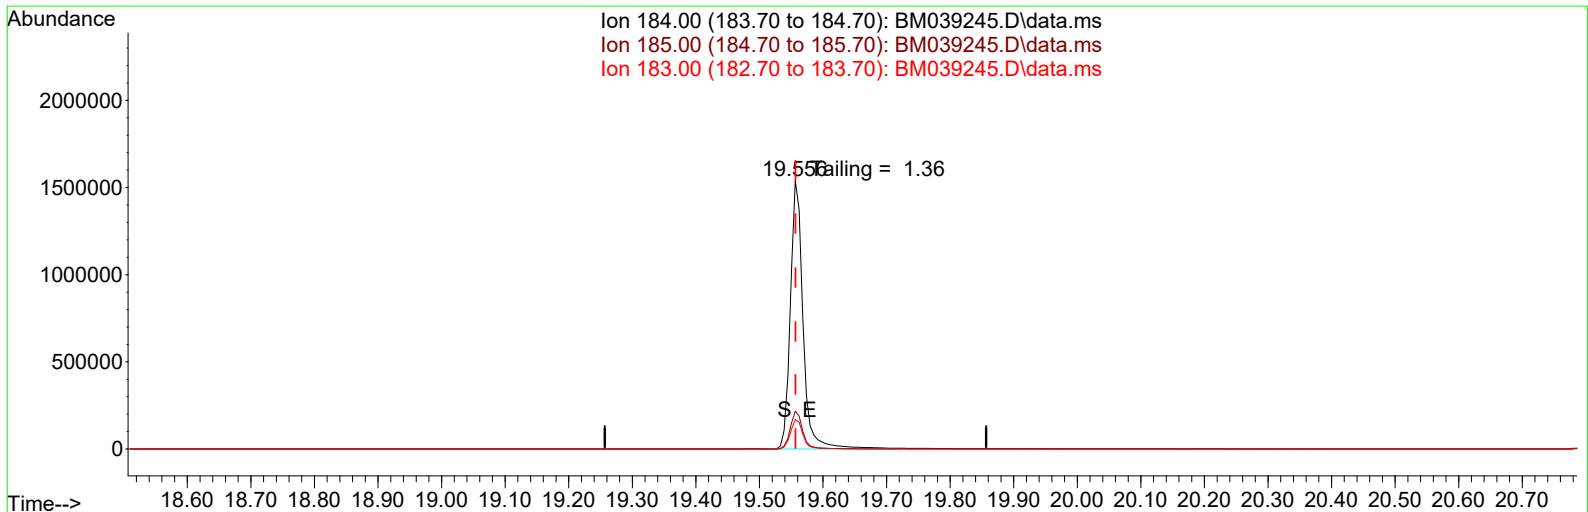

TIC: BM039245.D\data.ms

(77) Benzidine

19.556min (-0.000) 71443.72 ng

response 2168978

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.06
183.00	11.20	11.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2023	BNA_M	<u>BM039245.D</u>
Compound Name	Response	Retention Time
DDT	1155541	20.786
DDD	14114	20.398
DDE	815	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14929	1170470	1.28

Instrument :
BNA_M
ClientSampleId :
DFTPP