


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039253.D
Acq On : 31 Mar 2023 15:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 31 17:03:41 2023

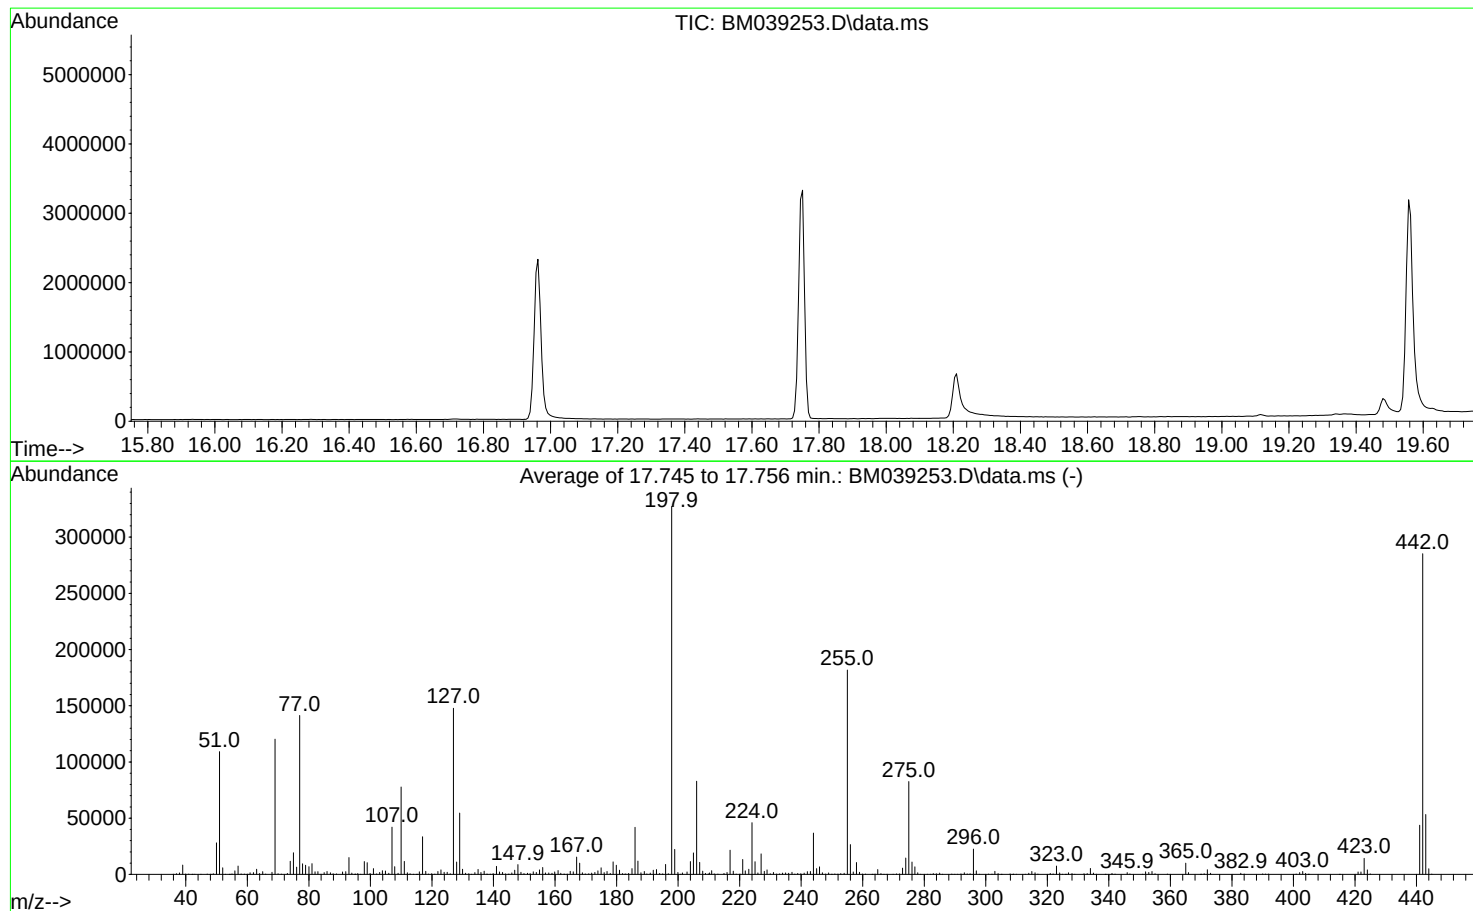




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	109150	PASS
68	69	0.00	2	1.5	1864	PASS
69	198	0.00	100	36.8	120308	PASS
70	69	0.00	2	0.5	551	PASS
127	198	10	80	45.1	147731	PASS
197	198	0.00	2	0.2	548	PASS
198	198	100	100	100.0	327253	PASS
199	198	5	9	6.8	22255	PASS
275	198	10	60	25.2	82509	PASS
365	198	1	100	3.0	9964	PASS
441	198	0.01	100	13.4	43728	PASS
442	442	50	100	100.0	285227	PASS
443	442	15	24	18.7	53261	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM033123\
Data File : BM039253.D
Acq On : 31 Mar 2023 15:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 01 05:09:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 17:03:41 2023
Response via : Initial Calibration

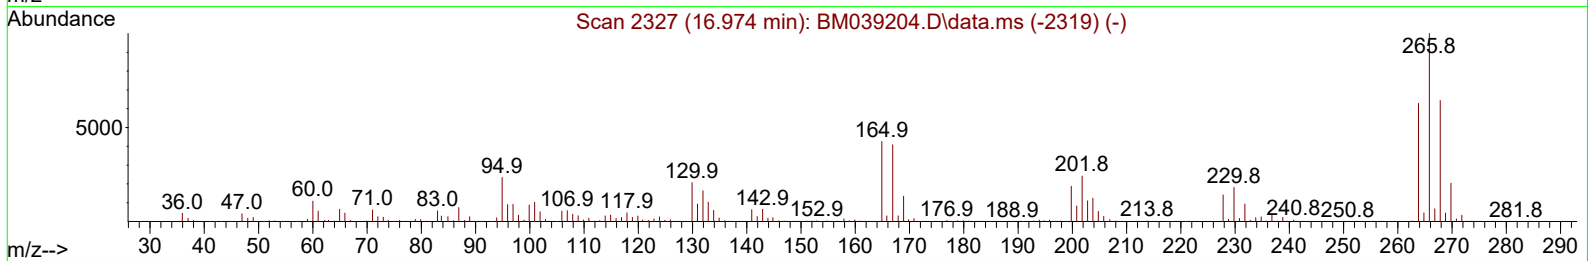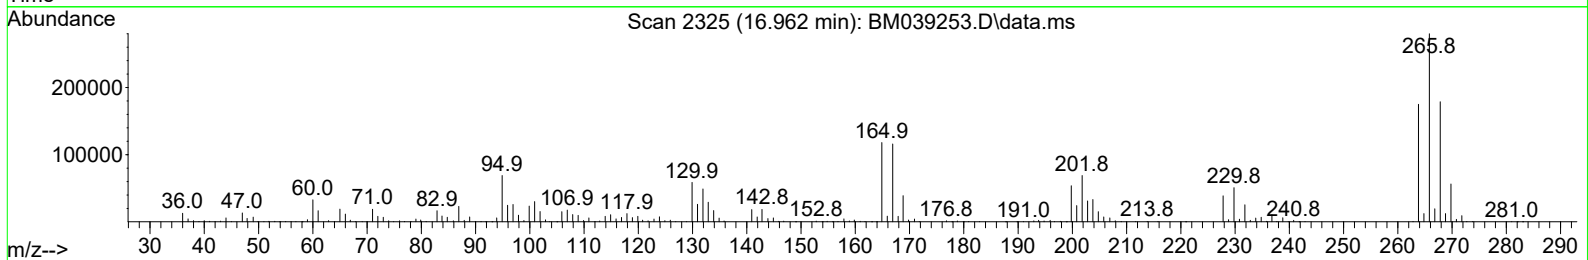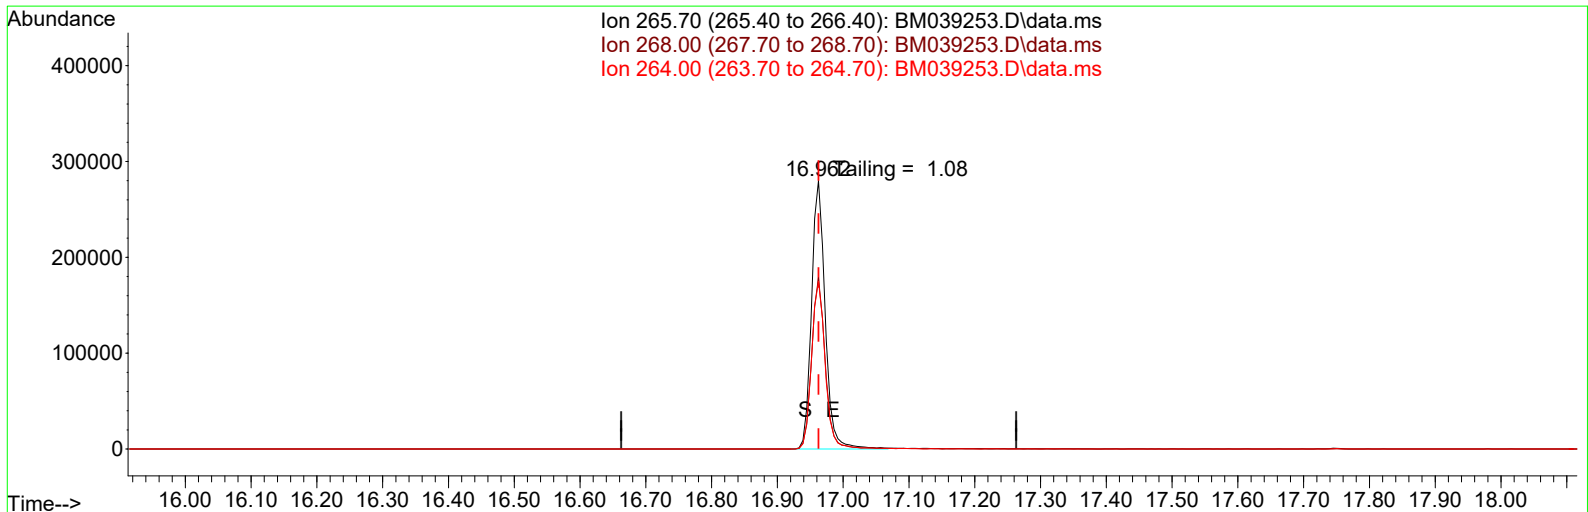

TIC: BM039253.D\data.ms

(70) Pentachlorophenol (C)

16.962min (-0.000) 374739.91 ng

response 404725

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.83
264.00	62.80	62.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2023	BNA_M	<u>BM039253.D</u>
Compound Name	Response	Retention Time
DDT	1138675	20.786
DDD	14528	20.397
DDE	836	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15364	1154039	1.33

Instrument :
BNA_M
ClientSampleId :
DFTPP