

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040115\
 Data File : BM000800.D
 Acq On : 02 Apr 2015 00:42
 Operator : TP/IZ
 Sample : PB82421BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB82421BL

Quant Time: Apr 02 02:52:55 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM033115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 01 04:17:30 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	27333	5.00	ng	0.00
4) Naphthalene-d8	10.40	136	93141	5.00	ng	0.00
8) Acenaphthene-d10	14.28	164	45644	5.00	ng	0.00
13) Phenanthrene-d10	17.01	188	101981	5.00	ng	0.00
19) Chrysene-d12	21.22	240	80820	5.00	ng	0.00
25) Perylene-d12	23.39	264	74412	5.00	ng	0.00
System Monitoring Compounds						
5) Nitrobenzene-d5	8.77	82	32596	5.76	ng	0.00
9) 2-Fluorobiphenyl	12.89	172	107751	7.61	ng	0.00
21) Terphenyl-d14	19.65	244	100112	10.29	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040115\
Data File : BM000800.D
Acq On : 02 Apr 2015 00:42
Operator : TP/IZ
Sample : PB82421BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB82421BL

Quant Time: Apr 02 02:52:55 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM033115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 01 04:17:30 2015
Response via : Initial Calibration

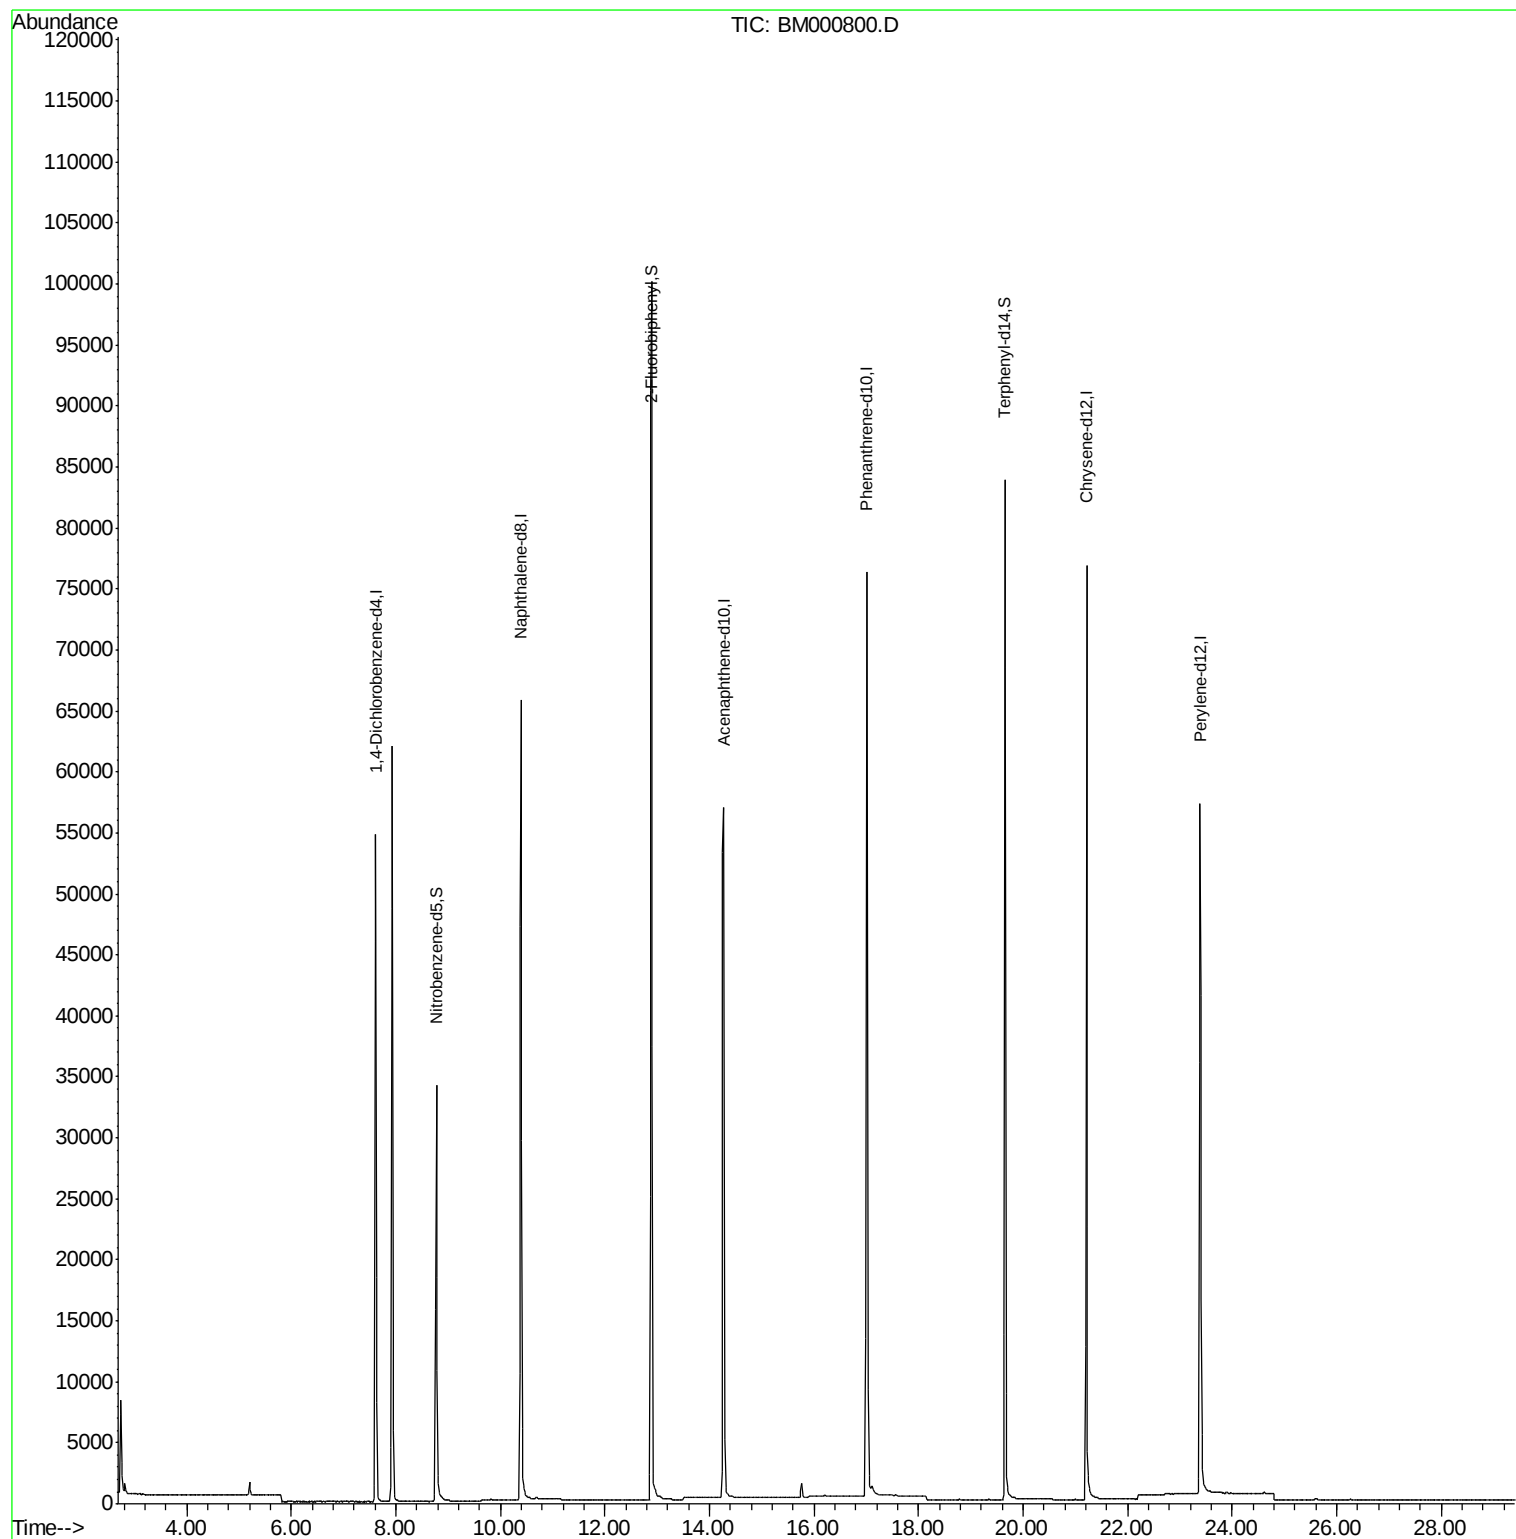

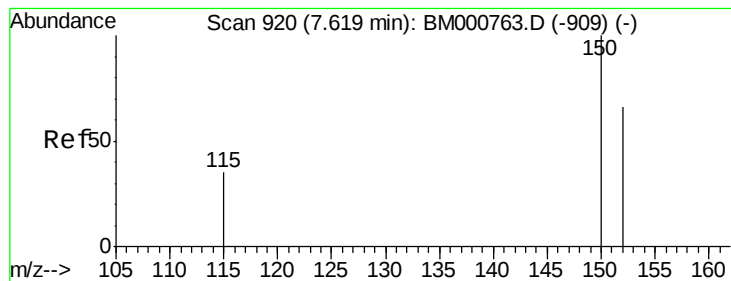

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.61 min Scan# 919

Delta R.T. -0.01 min

Lab File: BM000800.D

Acq: 02 Apr 2015 00:42

Instrument :

BNA_M

ClientSampleId :

PB82421BL


Tgt Ion:152 Resp: 27333

Ion Ratio Lower Upper

152 100

150 160.0 120.8 181.2




115 59.6 42.7 64.1

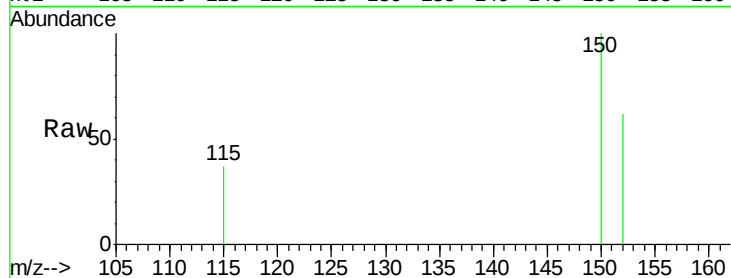

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

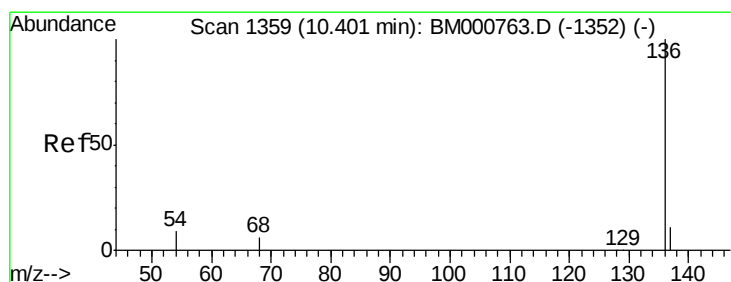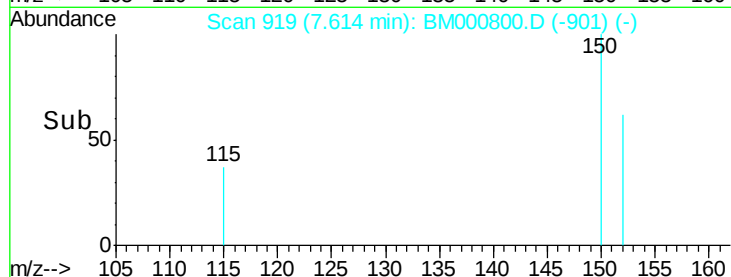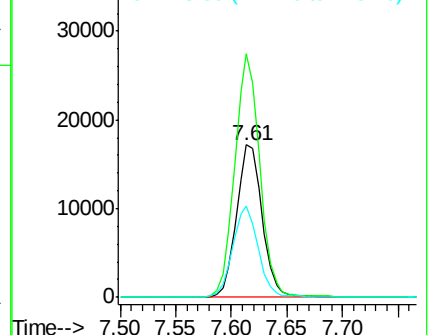

#4

Naphthalene-d8

Concen: 5.00 ng

RT: 10.40 min Scan# 1359

Delta R.T. -0.00 min

Lab File: BM000800.D

Acq: 02 Apr 2015 00:42


Tgt Ion:136 Resp: 93141

Ion Ratio Lower Upper

136 100

137 10.9 8.6 12.8



54 7.5 7.0 10.6

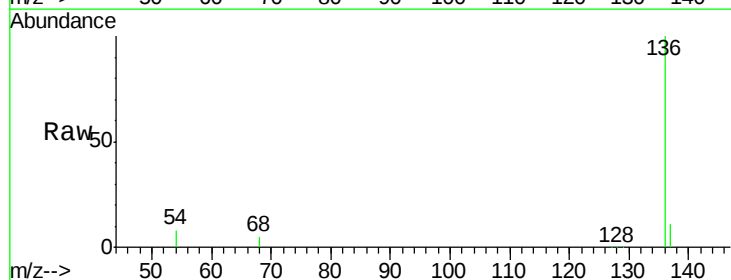


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BM

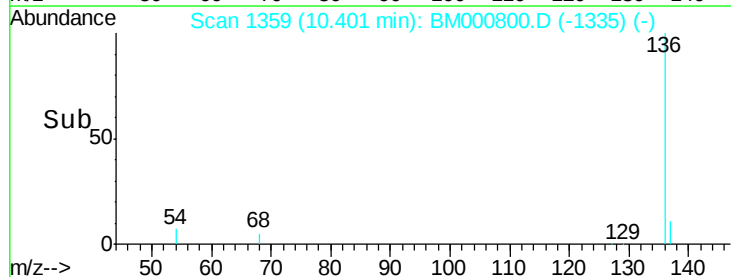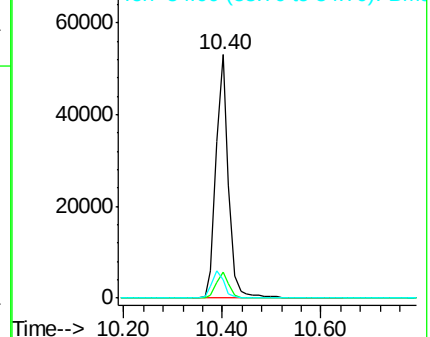

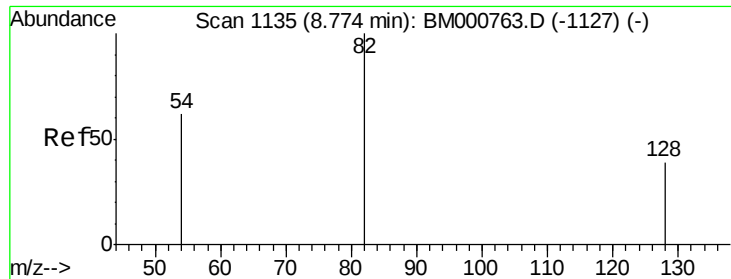

#5

Nitrobenzene-d5

Concen: 5.76 ng

RT: 8.77 min Scan# 1135

Delta R.T. 0.00 min

Lab File: BM000800.D

Acq: 02 Apr 2015 00:42

Instrument :

BNA_M

ClientSampleId :

PB82421BL


Tgt Ion: 82 Resp: 32596

Ion Ratio Lower Upper

82 100

128 41.0 32.2 48.2

54 59.0 50.2 75.4


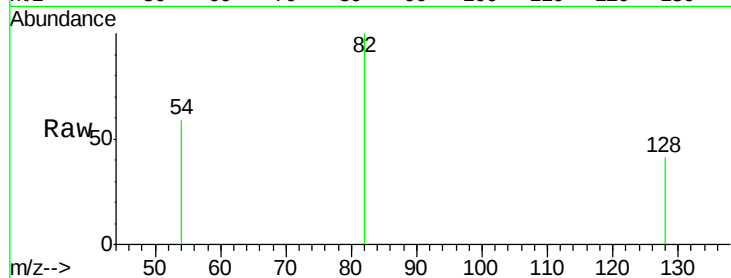


Abundance Ion 82.00 (81.70 to 82.70): BM000800.D (-1081) (-)

Ion 128.00 (127.70 to 128.70): BM000800.D (-1081) (-)

Ion 54.00 (53.70 to 54.70): BM000800.D (-1081) (-)

Time-->

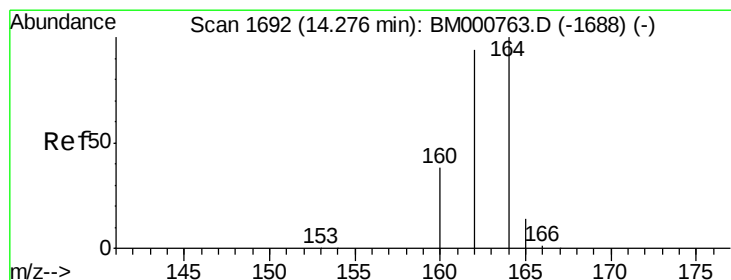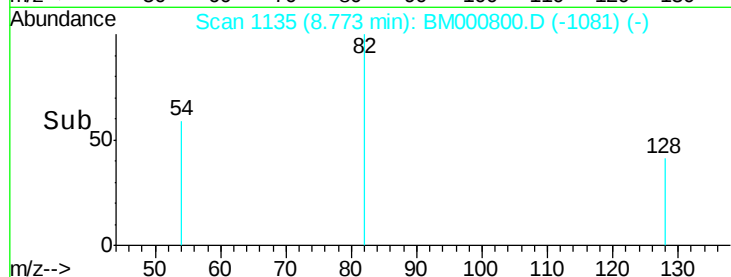

#8

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.28 min Scan# 1692

Delta R.T. -0.00 min

Lab File: BM000800.D

Acq: 02 Apr 2015 00:42


Tgt Ion: 164 Resp: 45644

Ion Ratio Lower Upper

164 100

162 91.5 75.4 113.2

160 36.6 30.8 46.2

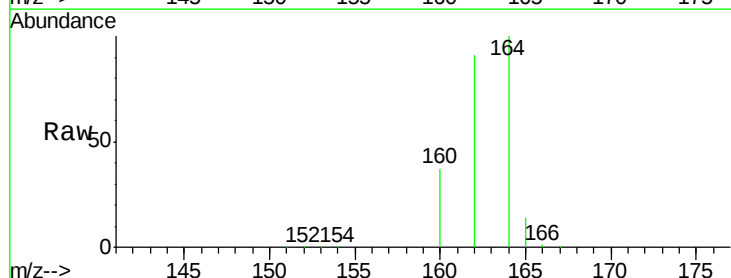



Abundance Ion 164.00 (163.70 to 164.70): BM000800.D (-1684) (-)

Ion 162.00 (161.70 to 162.70): BM000800.D (-1684) (-)

Ion 160.00 (159.70 to 160.70): BM000800.D (-1684) (-)

Time-->

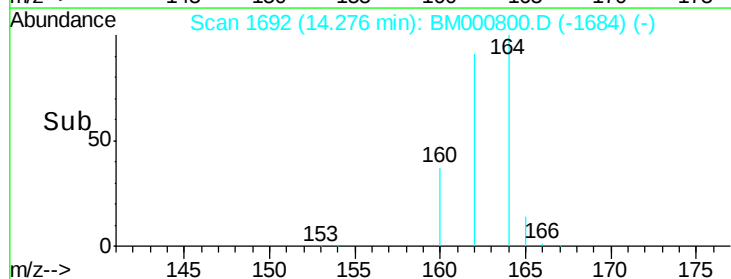

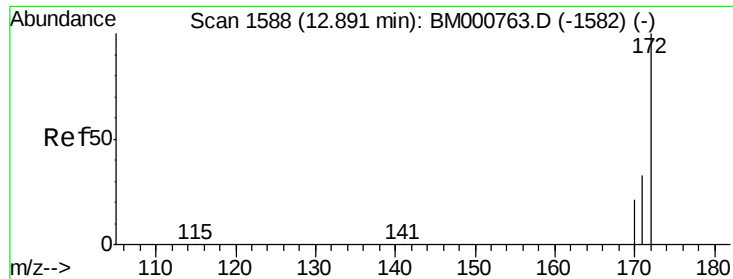

#9

2-Fluorobiphenyl

Concen: 7.61 ng

RT: 12.89 min Scan# 1588

Delta R.T. -0.00 min

Lab File: BM000800.D

Acq: 02 Apr 2015 00:42

Instrument :

BNA_M

ClientSampleId :

PB82421BL


Tgt Ion:172 Resp: 107751

Ion Ratio Lower Upper

172 100

171 31.4 26.6 39.8




170 19.1 17.1 25.7

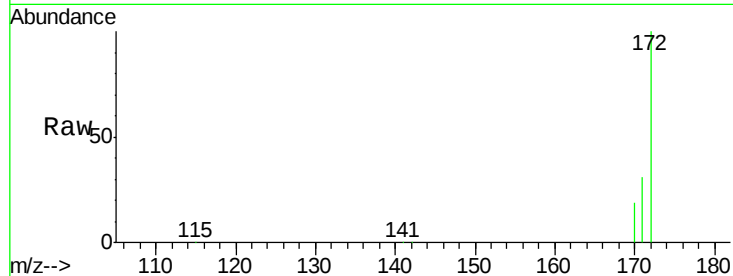

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

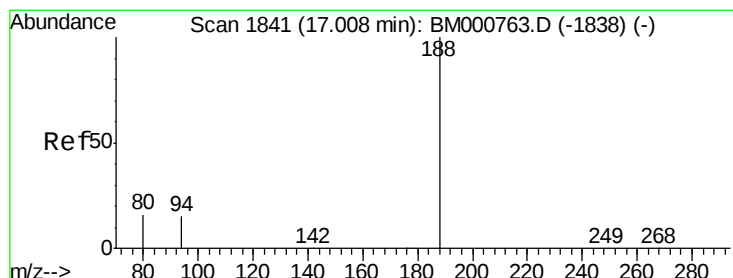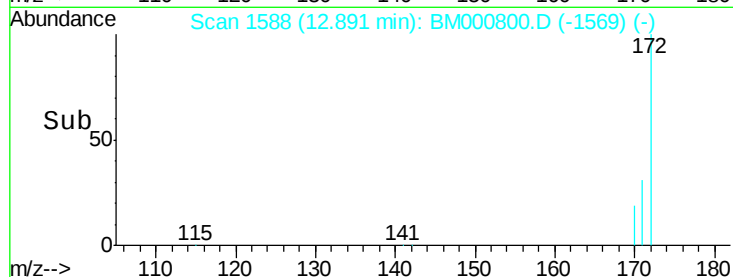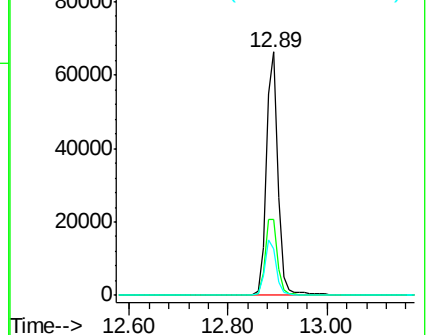

#13

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.01 min Scan# 1841

Delta R.T. 0.00 min

Lab File: BM000800.D

Acq: 02 Apr 2015 00:42


Tgt Ion:188 Resp: 101981

Ion Ratio Lower Upper

188 100

94 7.7 12.0 18.0#



80 7.5 12.8 19.2#

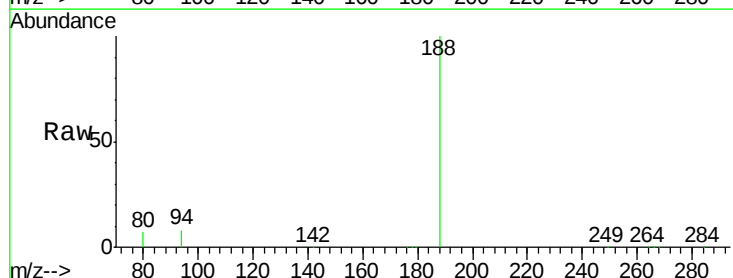


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

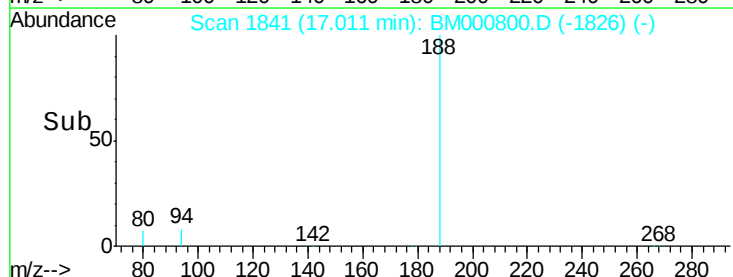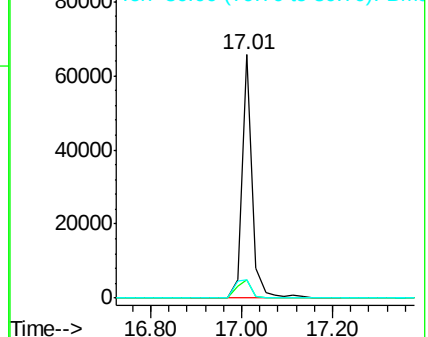

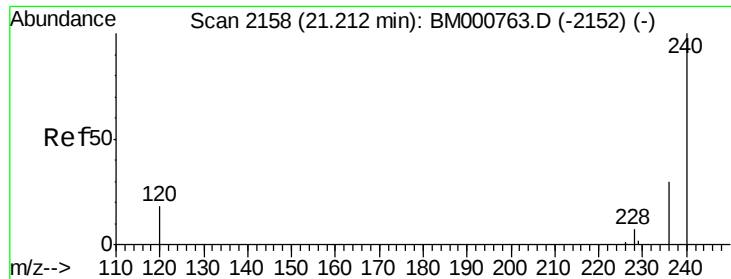

#19

Chrysene-d12

Concen: 5.00 ng

RT: 21.22 min Scan# 2158

Delta R.T. 0.00 min

Lab File: BM000800.D

Acq: 02 Apr 2015 00:42

Instrument :

BNA_M

ClientSampleId :

PB82421BL


Tgt Ion:240 Resp: 80820

Ion Ratio Lower Upper

240 100

120 7.9 14.9 22.3#




236 25.1 24.2 36.4

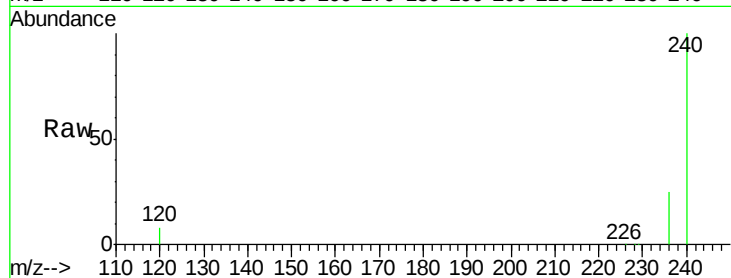

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

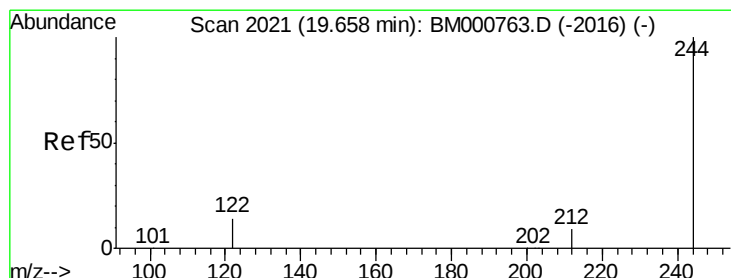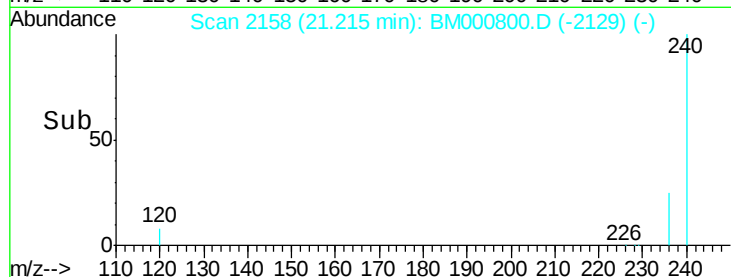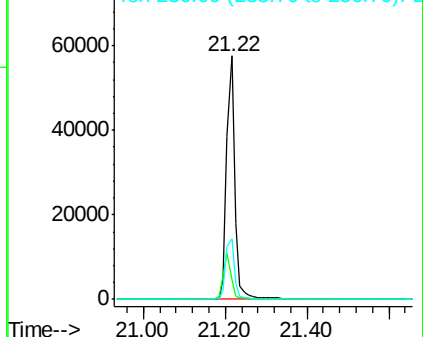

#21

Terphenyl-d14

Concen: 10.29 ng

RT: 19.65 min Scan# 2020

Delta R.T. -0.01 min

Lab File: BM000800.D

Acq: 02 Apr 2015 00:42


Tgt Ion:244 Resp: 100112

Ion Ratio Lower Upper

244 100

212 10.8 7.8 11.6



122 27.8 11.8 17.8#



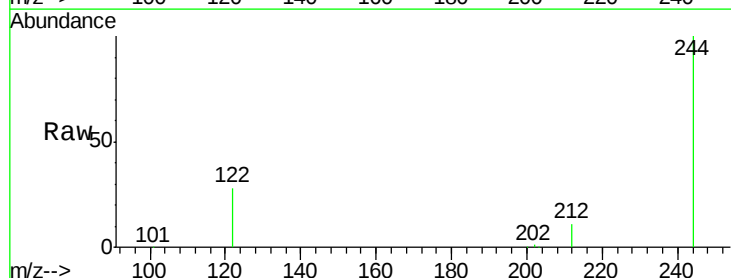


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

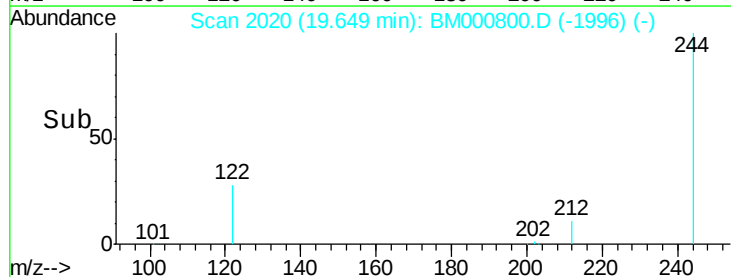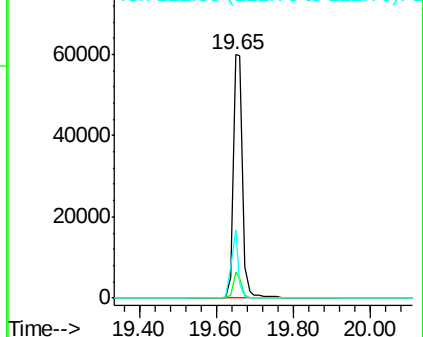

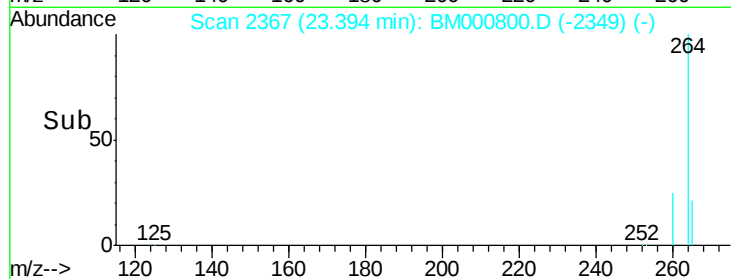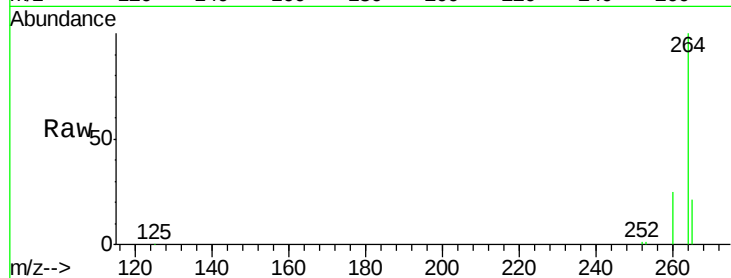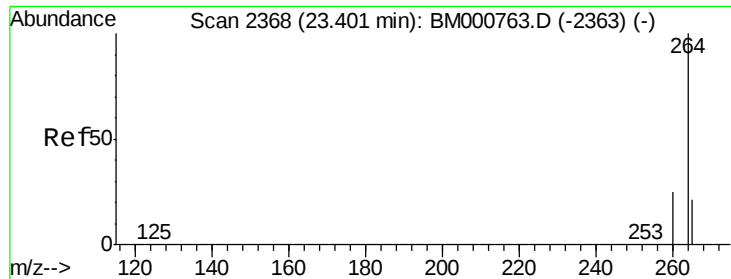

#25

Perylene-d12

Concen: 5.00 ng

RT: 23.39 min Scan# 2367

Delta R.T. -0.01 min

Lab File: BM000800.D

Acq: 02 Apr 2015 00:42

Instrument :

BNA_M

ClientSampleId :

PB82421BL

Tgt Ion: 264 Resp: 74412

Ion Ratio Lower Upper

264 100

260 25.3 20.1 30.1

265 21.3 17.4 26.0

