

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040116\
 Data File : BM004851.D
 Acq On : 01 Apr 2016 21:49
 Operator : UM/SJ
 Sample : PB89344BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK44

Quant Time: Apr 02 00:56:23 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM040116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 02 00:53:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	36171	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	172553	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.46	164	110658	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.20	188	268431	20.00	ng/ul	0.00
78) Chrysene-d12	21.39	240	334209	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	347564	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	5602	6.27	ng/uL	0.00
5) Phenol-d5	6.99	99	106896	33.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	66970	38.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	86071	35.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	89795	33.26	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	45517	37.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	50683	37.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	87131	34.33	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	13.87	166	352561	40.38	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	391231	37.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	60922	35.30	ng/ul	0.00
58) Fluorene-d10	15.46	176	294078	38.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.57	200	54480	33.87	ng/ul	0.00
71) Anthracene-d10	17.30	188	477026	39.72	ng/ul	0.00
79) Pyrene-d10	19.60	212	565436	38.97	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	679310	44.11	ng/ul	0.00

Target Compounds


						Ovalue
12) 2,2'-oxybis(1-Chloropropan	8.53	45	381	0.12	ng/ul#	59
15) N-Nitroso-di-n-propylamine	8.53	70	1946	0.94	ng/ul#	1
21) Isophorone	9.70	82	4151	0.71	ng/ul#	64
46) 2,6-Dinitrotoluene	13.87	165	2426	1.40	ng/ul#	45
59) Fluorene	15.46	166	454	0.05	ng/ul#	9
65) N-Nitrosodiphenylamine	15.57	169	273	0.04	ng/ul#	11
76) Di-n-butylphthalate	18.17	149	300	0.02	ng/ul#	78
80) Pyrene	19.60	202	613	0.03	ng/ul#	1
83) Benzo(a)anthracene	21.40	228	605	0.03	ng/ul#	52
84) Bis(2-ethylhexyl)phthalate	21.30	149	470	0.04	ng/ul#	53
85) Chrysene	21.40	228	605	0.03	ng/ul#	50
87) Di-n-octyl phthalate	22.17	149	113	0.01	ng/ul#	1
91) Benzo(a)pyrene	23.54	252	2067	0.11	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040116\
Data File : BM004851.D
Acq On : 01 Apr 2016 21:49
Operator : UM/SJ
Sample : PB89344BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK44

Quant Time: Apr 02 00:56:23 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 02 00:53:13 2016
Response via : Initial Calibration




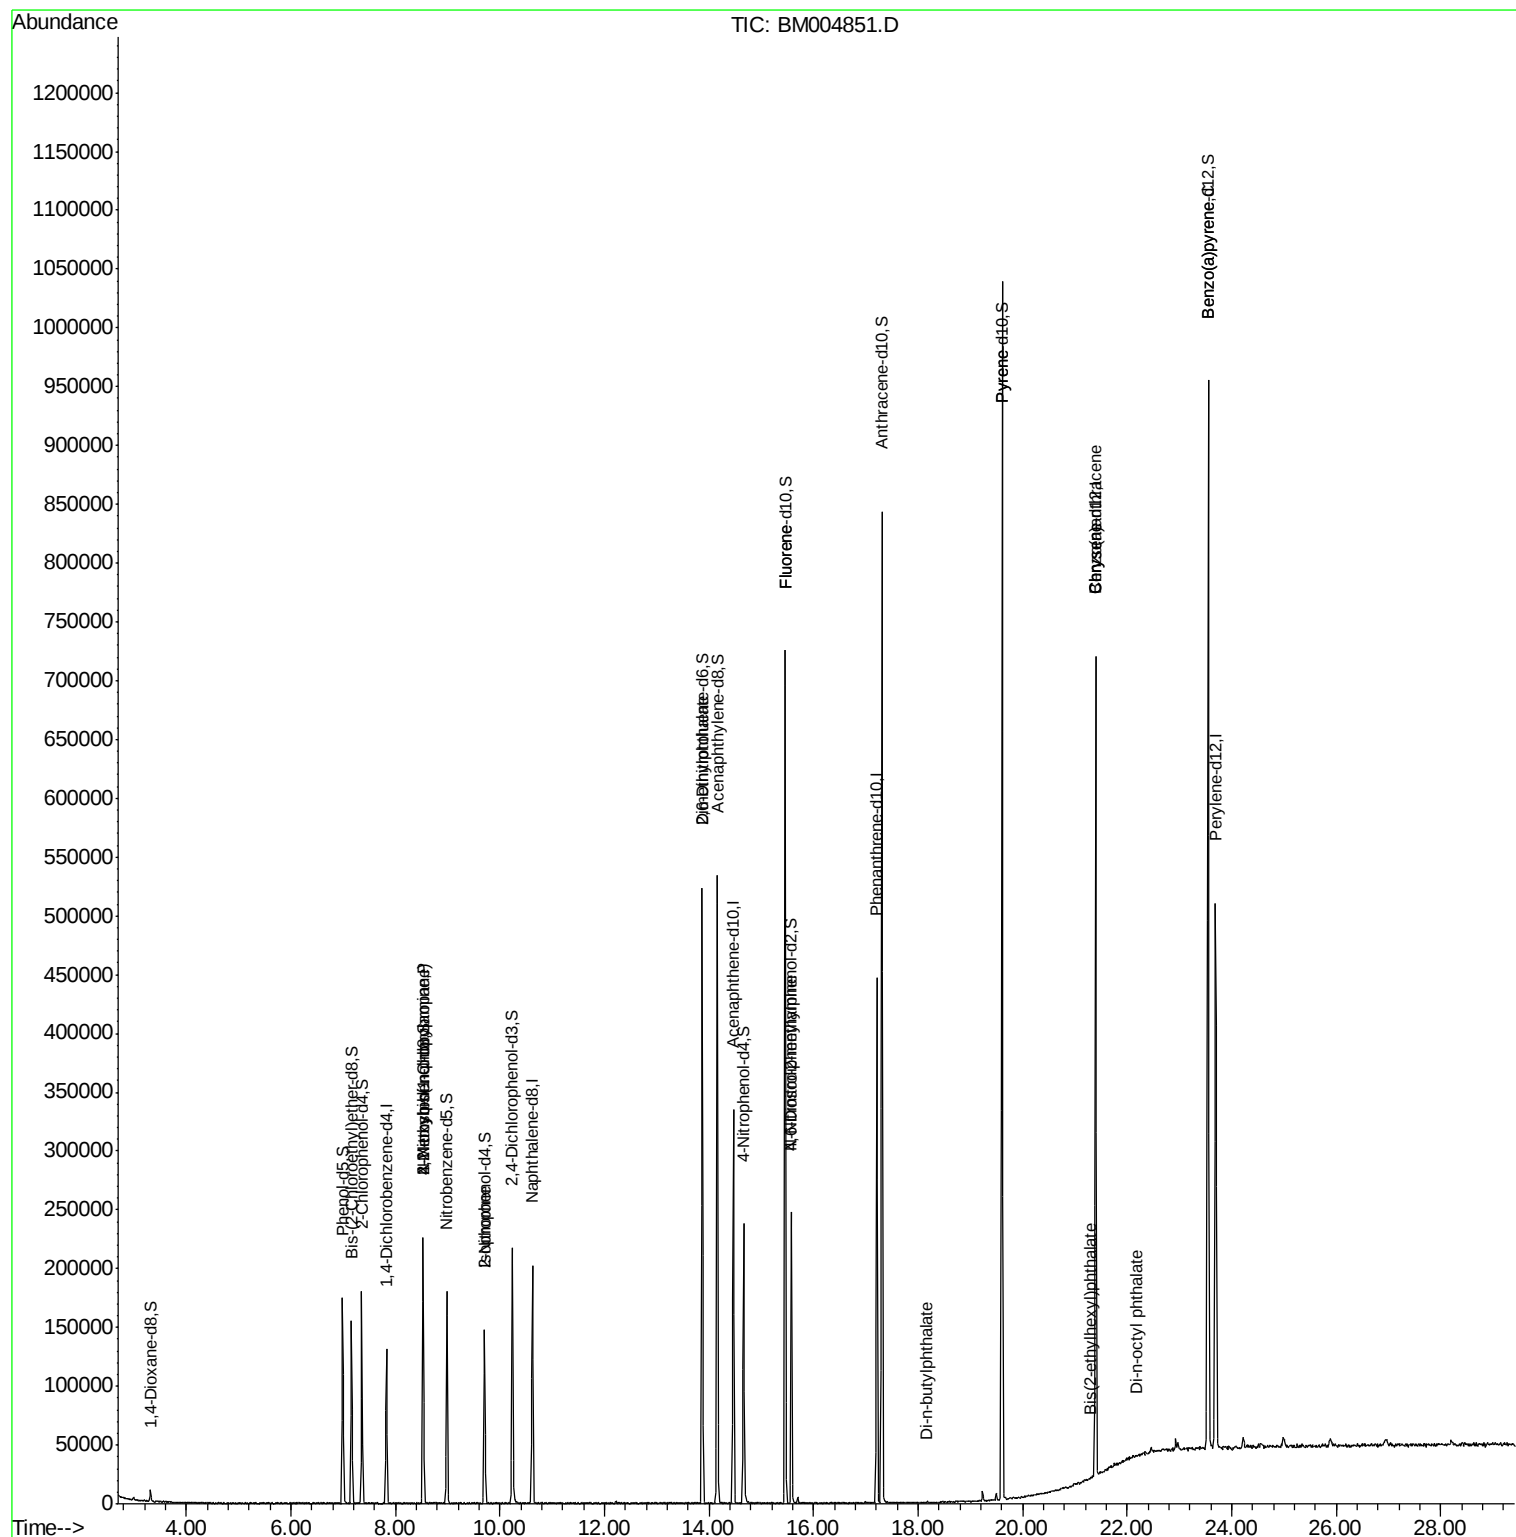


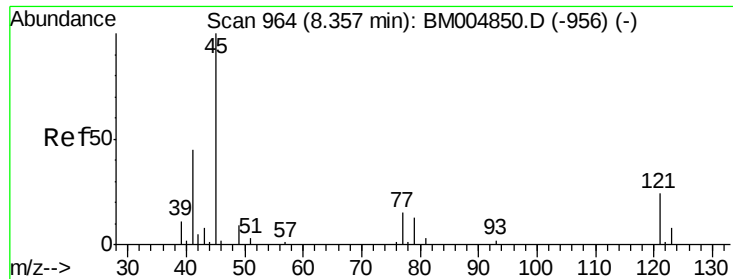

#12
 2,2'-oxvbis(1-Chloropropane)
 Concen: 0.12 ng/ul
 RT: 8.53 min Scan# 993
 Delta R.T. 0.17 min
 Lab File: BM004851.D
 Acq: 01 Apr 2016 21:49




Instrument :
 BNA_M
 ClientSampleId :
 SBLK44


Tot Ion: 45 Resp: 381
 Ion Ratio Lower Upper
 45 100
 77 0.0 15.9 23.9#
 79 0.0 12.5 18.7#

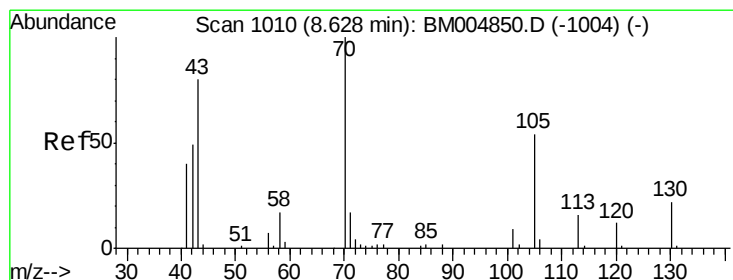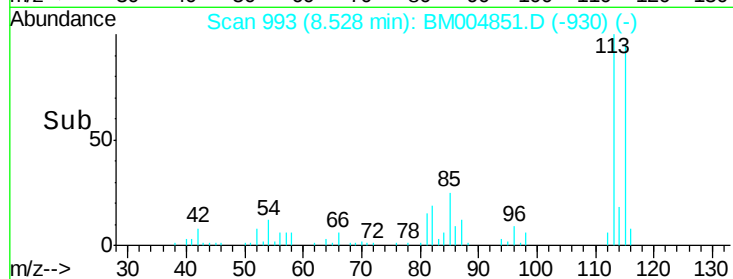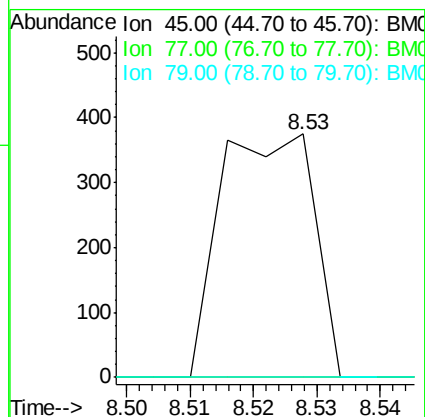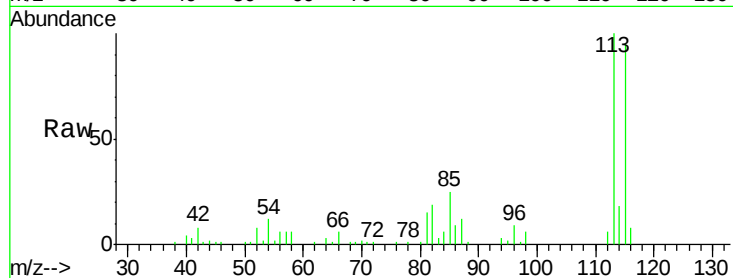

#15
 N-Nitroso-di-n-propylamine
 Concen: 0.94 ng/ul
 RT: 8.53 min Scan# 993
 Delta R.T. -0.10 min
 Lab File: BM004851.D
 Acq: 01 Apr 2016 21:49

Tgt Ion: 70 Resp: 1946
 Ion Ratio Lower Upper
 70 100
 42 319.4 35.4 53.0#
 101 0.0 8.4 12.6#
 130 0.0 18.2 27.4#

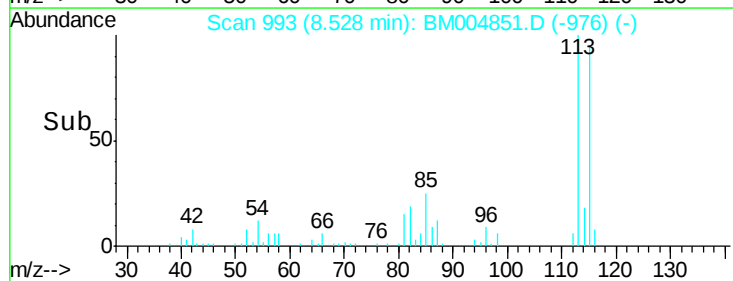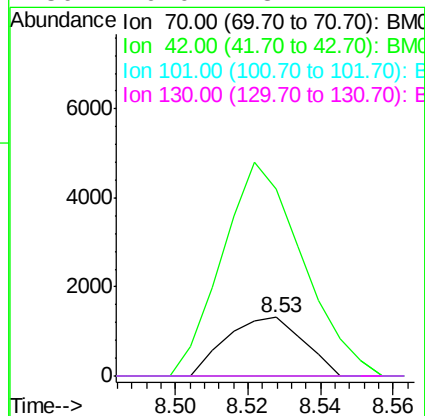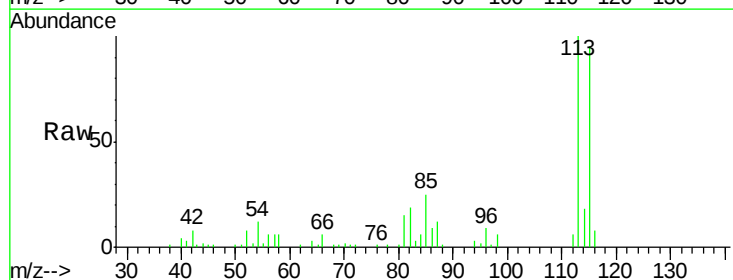

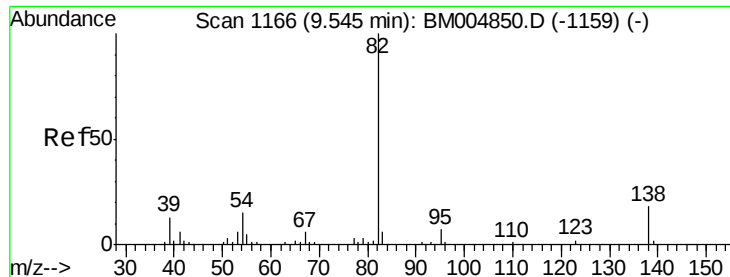

#21

Isophorone

Concen: 0.71 ng/ul

RT: 9.70 min Scan# 1193

Delta R.T. 0.16 min

Lab File: BM004851.D

Acq: 01 Apr 2016 21:49

Instrument :

BNA_M

ClientSampleId :

SBLK44


Tot Ion: 82 Resp: 4151

Ion Ratio Lower Upper

82 100

95 0.0 6.4 9.6#




138 0.0 14.9 22.3#

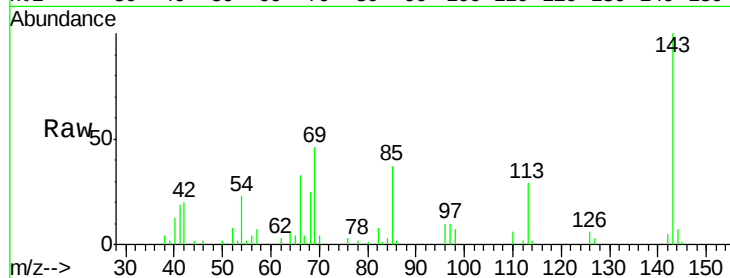

Abundance Ion 82.00 (81.70 to 82.70): BM004851.D (-1159) (-)

Ion 95.00 (94.70 to 95.70): BM004851.D (-1159) (-)

Ion 138.00 (137.70 to 138.70): BM004851.D (-1159) (-)

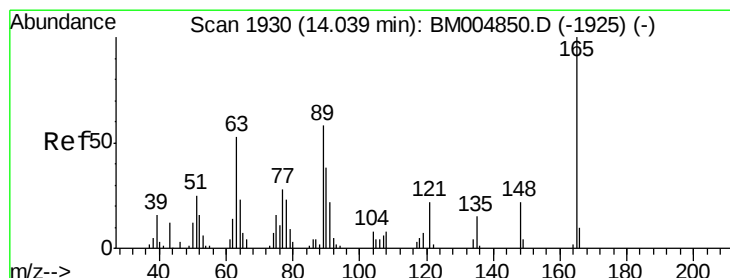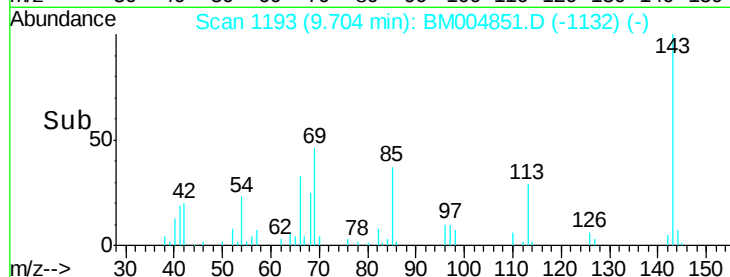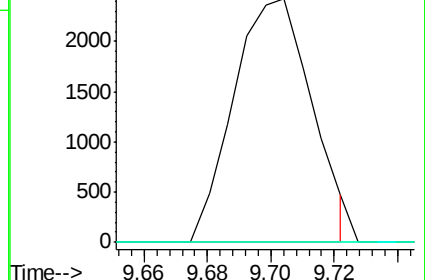

#46

2,6-Dinitrotoluene

Concen: 1.40 ng/ul

RT: 13.87 min Scan# 1902

Delta R.T. -0.16 min

Lab File: BM004851.D

Acq: 01 Apr 2016 21:49


Tgt Ion:165 Resp: 2426

Ion Ratio Lower Upper

165 100

89 0.0 42.4 63.6#



121 22.5 16.6 24.8

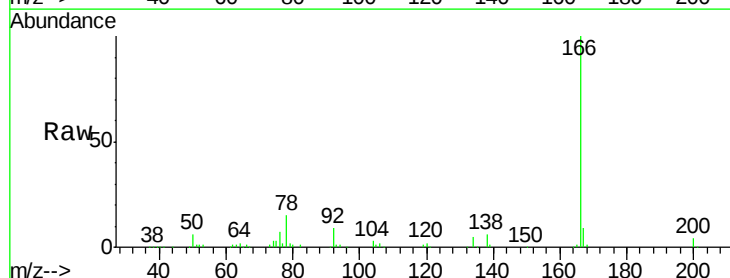


Abundance Ion 165.00 (164.70 to 165.70): BM004851.D (-1896) (-)

Ion 89.00 (88.70 to 89.70): BM004851.D (-1896) (-)

Ion 121.00 (120.70 to 121.70): BM004851.D (-1896) (-)

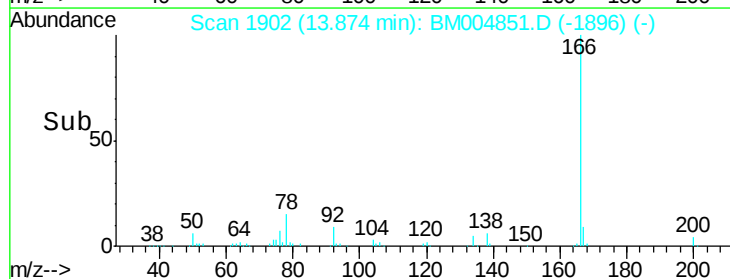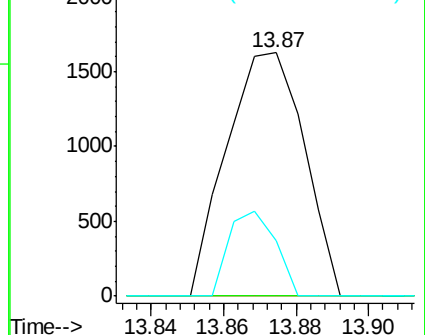

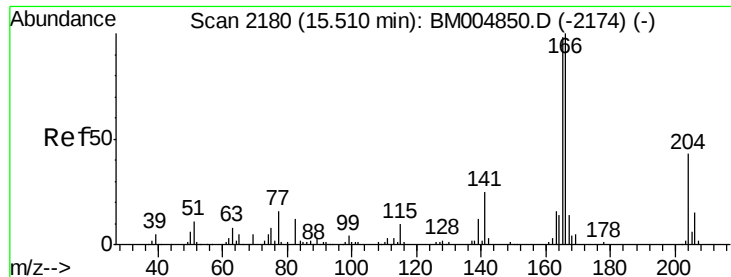

#59

Fluorene

Concen: 0.05 ng/ul

RT: 15.46 min Scan# 2171

Delta R.T. -0.05 min

Lab File: BM004851.D

Acq: 01 Apr 2016 21:49

Instrument :

BNA_M

ClientSampleId :

SBLK44


Tot Ion:166 Resp: 454

Ion Ratio Lower Upper

166 100

165 0.0 78.5 117.7#

167 0.0 10.7 16.1#



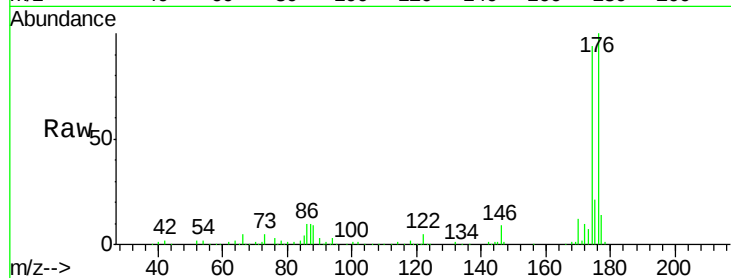


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.46

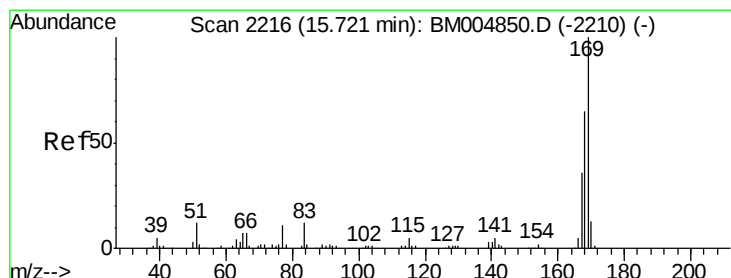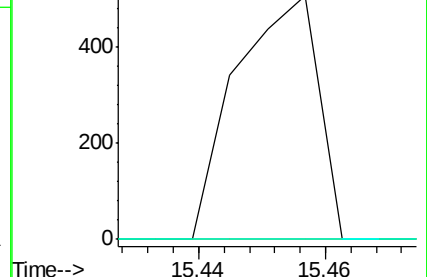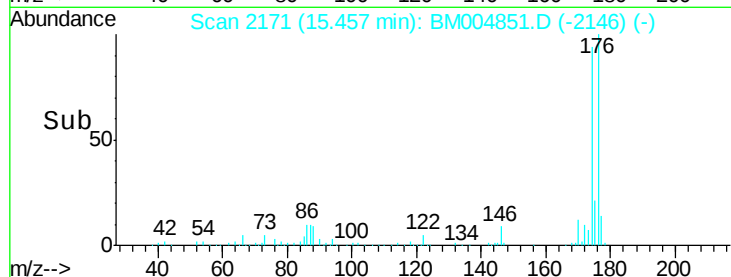

#65

N-Nitrosodiphenylamine

Concen: 0.04 ng/ul

RT: 15.57 min Scan# 2191

Delta R.T. -0.15 min

Lab File: BM004851.D

Acq: 01 Apr 2016 21:49


Tgt Ion:169 Resp: 273

Ion Ratio Lower Upper

169 100

168 0.0 53.8 80.8#

167 95.8 29.3 43.9#


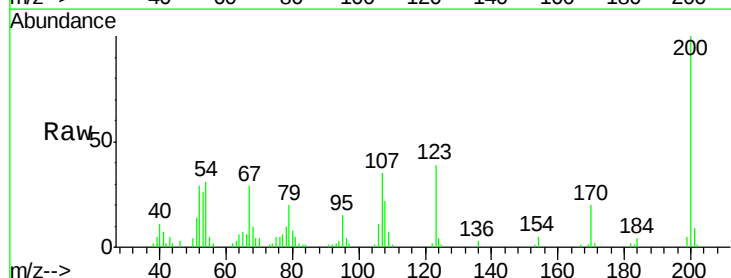



Abundance Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E

Ion 167.00 (166.70 to 167.70): E

15.57

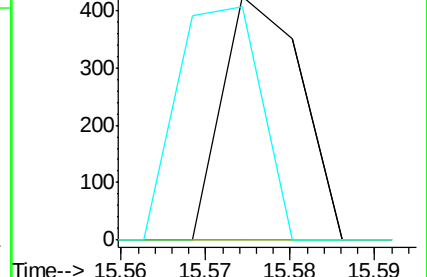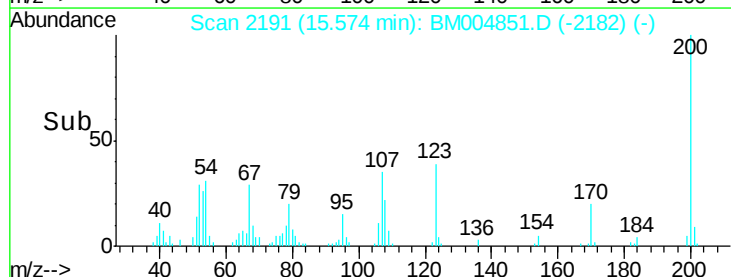

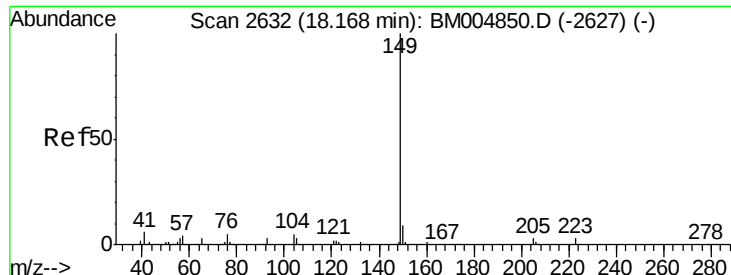

#76

Di-n-butylphthalate

Concen: 0.02 ng/ul

RT: 18.17 min Scan# 2632

Delta R.T. -0.00 min

Lab File: BM004851.D

Acq: 01 Apr 2016 21:49

Instrument :

BNA_M

ClientSampleId :

SBLK44


Tot Ion:149 Resp: 300

Ion Ratio Lower Upper

149 100

150 0.0 7.4 11.0#




104 0.0 4.0 6.0#

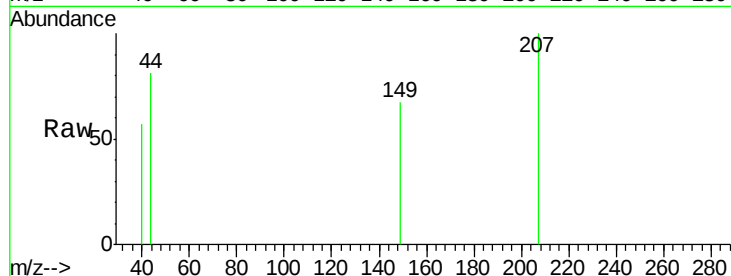

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

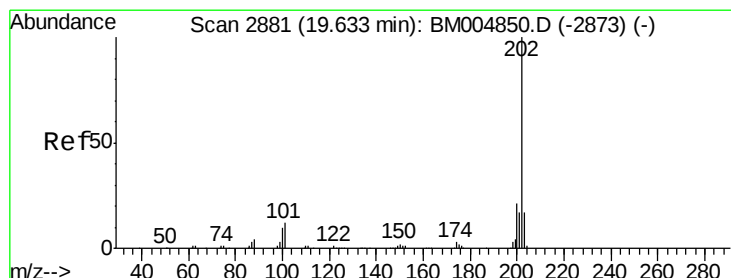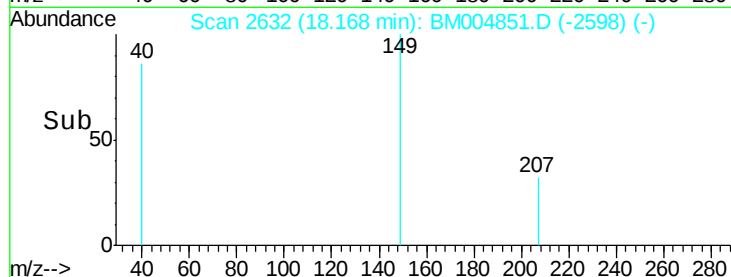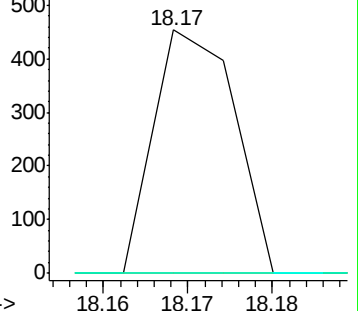

#80

Pyrene

Concen: 0.03 ng/ul

RT: 19.60 min Scan# 2876

Delta R.T. -0.03 min

Lab File: BM004851.D

Acq: 01 Apr 2016 21:49


Tgt Ion:202 Resp: 613

Ion Ratio Lower Upper

202 100

101 161.1 10.2 15.2#



100 974.5 8.5 12.7#

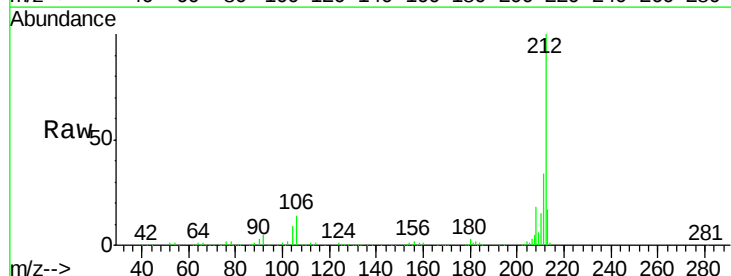


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

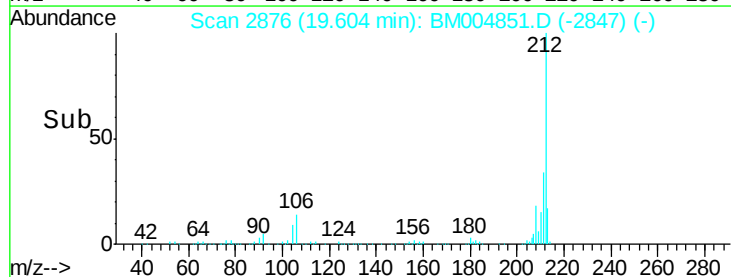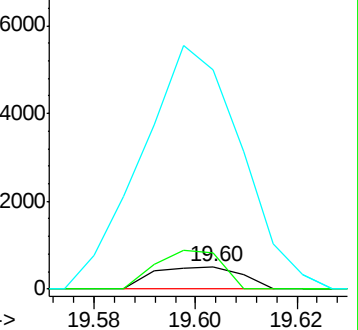

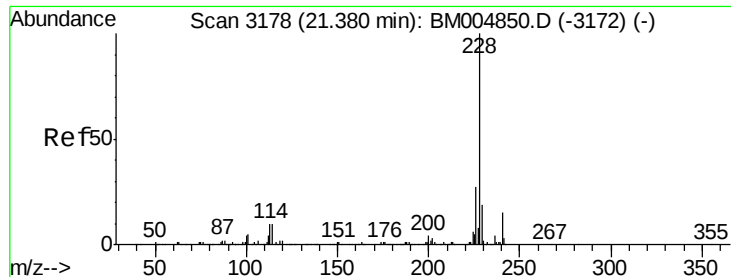

#83

Benzo(a)anthracene

Concen: 0.03 ng/ul

RT: 21.40 min Scan# 3181

Delta R.T. 0.02 min

Lab File: BM004851.D

Acq: 01 Apr 2016 21:49

Instrument :

BNA_M

ClientSampleId :

SBLK44


Tot Ion:228 Resp: 605

Ion Ratio Lower Upper

228 100

229 0.0 15.7 23.5#




226 0.0 21.8 32.6#

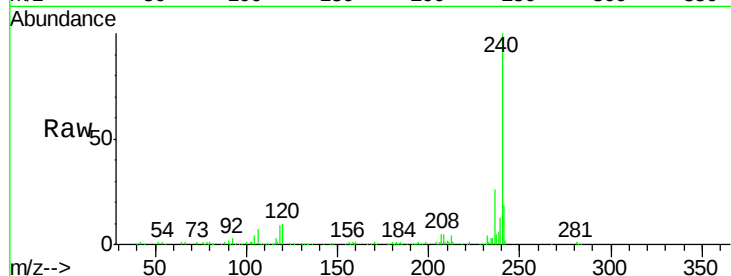

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

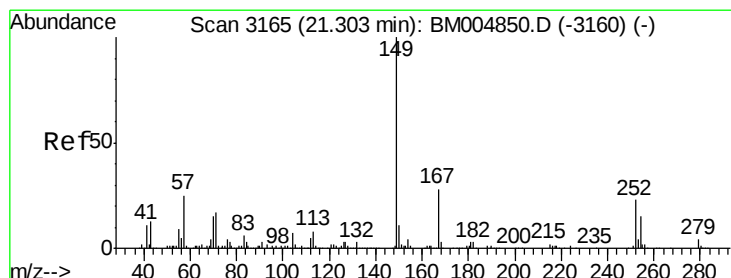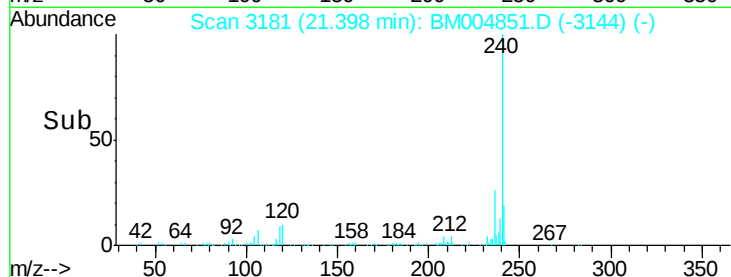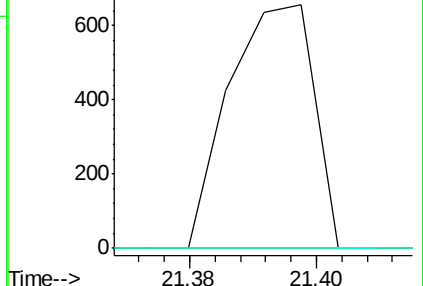

#84

Bis(2-ethylhexyl)phthalate

Concen: 0.04 ng/ul

RT: 21.30 min Scan# 3165

Delta R.T. -0.00 min

Lab File: BM004851.D

Acq: 01 Apr 2016 21:49


Tgt Ion:149 Resp: 470

Ion Ratio Lower Upper

149 100

167 0.0 21.6 32.4#



279 0.0 3.0 4.4#

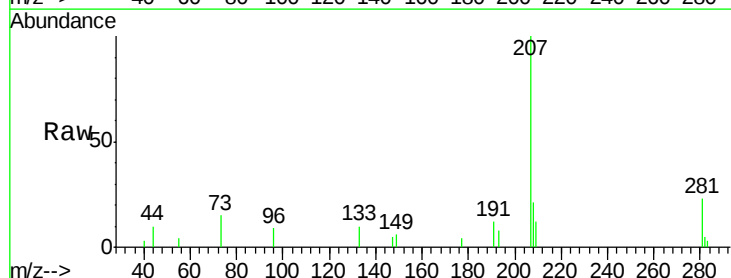


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E



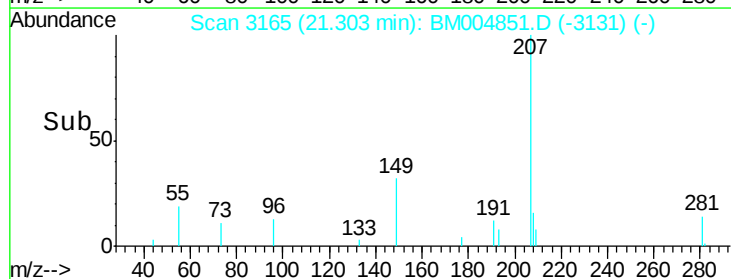
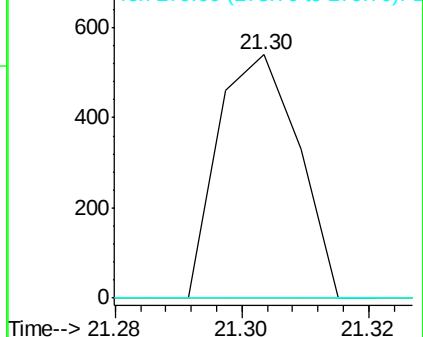


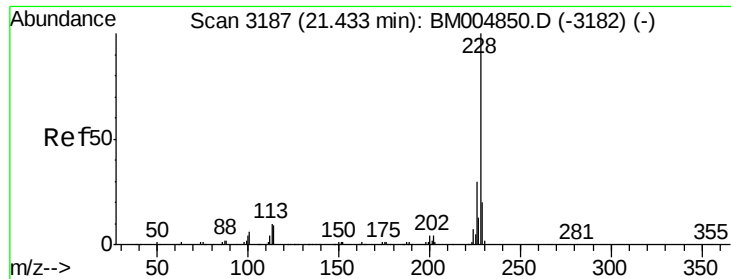

#85
 Chrysene
 Concen: 0.03 ng/ul
 RT: 21.40 min Scan# 3181
 Delta R.T. -0.04 min
 Lab File: BM004851.D
 Acq: 01 Apr 2016 21:49




Instrument :
 BNA_M
 ClientSampleId :
 SBLK44


Tot Ion:228 Resp: 605
 Ion Ratio Lower Upper
 228 100
 226 0.0 24.0 36.0#
 229 0.0 15.6 23.4#

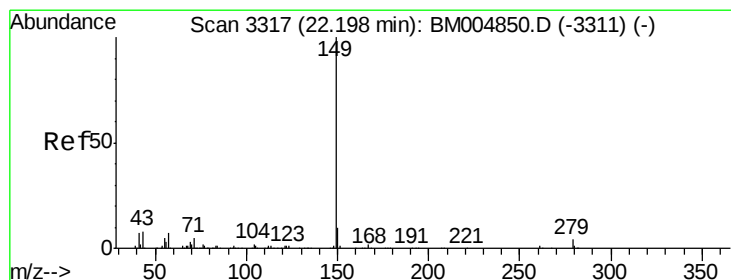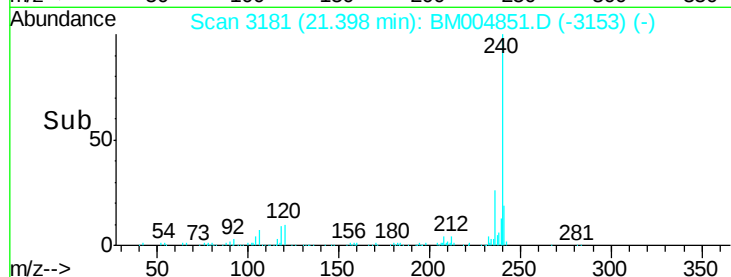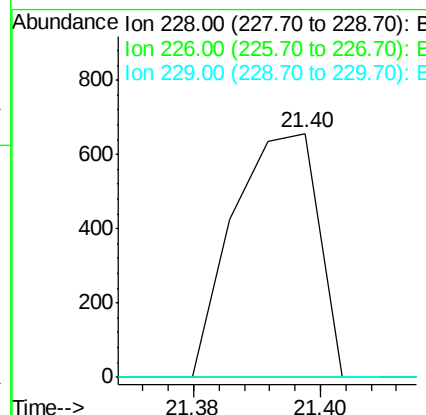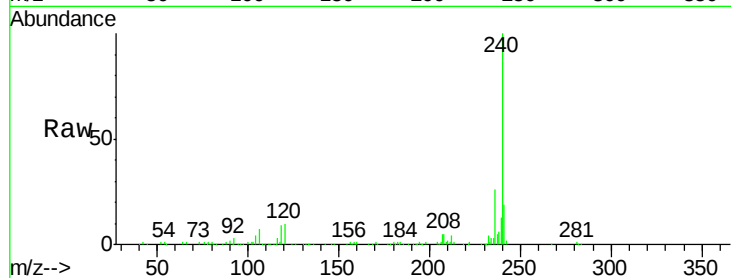

#87
 Di-n-octyl phthalate
 Concen: 0.01 ng/ul
 RT: 22.17 min Scan# 3313
 Delta R.T. -0.02 min
 Lab File: BM004851.D
 Acq: 01 Apr 2016 21:49

Tgt Ion:149 Resp: 113
 Ion Ratio Lower Upper
 149 100
 167 0.0 1.2 1.8#
 43 104.4 5.6 8.4#

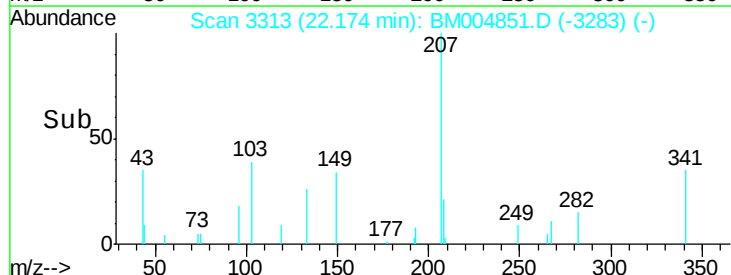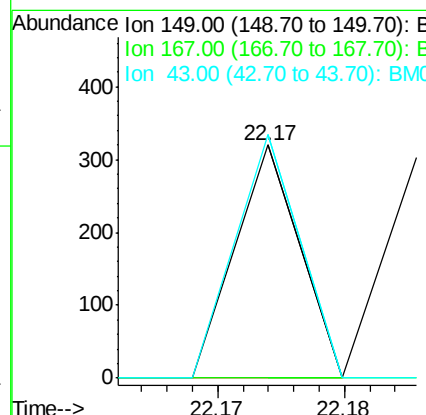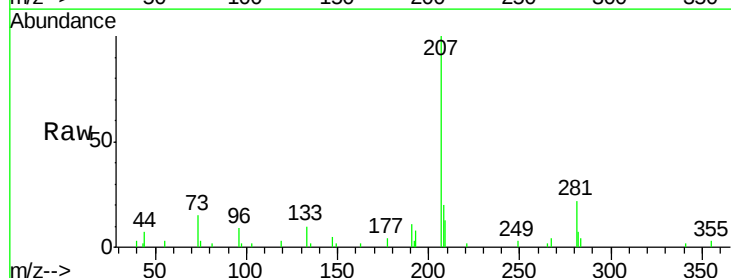

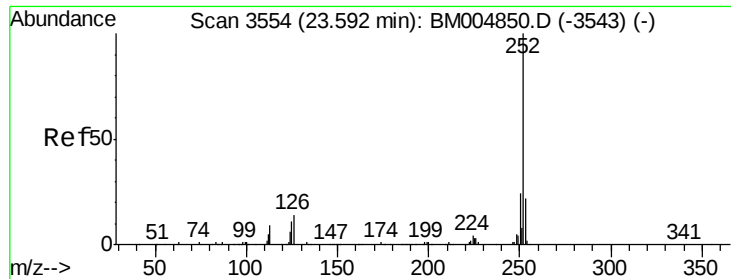

#91

Benzo(a)pyrene

Concen: 0.11 ng/ul

RT: 23.54 min Scan# 3546

Delta R.T. -0.05 min

Lab File: BM004851.D

Acq: 01 Apr 2016 21:49

Instrument :

BNA_M

ClientSampleId :

SBLK44

Tot Ion: 252 Resp: 2067

Ion Ratio Lower Upper

252 100

253 39.9 17.2 25.8#

125 27.5 9.0 13.6#

