

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040116\  
 Data File : BM004865.D  
 Acq On : 02 Apr 2016 06:54  
 Operator : UM/SJ  
 Sample : H2004-14  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0AE9

Quant Time: Apr 04 00:38:46 2016  
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM040116.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Mon Apr 04 00:33:02 2016  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.82  | 152  | 52300    | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.62 | 136  | 241498   | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.46 | 164  | 151989   | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 17.20 | 188  | 367387   | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.39 | 240  | 444889   | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 23.68 | 264  | 460054   | 20.00 | ng/ul | 0.00     |

| System Monitoring Compounds    | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 3) 1,4-Dioxane-d8              | 3.32  | 96   | 1354     | 1.05  | ng/uL | 0.00     |
| 5) Phenol-d5                   | 6.99  | 99   | 25639    | 5.52  | ng/ul | 0.00     |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.15  | 67   | 87567    | 34.77 | ng/ul | 0.00     |
| 9) 2-Chlorophenol-d4           | 7.35  | 132  | 90936    | 25.78 | ng/ul | 0.00     |
| 13) 4-Methylphenol-d8          | 8.52  | 113  | 55671    | 14.26 | ng/ul | 0.00     |
| 19) Nitrobenzene-d5            | 8.98  | 128  | 61003    | 35.60 | ng/ul | 0.00     |
| 22) 2-Nitrophenol-d4           | 9.70  | 143  | 68662    | 36.04 | ng/ul | 0.00     |
| 26) 2,4-Dichlorophenol-d3      | 10.23 | 165  | 109146   | 30.73 | ng/ul | 0.00     |
| 29) 4-Chloroaniline-d4         | 0.00  | 131  | 0        | 0.00  | ng/ul | 0.00     |
| 44) Dimethylphthalate-d6       | 13.87 | 166  | 451607   | 37.66 | ng/ul | 0.00     |
| 47) Acenaphthylene-d8          | 14.15 | 160  | 528034   | 36.81 | ng/ul | 0.00     |
| 52) 4-Nitrophenol-d4           | 14.65 | 143  | 10094    | 4.26  | ng/ul | 0.00     |
| 58) Fluorene-d10               | 15.45 | 176  | 394594   | 38.07 | ng/ul | 0.00     |
| 63) 4,6-Dinitro-2-methylphenol | 15.57 | 200  | 70528    | 32.04 | ng/ul | 0.00     |
| 71) Anthracene-d10             | 17.30 | 188  | 632519   | 38.48 | ng/ul | 0.00     |
| 79) Pyrene-d10                 | 19.60 | 212  | 728178   | 37.70 | ng/ul | 0.00     |
| 90) Benzo(a)pyrene-d12         | 23.54 | 264  | 855150   | 41.96 | ng/ul | 0.00     |


| Target Compounds               | R.T.  | QIon | Response | Conc | Units | Ovalue |
|--------------------------------|-------|------|----------|------|-------|--------|
| 73) 1,2,3,4-Tetrachlorobenzene | 13.26 | 216  | 11301    | 2.37 | ng/uL | 96     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040116\  
Data File : BM004865.D  
Acq On : 02 Apr 2016 06:54  
Operator : UM/SJ  
Sample : H2004-14  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
C0AE9

Quant Time: Apr 04 00:38:46 2016  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM040116.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Apr 04 00:33:02 2016  
Response via : Initial Calibration

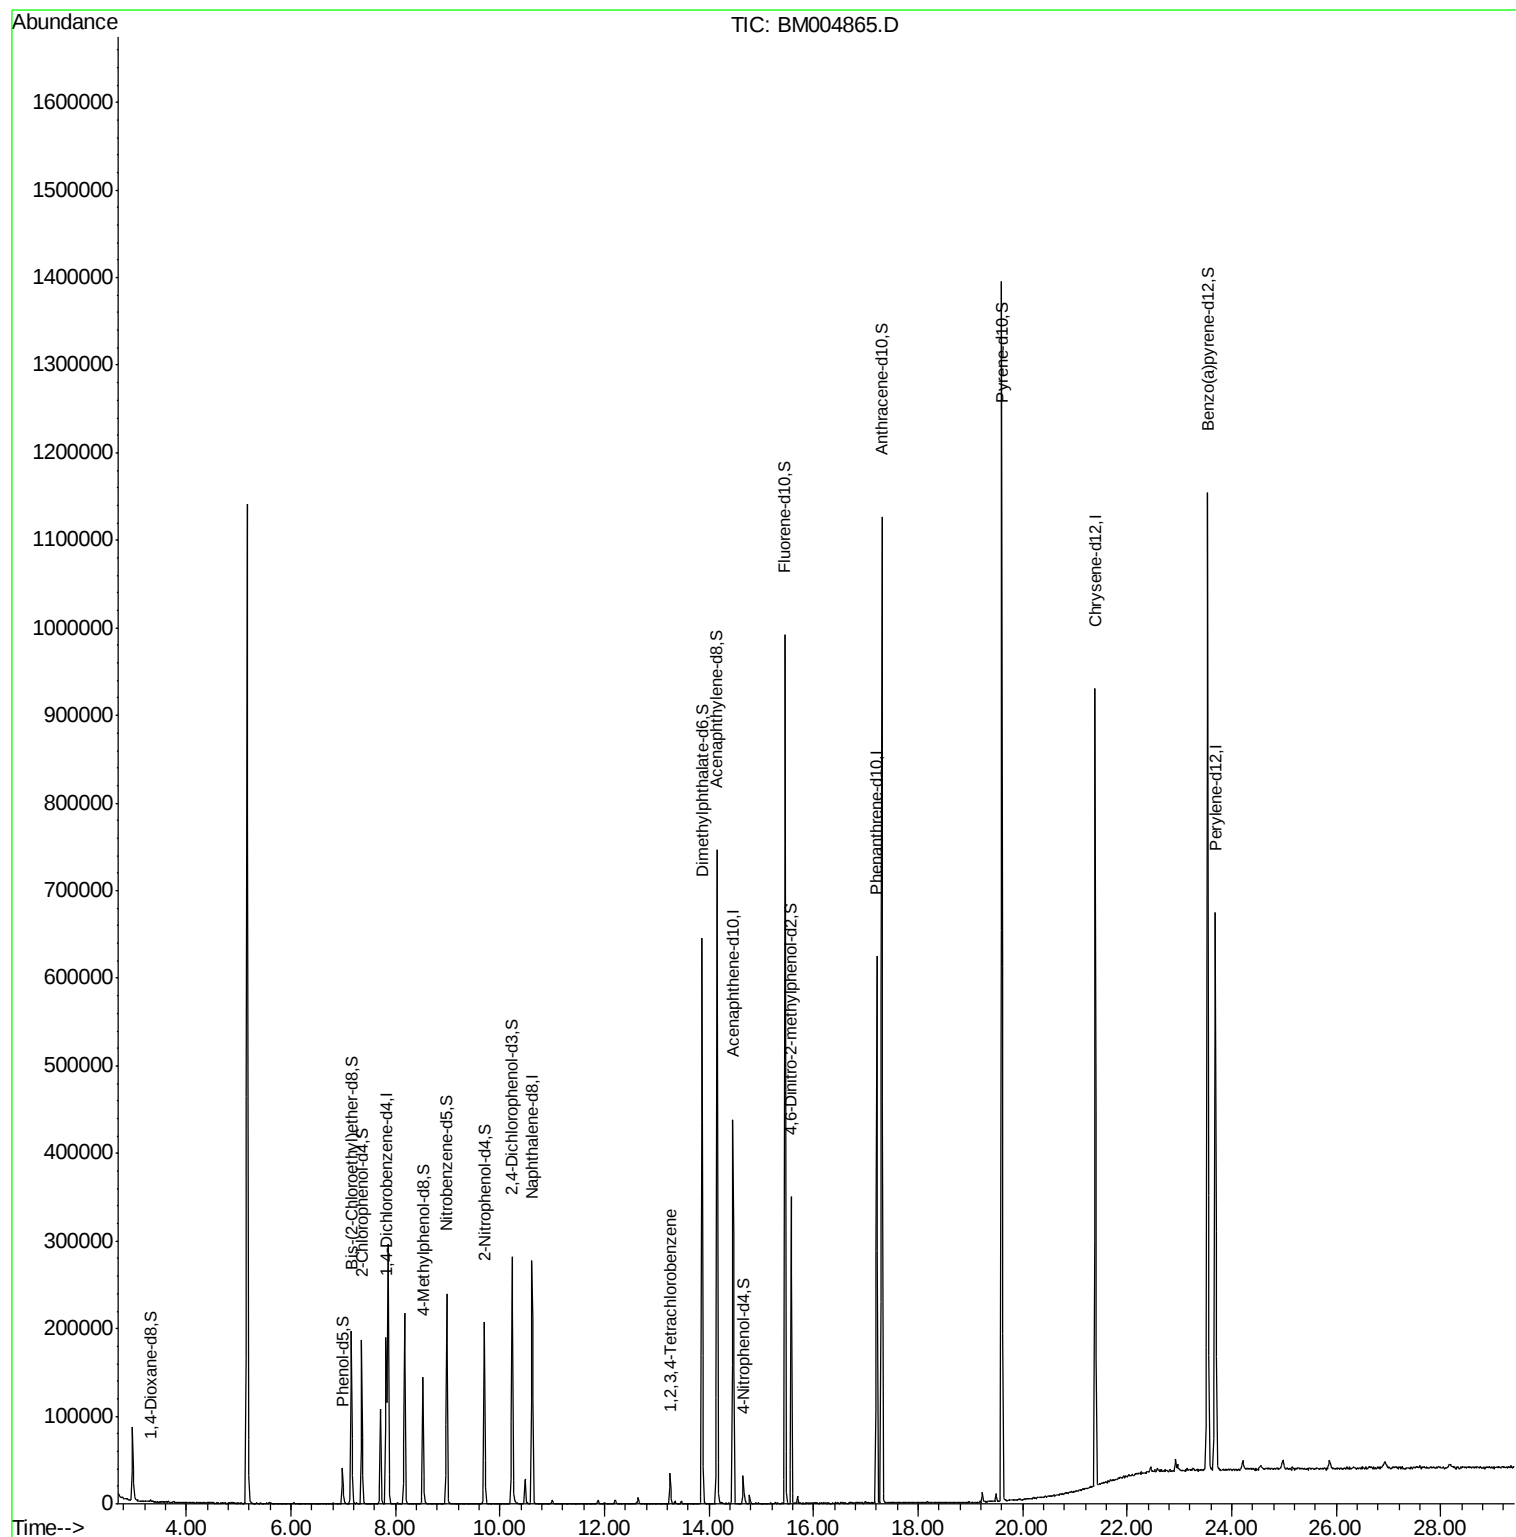

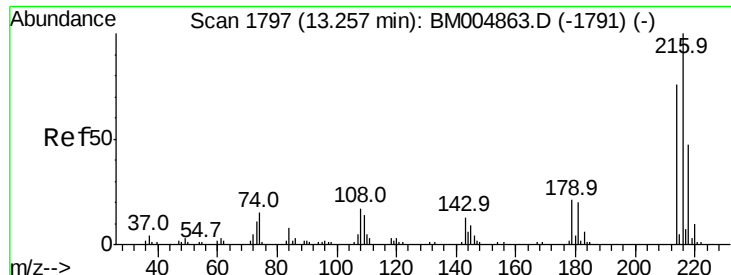

#73

1,2,3,4-Tetrachlorobenzene

Concen: 2.37 ng/uL

RT: 13.26 min Scan# 1797

Delta R.T. -0.00 min

Lab File: BM004865.D


Acq: 02 Apr 2016 06:54

Instrument :

BNA\_M

ClientSampleId :

C0AE9

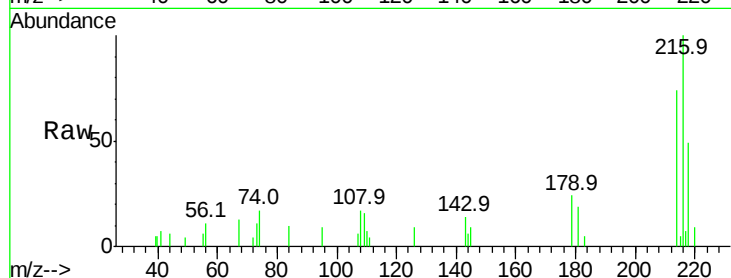


Tot Ion: 216 Resp: 11301

Ion Ratio Lower Upper

216 100

214 73.5 62.5 93.7

218 49.0 38.4 57.6

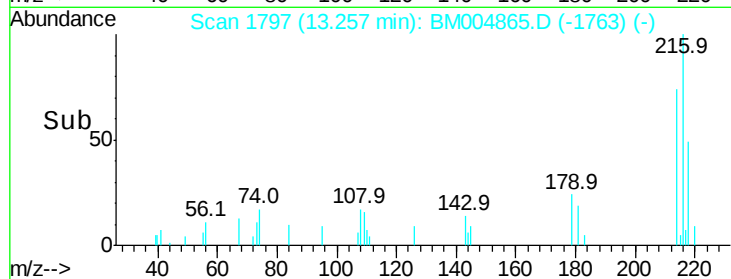

Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

