

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040116\
 Data File : BM004874.D
 Acq On : 02 Apr 2016 12:19
 Operator : UM/SJ
 Sample : H2004-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF0

Quant Time: Apr 04 01:01:38 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM040116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 04 01:00:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	59239	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	280638	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.46	164	169668	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.20	188	399984	20.00	ng/ul	0.00
78) Chrysene-d12	21.39	240	486454	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	485349	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	1325	0.90	ng/uL	0.00
5) Phenol-d5	6.99	99	30993	5.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	74813	26.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	84601	21.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	62814	14.21	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	52364	26.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	58758	26.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	103892	25.17	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	782	0.16	ng/ul	0.01
44) Dimethylphthalate-d6	13.86	166	378910	28.31	ng/ul	0.00
47) Acenaphthylene-d8	14.15	160	446905	27.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.65	143	13692	5.17	ng/ul	0.00
58) Fluorene-d10	15.45	176	334046	28.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.57	200	58388	24.36	ng/ul	0.00
71) Anthracene-d10	17.30	188	542249	30.30	ng/ul	0.00
79) Pyrene-d10	19.60	212	633076	29.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	720733	33.52	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.91	163	48518	3.56	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040116\
Data File : BM004874.D
Acq On : 02 Apr 2016 12:19
Operator : UM/SJ
Sample : H2004-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF0

Quant Time: Apr 04 01:01:38 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 04 01:00:14 2016
Response via : Initial Calibration

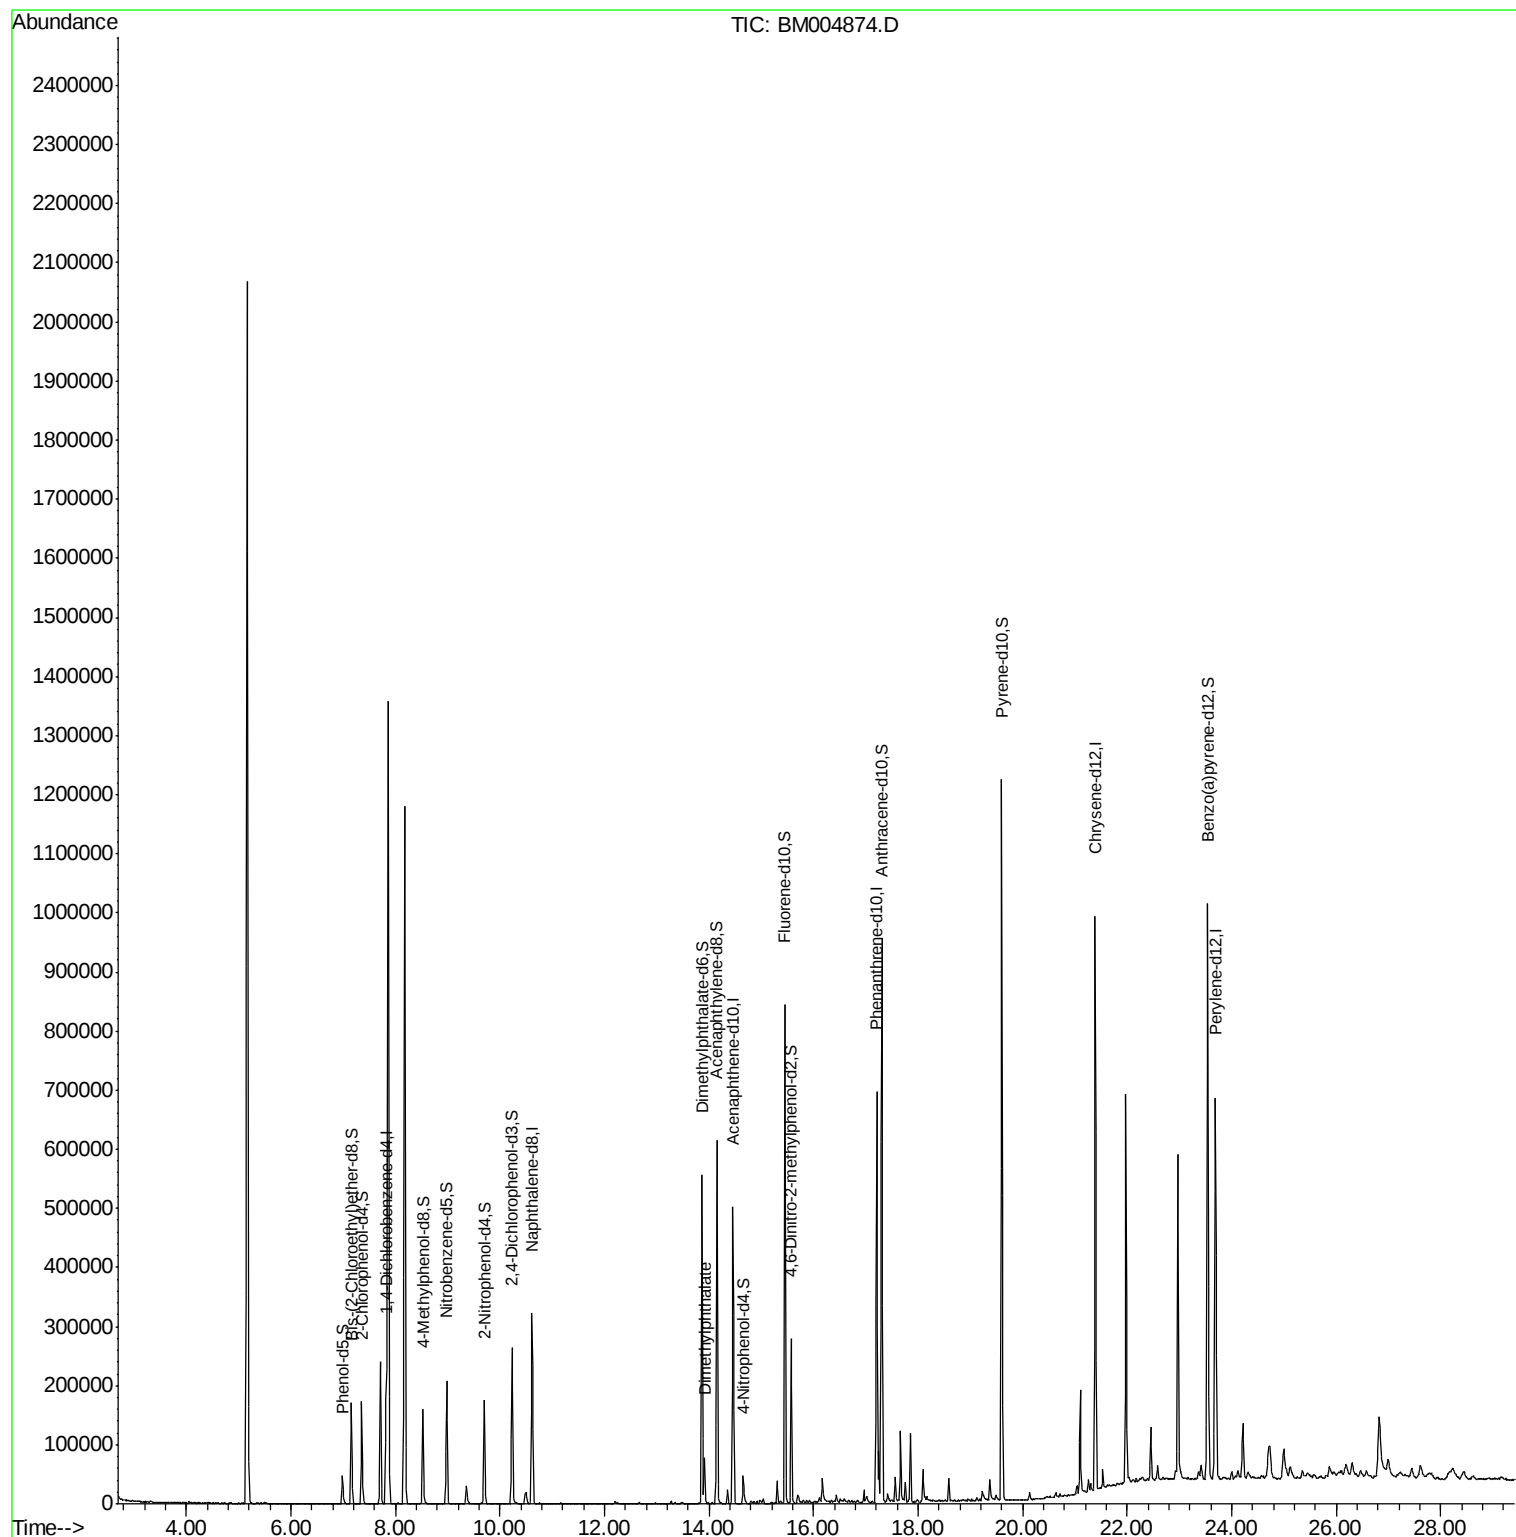

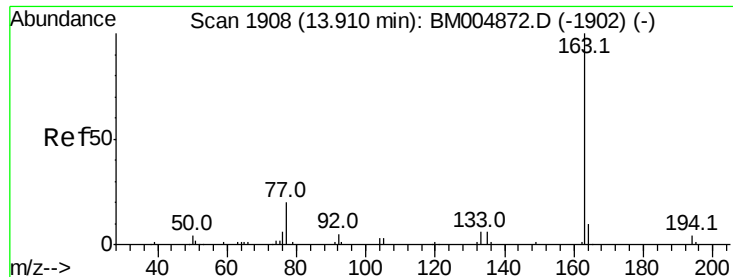

#45

Dimethylphthalate

Concen: 3.56 ng/ul

RT: 13.91 min Scan# 1908

Delta R.T. -0.00 min

Lab File: BM004874.D

Acq: 02 Apr 2016 12:19

Instrument :

BNA_M

ClientSampleId :

C0AF0


Tot Ion:163 Resp: 48518

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 9.6 7.8 11.8

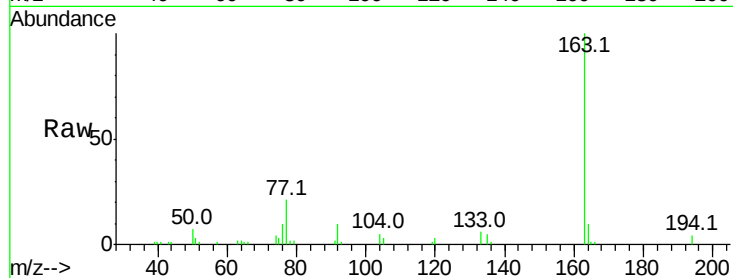

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

